

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
 Data File : BF127877.D
 Acq On : 25 Apr 2022 13:36
 Operator : CG\JU
 Sample : N2548-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127877.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.081	301	305	310	rVB	41601	50658	1.19%	0.179%
2	5.187	489	493	501	rVB	36194	45278	1.07%	0.160%
3	5.563	552	557	560	rBV	3443581	3514855	82.77%	12.399%
4	6.563	721	727	730	rBV	3443308	3591772	84.58%	12.670%
5	6.939	787	791	794	rBV	1254768	986705	23.24%	3.481%
6	7.504	882	887	890	rBV	2535959	2434996	57.34%	8.590%
7	8.222	1005	1009	1012	rBV	1517906	1284180	30.24%	4.530%
8	9.298	1187	1192	1195	rBV	4640459	4246611	100.00%	14.980%
9	9.980	1303	1308	1312	rBV	1792309	1497269	35.26%	5.282%
10	10.286	1353	1360	1366	rBV	37034	71583	1.69%	0.253%
11	10.774	1438	1443	1446	rBV	2597275	2581648	60.79%	9.107%
12	11.474	1558	1562	1565	rBV	1812365	1546719	36.42%	5.456%
13	11.986	1646	1649	1653	rBV	45816	48197	1.13%	0.170%
14	13.063	1827	1832	1835	rBV	4400148	4139703	97.48%	14.603%
15	14.080	1995	2005	2007	rBV5	65483	182656	4.30%	0.644%
16	14.115	2007	2011	2015	rVB	1142340	1074068	25.29%	3.789%
17	14.215	2024	2028	2034	rVB	89839	104280	2.46%	0.368%
18	15.627	2263	2268	2279	rBV	690620	946930	22.30%	3.340%




Sum of corrected areas: 28348108

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
Data File : BF127877.D
Acq On : 25 Apr 2022 13:36
Operator : CG\JU
Sample : N2548-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

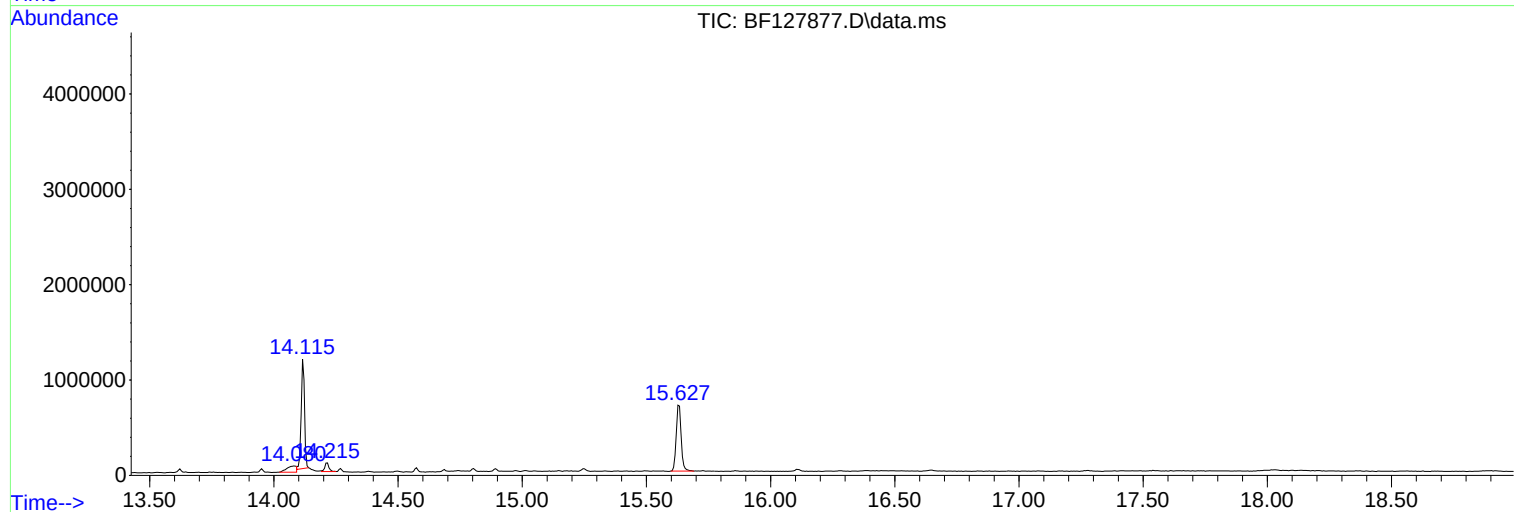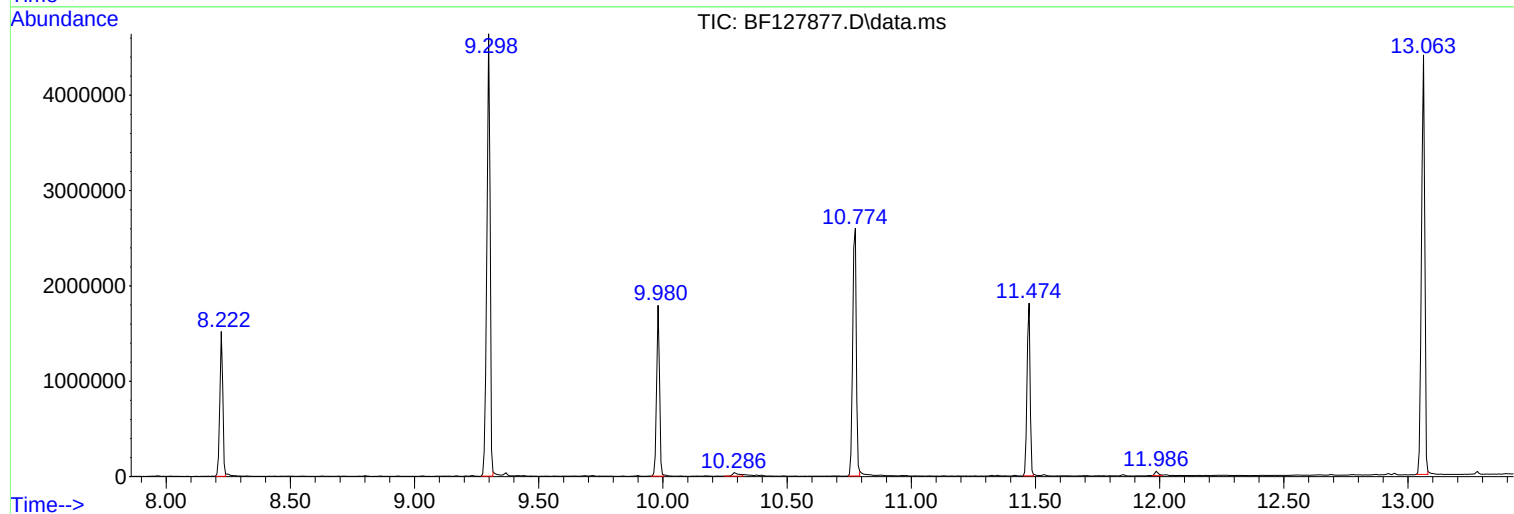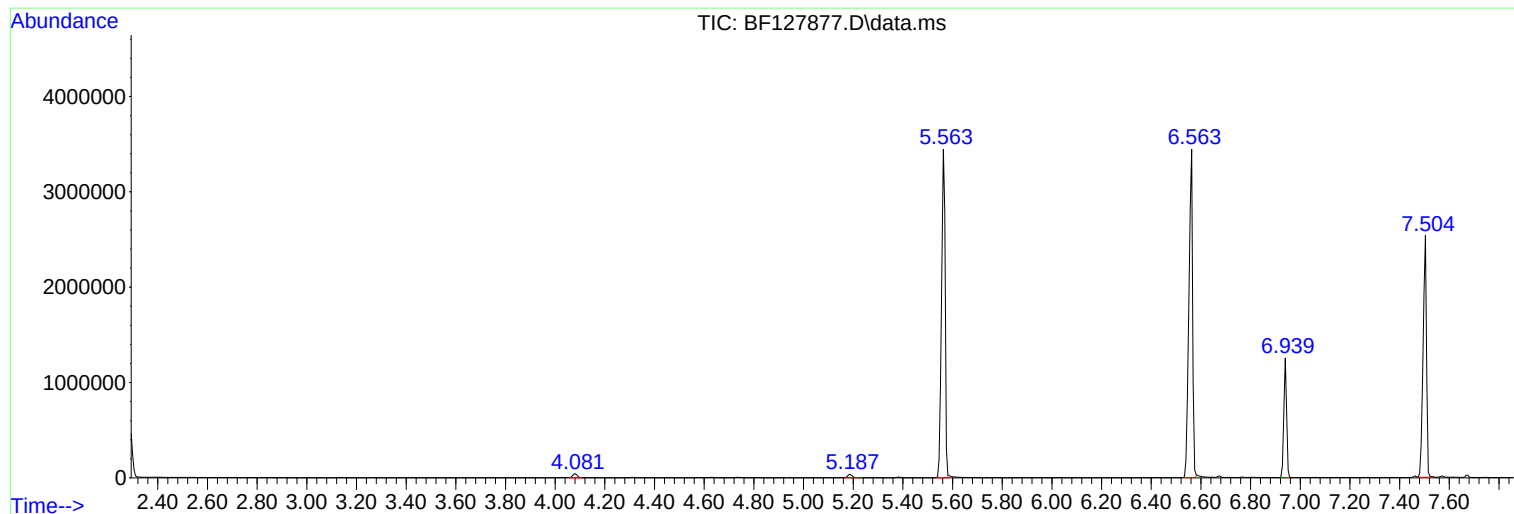

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
Data File : BF127877.D
Acq On : 25 Apr 2022 13:36
Operator : CG\JU
Sample : N2548-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
Data File : BF127877.D
Acq On : 25 Apr 2022 13:36
Operator : CG\JU
Sample : N2548-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------