

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
 Data File : BF127883.D
 Acq On : 25 Apr 2022 16:32
 Operator : CG\JU
 Sample : N2550-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PUMP-STATION-207ST-TRAIN-FACILITY

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127883.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.557	551	556	559	rBV	1376109	1301198	23.48%	4.765%
2	6.551	721	725	738	rVB	957917	804052	14.51%	2.945%
3	6.940	787	791	794	rBV	1281852	1014939	18.32%	3.717%
4	7.504	881	887	890	rBV	3062677	3298283	59.52%	12.079%
5	8.222	1005	1009	1013	rBV	1572822	1331983	24.04%	4.878%
6	9.298	1187	1192	1195	rBV	5423515	5541164	100.00%	20.294%
7	9.981	1303	1308	1311	rBV	1883892	1564291	28.23%	5.729%
8	10.769	1438	1442	1458	rBV	2584166	2638780	47.62%	9.664%
9	11.475	1557	1562	1565	rBV	1741013	1657938	29.92%	6.072%
10	13.063	1827	1832	1835	rBV	5214007	5430225	98.00%	19.887%
11	14.116	2007	2011	2015	rBV	1305158	1202079	21.69%	4.402%
12	14.198	2021	2025	2033	rVB	338395	541198	9.77%	1.982%
13	15.627	2263	2268	2277	rBV2	745776	978887	17.67%	3.585%




Sum of corrected areas: 27305017

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
Data File : BF127883.D
Acq On : 25 Apr 2022 16:32
Operator : CG\JU
Sample : N2550-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PUMP-STATION-207ST-TRAIN-FACILITY

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

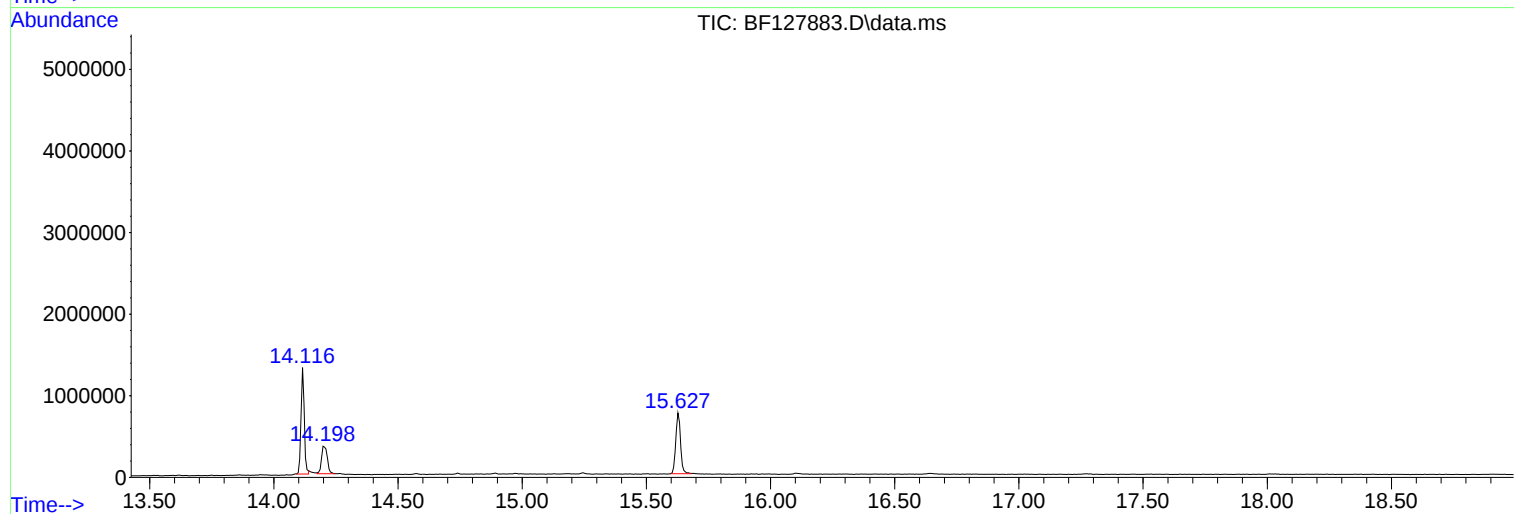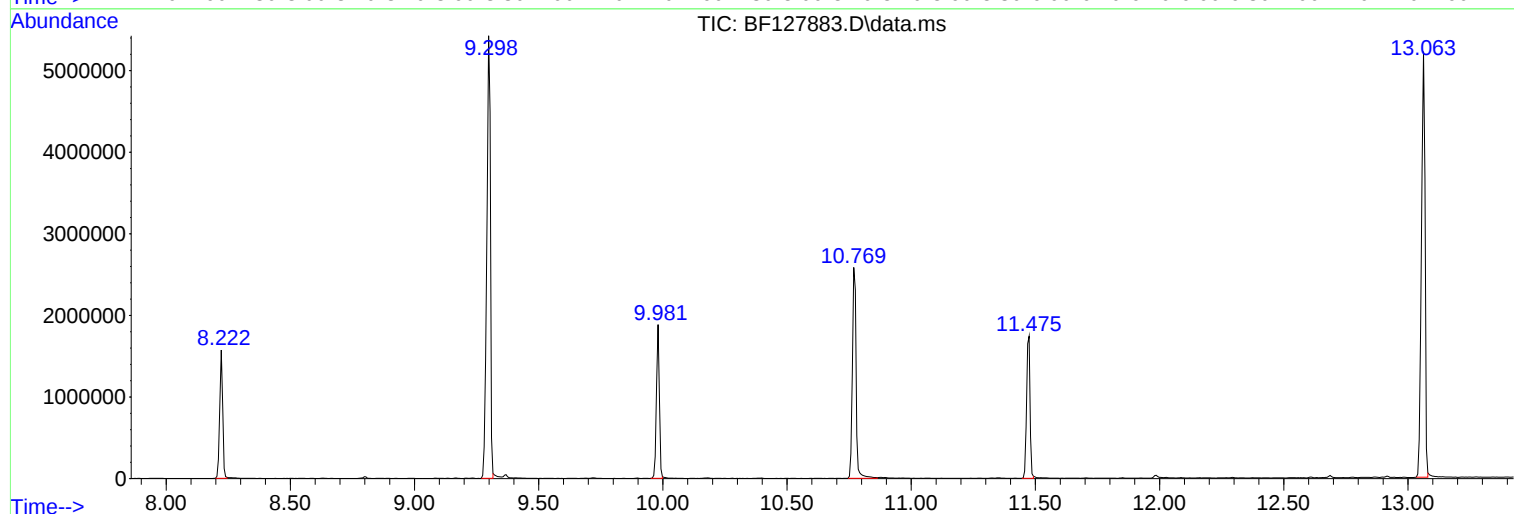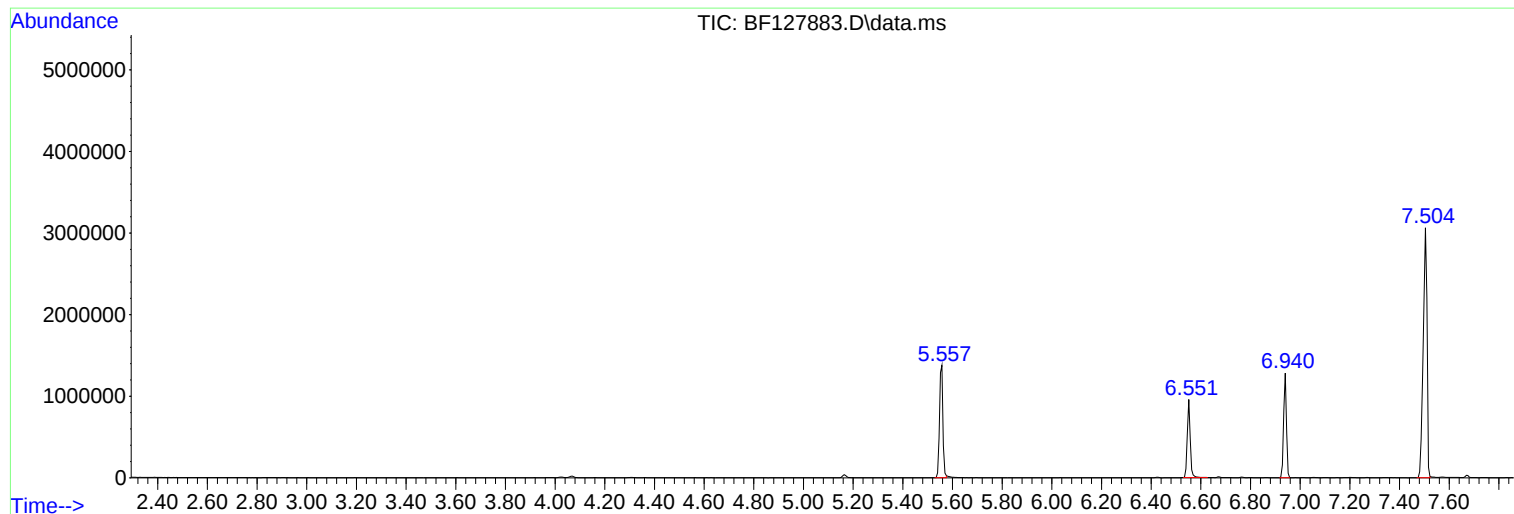

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
Data File : BF127883.D
Acq On : 25 Apr 2022 16:32
Operator : CG\JU
Sample : N2550-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PUMP-STATION-207ST-TRAIN-FACILITY










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.198	9.00 ng	541198	Chrysene-d12	14.116

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	96
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	50
4			1H-Indole-3-acetic acid, 5-[(tri...]	277	C14H19NO3Si	072101-35-0	23
5			Oxoprophines	277	C17H11NO3	1000128-51-1	9

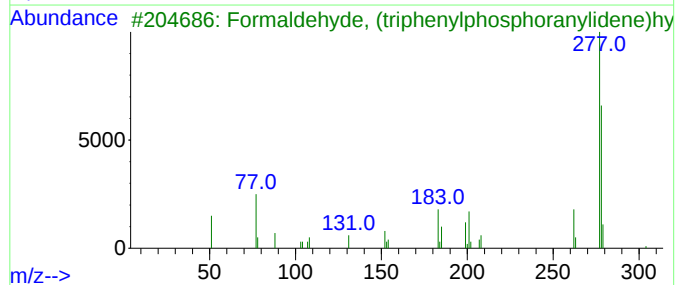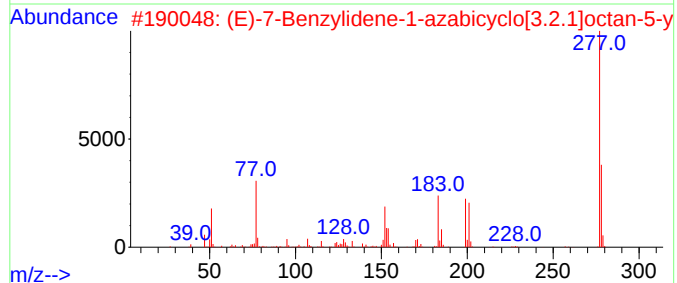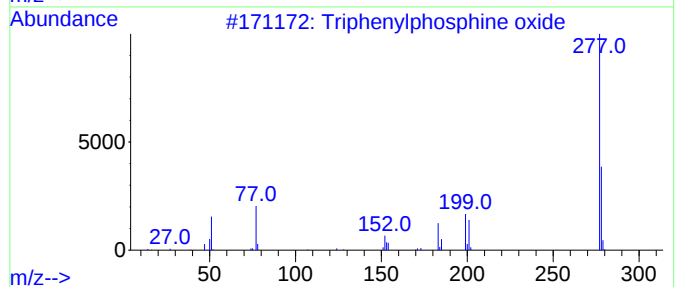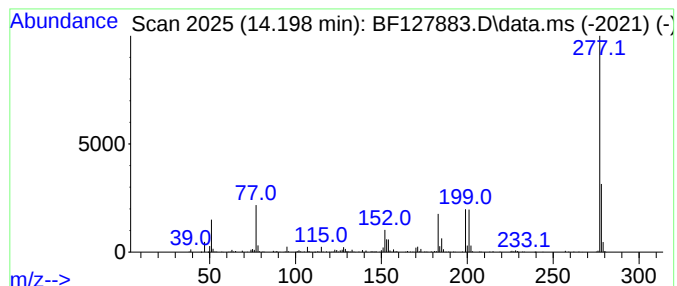

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
Data File : BF127883.D
Acq On : 25 Apr 2022 16:32
Operator : CG\JU
Sample : N2550-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PUMP-STATION-207ST-TRAIN-FACILITY

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.198	9.0	ng	541198	5	14.116	1202080	20.0