

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
 Data File : BF127894.D
 Acq On : 25 Apr 2022 21:46
 Operator : CG\JU
 Sample : N2548-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MH-8D

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127894.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.187	485	493	499	rBV	29970	44689	1.04%	0.154%
2	5.563	552	557	560	rBV	3561943	3605834	84.08%	12.408%
3	6.563	721	727	730	rBV	3471326	3722857	86.80%	12.811%
4	6.939	787	791	794	rBV	1278897	997297	23.25%	3.432%
5	7.504	882	887	890	rBV	2659169	2532836	59.06%	8.716%
6	8.222	1005	1009	1012	rBV	1542134	1293436	30.16%	4.451%
7	8.933	1126	1130	1134	rBV	230916	184659	4.31%	0.635%
8	9.033	1142	1147	1150	rBV	109661	95665	2.23%	0.329%
9	9.298	1187	1192	1195	rBV	4631242	4288800	100.00%	14.759%
10	9.369	1201	1204	1207	rVB	52485	50167	1.17%	0.173%
11	9.557	1233	1236	1240	rBV2	35348	48681	1.14%	0.168%
12	9.686	1255	1258	1261	rVB2	52093	47347	1.10%	0.163%
13	9.980	1299	1308	1311	rBV	1799781	1538302	35.87%	5.294%
14	10.010	1311	1313	1317	rVB	70594	62980	1.47%	0.217%
15	10.398	1372	1379	1382	rBV3	37746	55372	1.29%	0.191%
16	10.616	1411	1416	1423	rVB2	53410	74554	1.74%	0.257%
17	10.769	1438	1442	1446	rBV	2657986	2672246	62.31%	9.196%
18	10.886	1457	1462	1469	rVB	93692	123791	2.89%	0.426%
19	11.351	1538	1541	1548	rVB2	60150	73827	1.72%	0.254%
20	11.474	1558	1562	1565	rBV	1600219	1526405	35.59%	5.253%
21	11.986	1645	1649	1654	rBV2	39904	59954	1.40%	0.206%
22	12.686	1765	1768	1772	rBV	54241	50841	1.19%	0.175%
23	12.915	1802	1807	1810	rBV2	60154	67475	1.57%	0.232%
24	13.063	1827	1832	1835	rBV	3818153	3682288	85.86%	12.672%
25	14.115	2007	2011	2021	rVB	1044840	1020890	23.80%	3.513%
26	14.210	2023	2027	2032	rBV	146322	153596	3.58%	0.529%
27	15.562	2253	2257	2263	rBV2	26125	49304	1.15%	0.170%
28	15.627	2263	2268	2275	rBV2	690058	935458	21.81%	3.219%




Sum of corrected areas: 29059551

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
Data File : BF127894.D
Acq On : 25 Apr 2022 21:46
Operator : CG\JU
Sample : N2548-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-8D

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

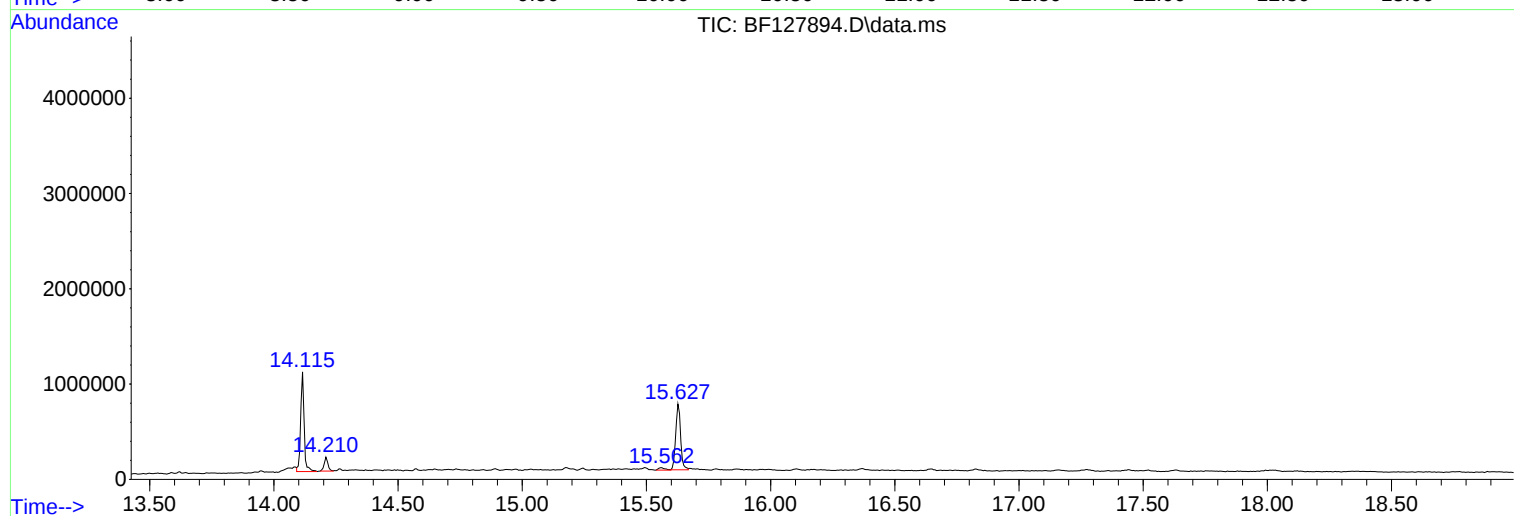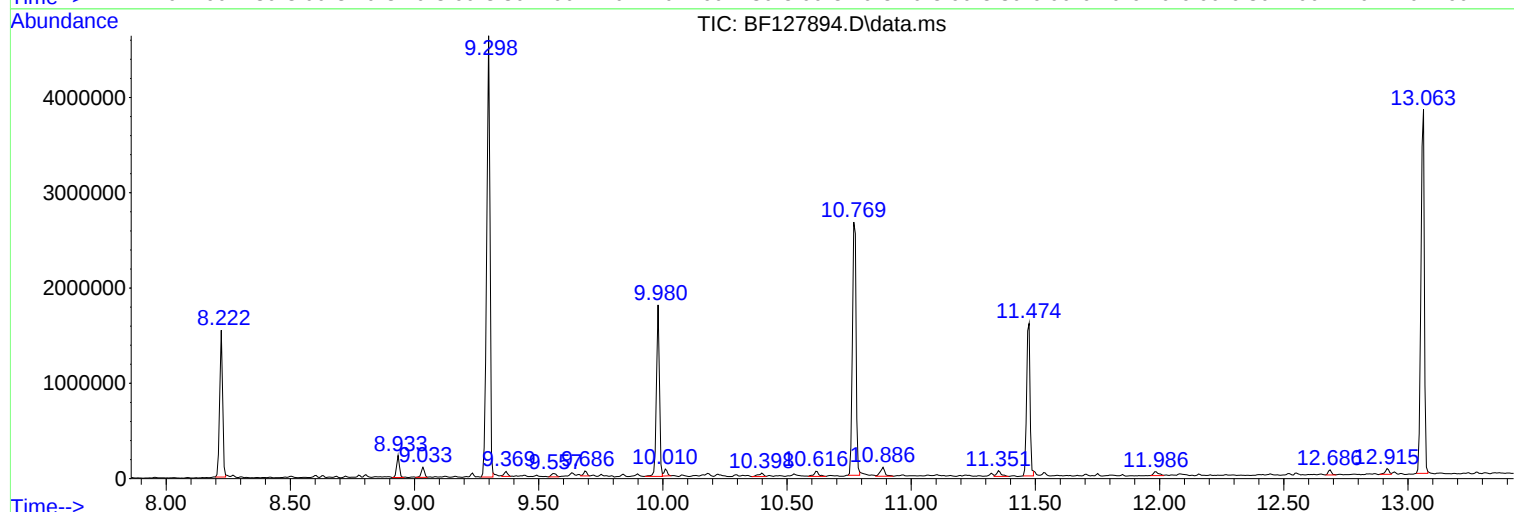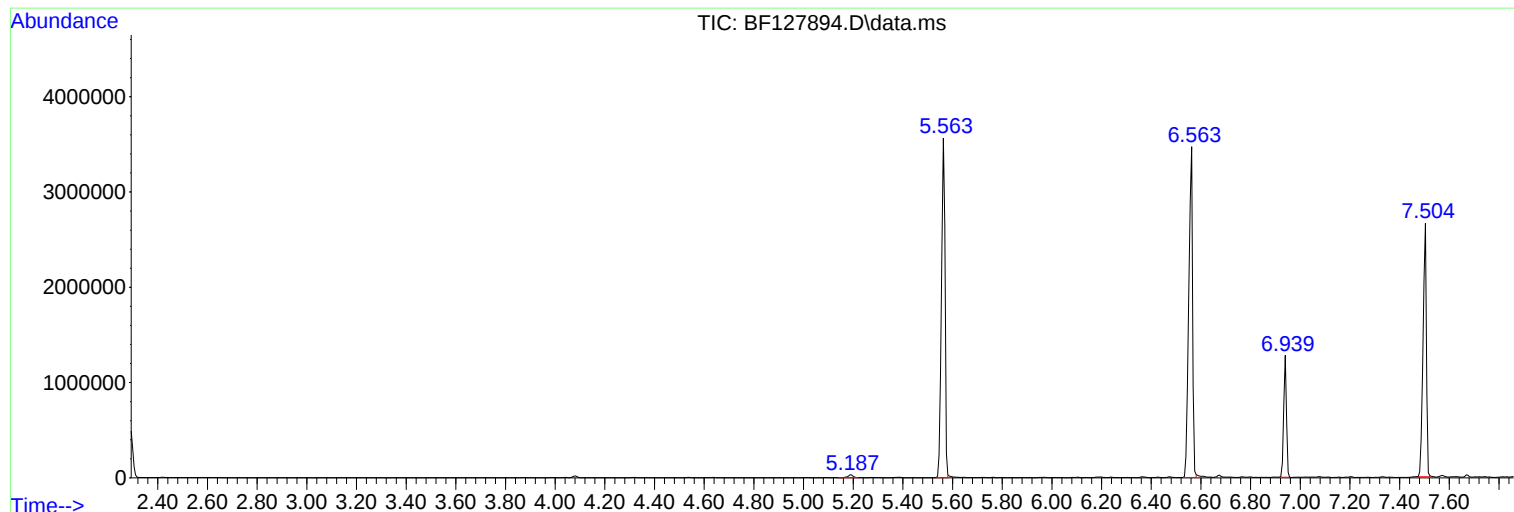

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
Data File : BF127894.D
Acq On : 25 Apr 2022 21:46
Operator : CG\JU
Sample : N2548-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-8D










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.210	3.01 ng	153596	Chrysene-d12	14.115

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	95
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	90
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	50
4			3-(3,4-Dichlorophenyl)-2-thioxo-...	277	C9H5Cl2NOS2	017046-34-3	25
5			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	23

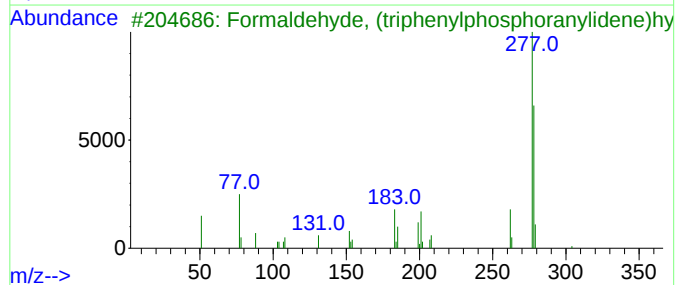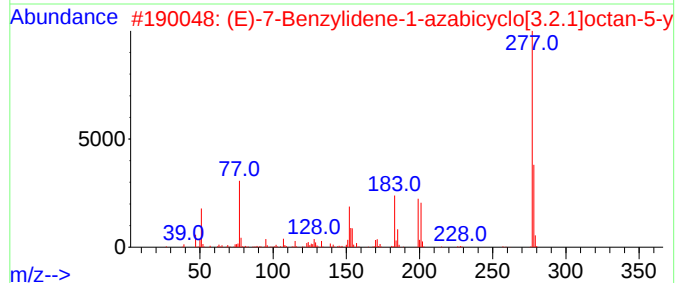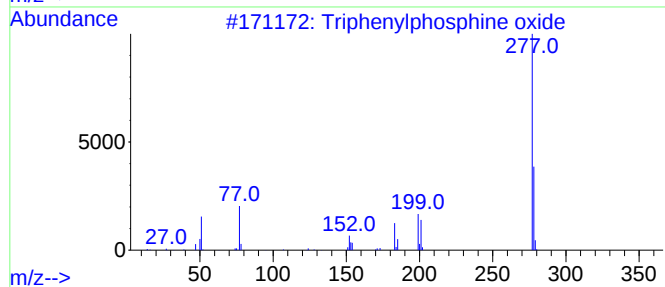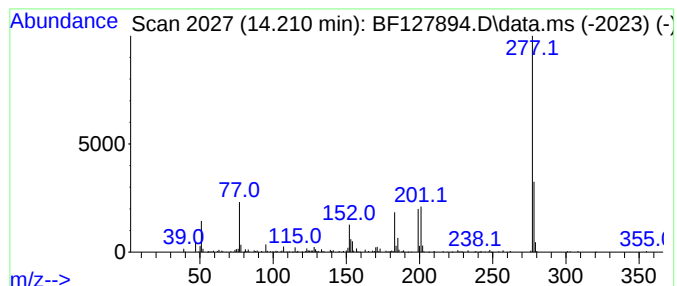

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
Data File : BF127894.D
Acq On : 25 Apr 2022 21:46
Operator : CG\JU
Sample : N2548-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-8D

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.210	3.0	ng	153596	5	14.115	1020890	20.0