
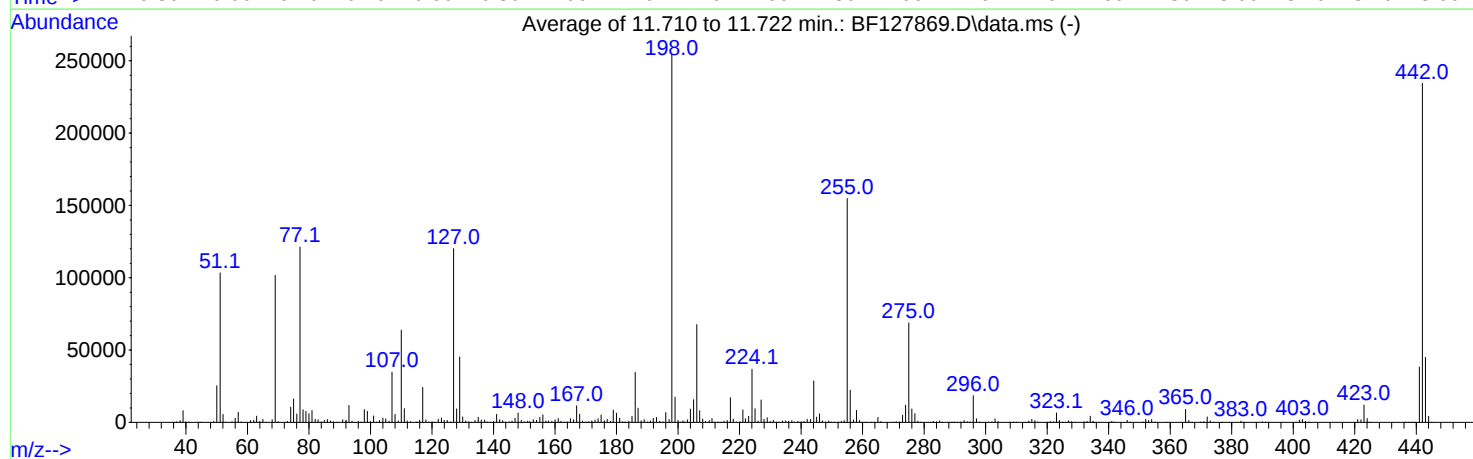


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
 Data File : BF127869.D
 Acq On : 25 Apr 2022 09:44
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Apr 24 00:43:03 2022

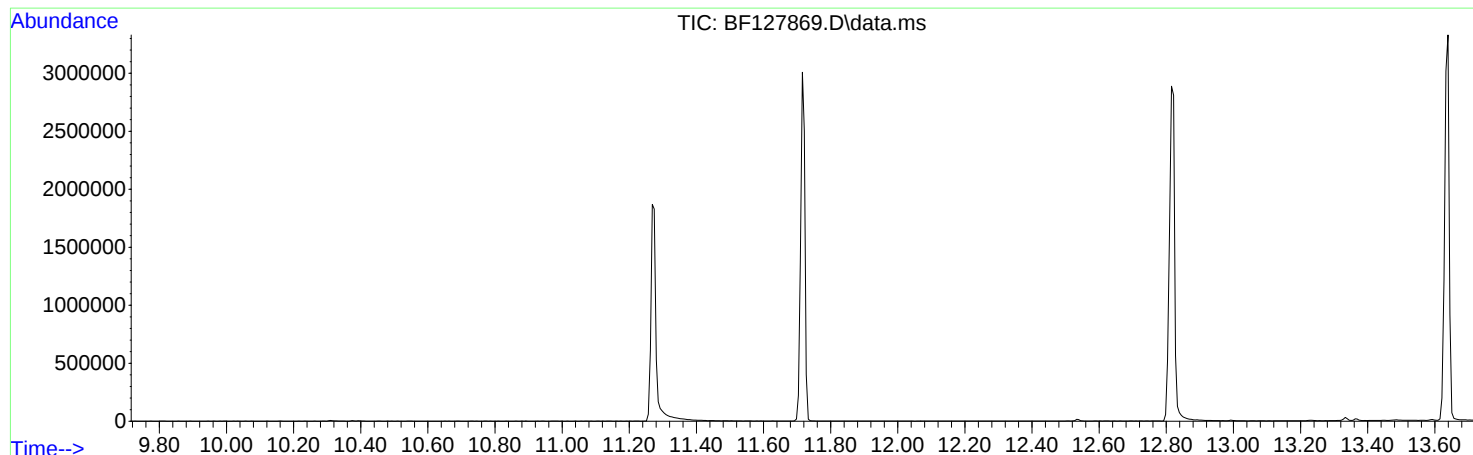




AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	103363	PASS
68	69	0.00	2	1.9	1883	PASS
69	198	0.00	100	40.0	101640	PASS
70	69	0.00	2	0.6	621	PASS
127	198	10	80	47.2	120133	PASS
197	198	0.00	2	0.8	2050	PASS
198	198	100	100	100.0	254357	PASS
199	198	5	9	6.9	17511	PASS
275	198	10	60	27.1	68827	PASS
365	198	1	100	3.5	9006	PASS
441	198	0.01	100	15.1	38291	PASS
442	442	50	100	100.0	234403	PASS
443	442	15	24	19.2	44944	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
Data File : BF127869.D
Acq On : 25 Apr 2022 09:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 25 17:09:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 00:43:03 2022
Response via : Initial Calibration

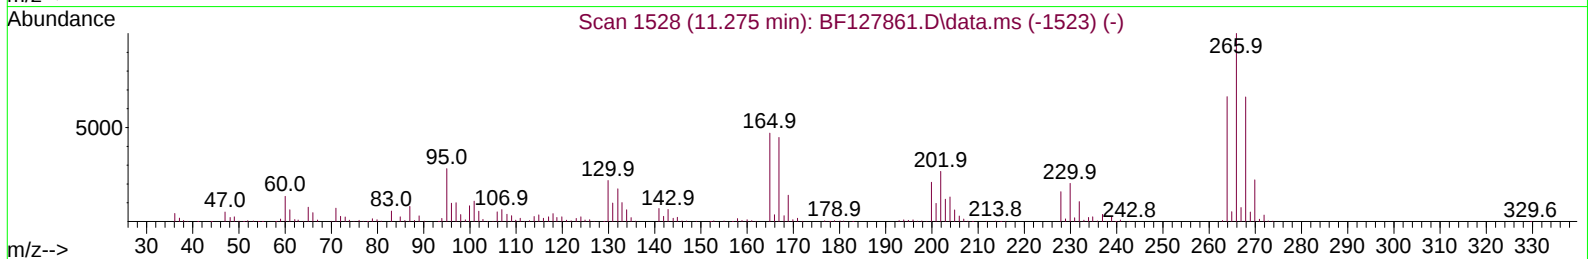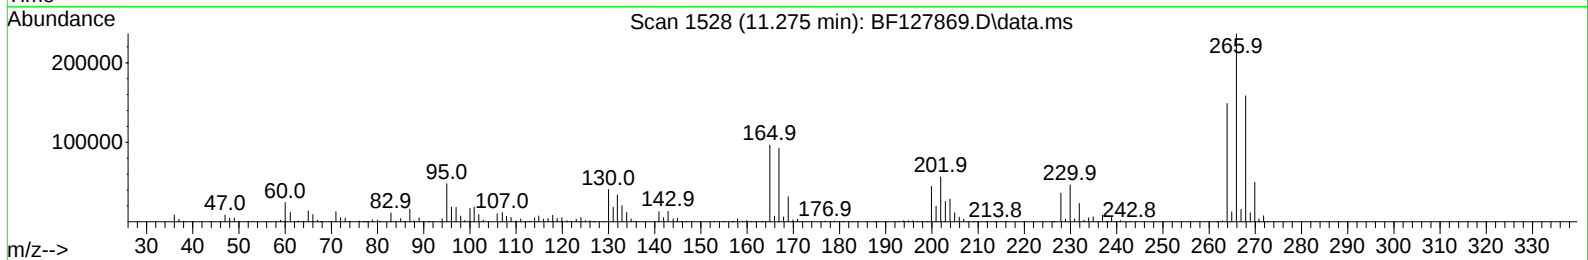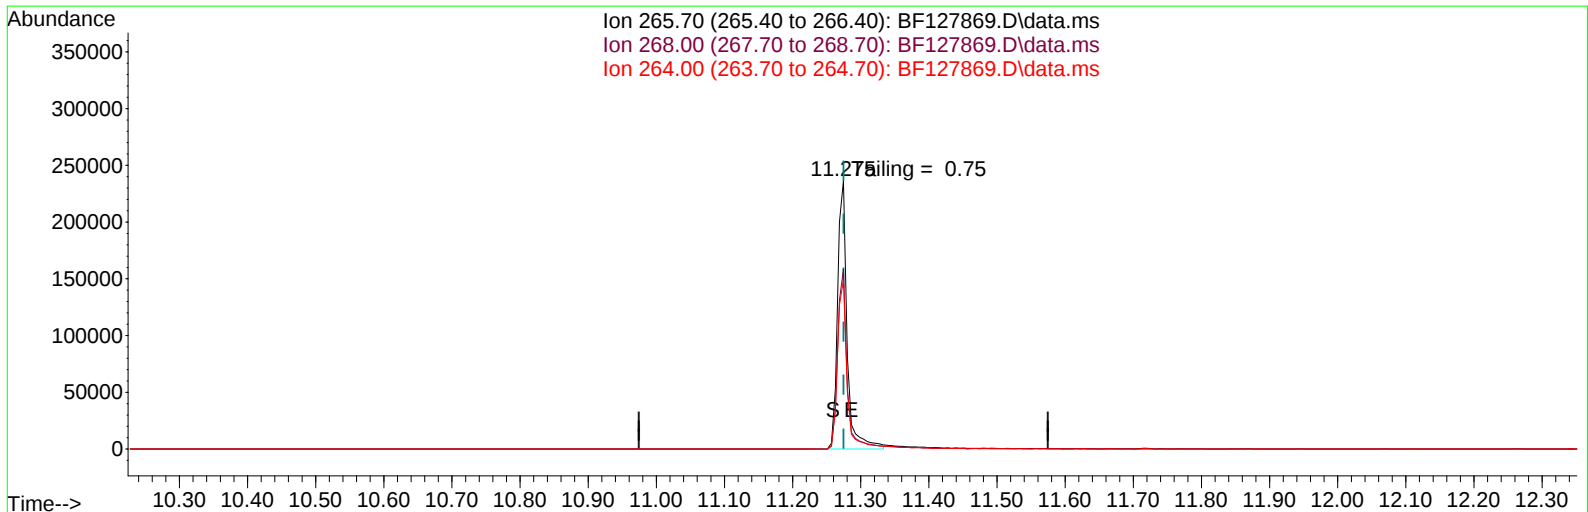

TIC: BF127869.D\data.ms

(70) Pentachlorophenol (C)

11.275min (-0.000) 473855.03 ng




response 234427

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	67.02
264.00	66.40	62.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
 Data File : BF127869.D
 Acq On : 25 Apr 2022 09:44
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 25 17:09:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Apr 24 00:43:03 2022
 Response via : Initial Calibration

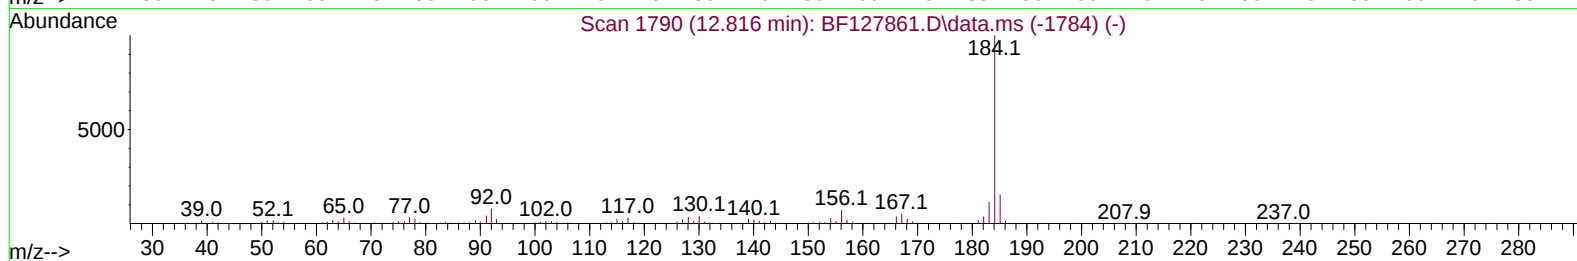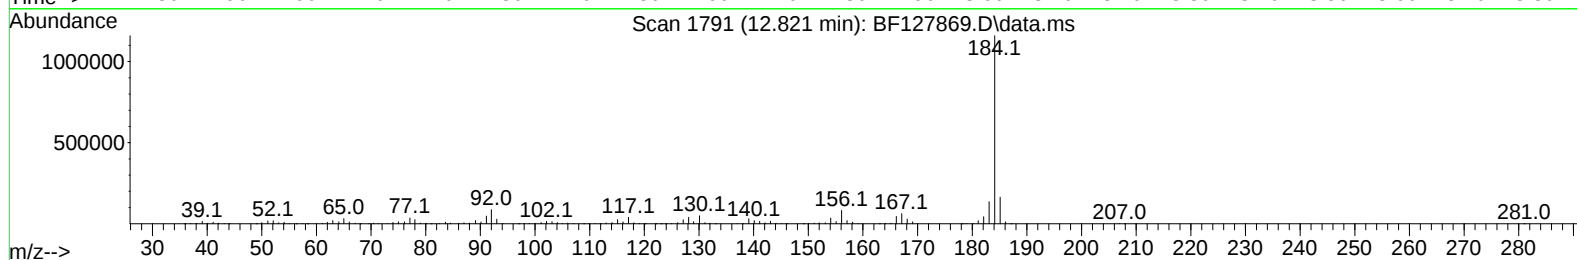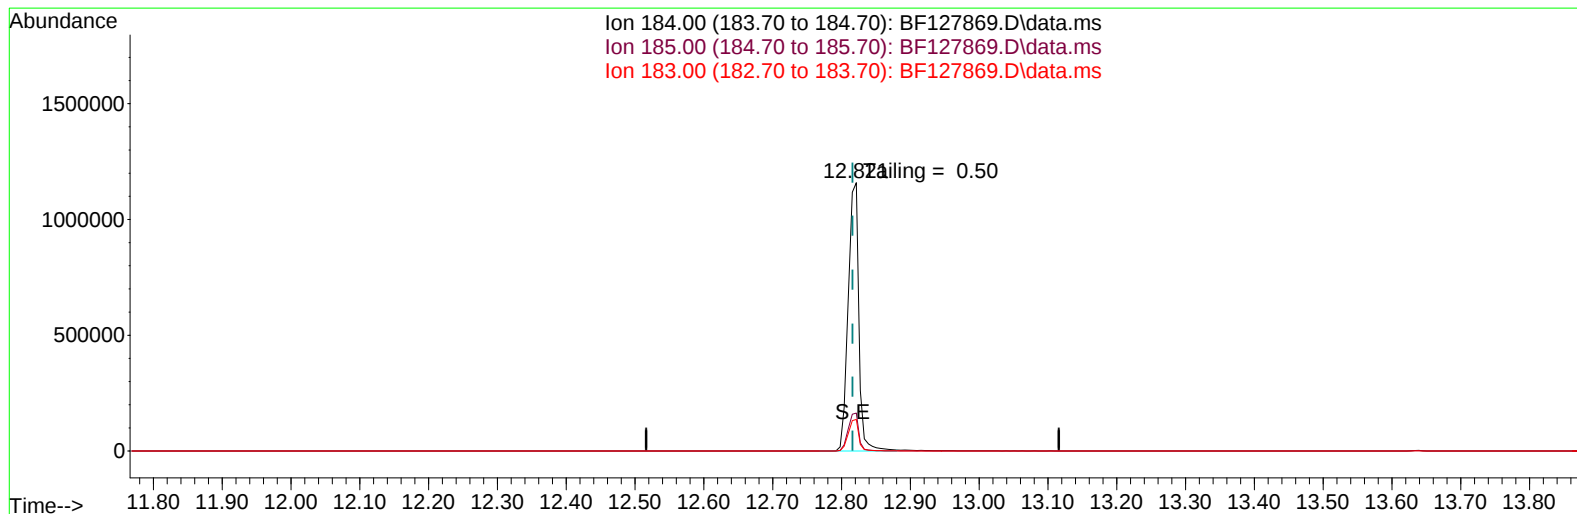

TIC: BF127869.D\data.ms

(77) Benzidine

12.821min (+ 0.005) 7454.68 ng m

response 1250860

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.13
183.00	11.20	11.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/25/2022	BNA_F	<u>BF127869.D</u>
Compound Name	Response	Retention Time
DDT	594227	13.63
DDD	5048	13.33
DDE	1041	12.99
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6089	600316	1.01

Instrument :
BNA_F
ClientSampleId :
DFTPP