
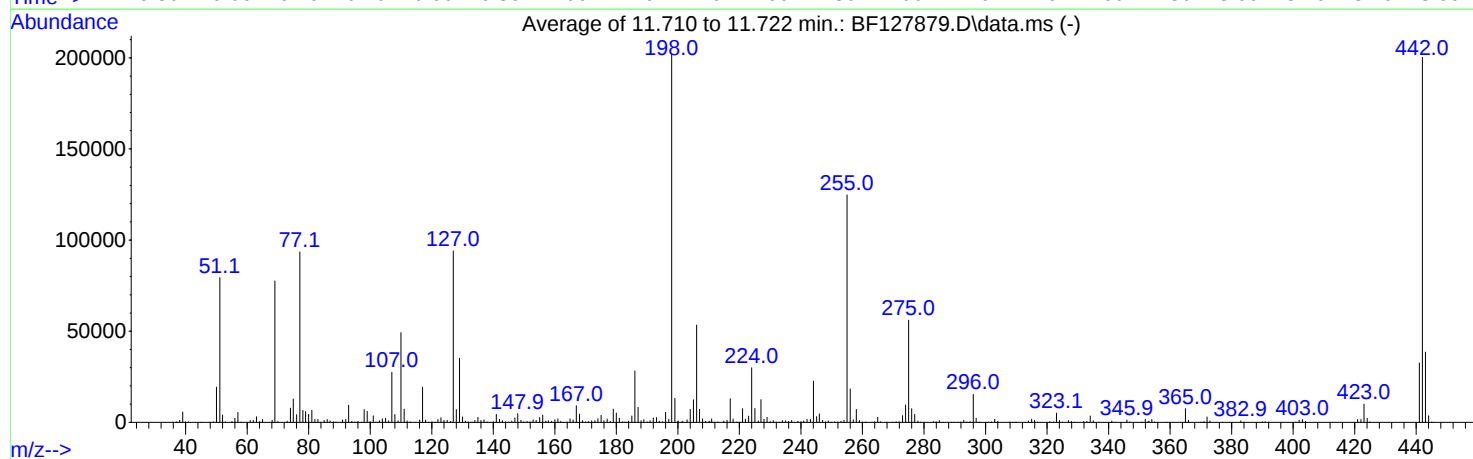


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
 Data File : BF127879.D
 Acq On : 25 Apr 2022 14:36
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Apr 24 00:43:03 2022

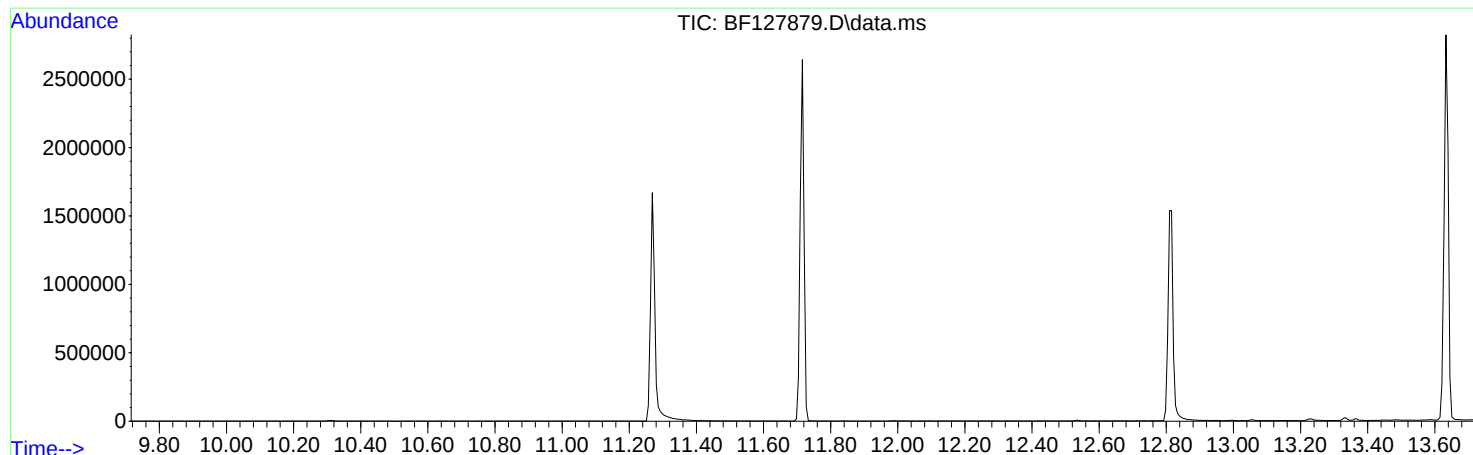




AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	79416	PASS
68	69	0.00	2	1.5	1169	PASS
69	198	0.00	100	38.4	77573	PASS
70	69	0.00	2	0.5	406	PASS
127	198	10	80	46.6	94035	PASS
197	198	0.00	2	0.8	1638	PASS
198	198	100	100	100.0	201827	PASS
199	198	5	9	6.5	13215	PASS
275	198	10	60	27.8	56040	PASS
365	198	1	100	3.8	7580	PASS
441	198	0.01	100	16.2	32606	PASS
442	442	50	100	100.0	200211	PASS
443	442	15	24	19.3	38560	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\  
Data File : BF127879.D  
Acq On    : 25 Apr 2022  14:36  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 25 17:11:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Sun Apr 24 00:43:03 2022
Response via : Initial Calibration

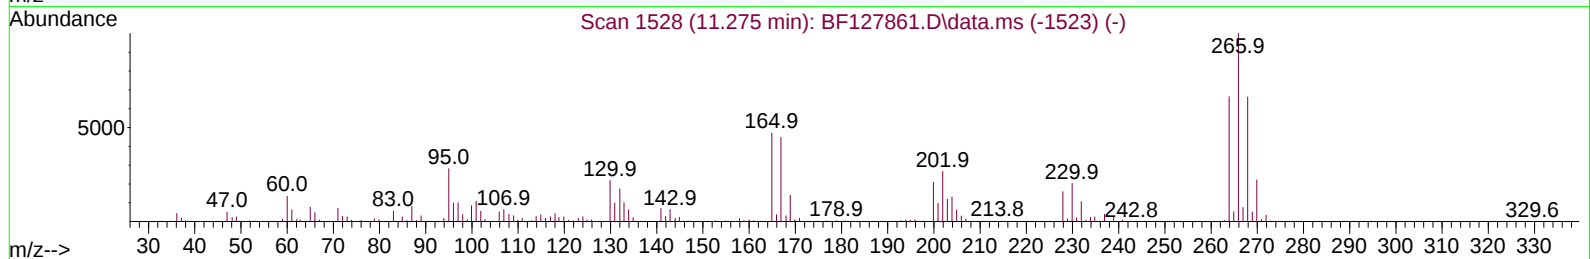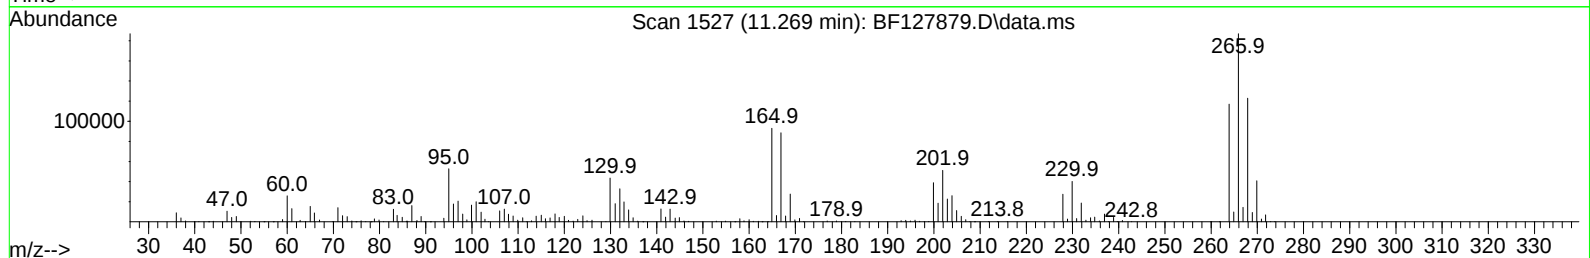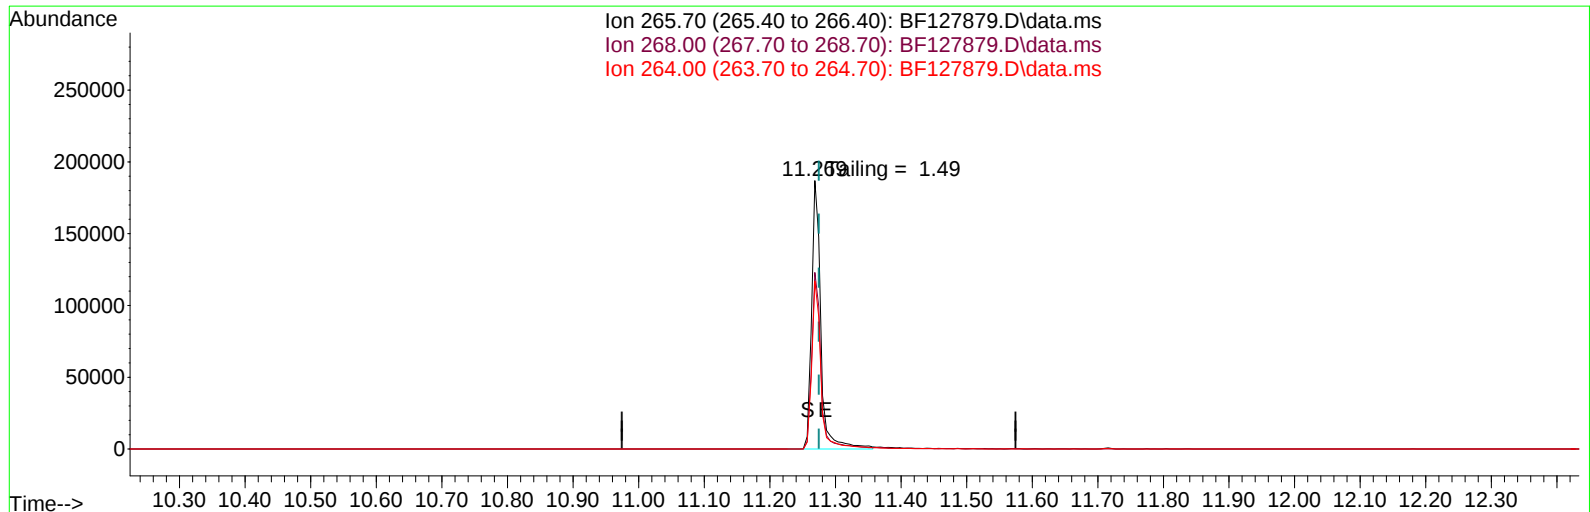

TIC: BF127879.D\data.ms

(70) Pentachlorophenol (C)

11.269min (-0.006) 26641.07 ng




response	186899
----------	--------

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	65.77
264.00	66.40	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
 Data File : BF127879.D
 Acq On : 25 Apr 2022 14:36
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 25 17:11:48 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Apr 24 00:43:03 2022
 Response via : Initial Calibration

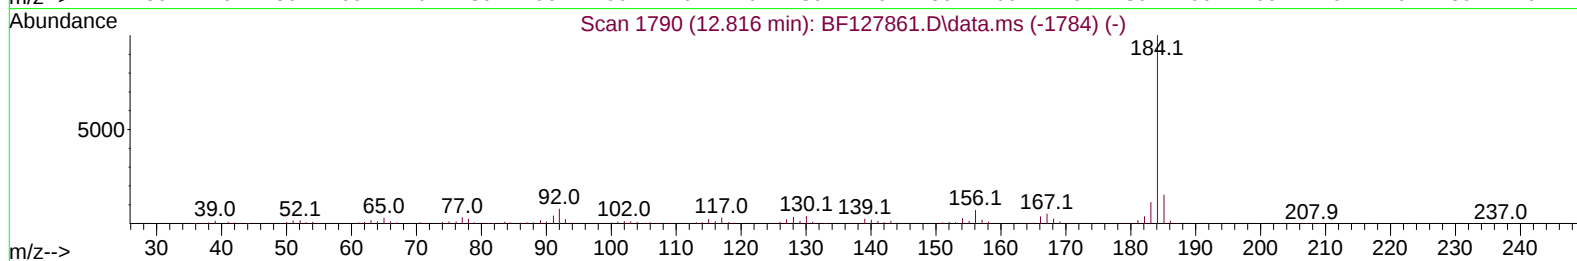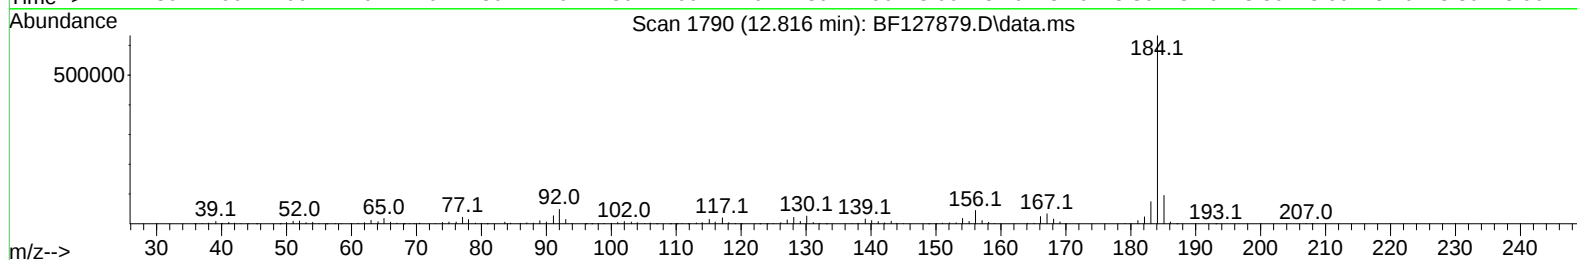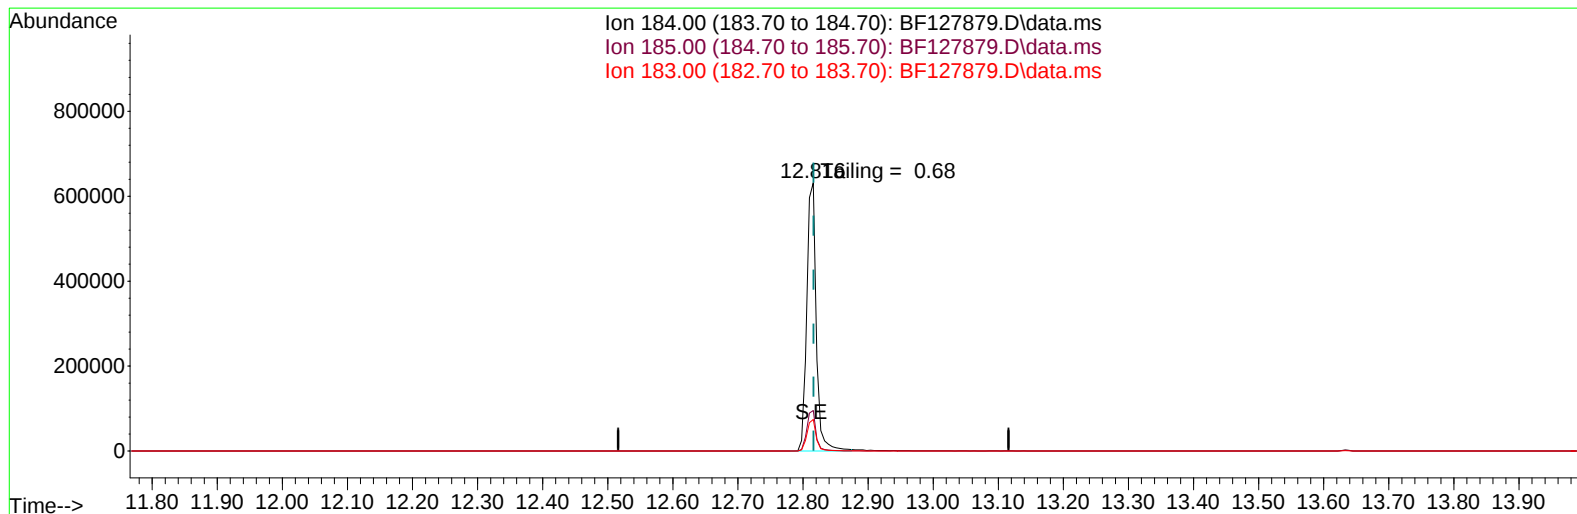

TIC: BF127879.D\data.ms

(77) Benzidine

12.816min (-0.000) 0.00 ng

response 645568

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	15.12
183.00	11.20	11.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/25/2022	BNA_F	<u>BF127879.D</u>
Compound Name	Response	Retention Time
DDT	472236	13.63
DDD	227	13.36
DDE	533	12.99
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
760	472996	0.16

Instrument :
BNA_F
ClientSampleId :
DFTPP