
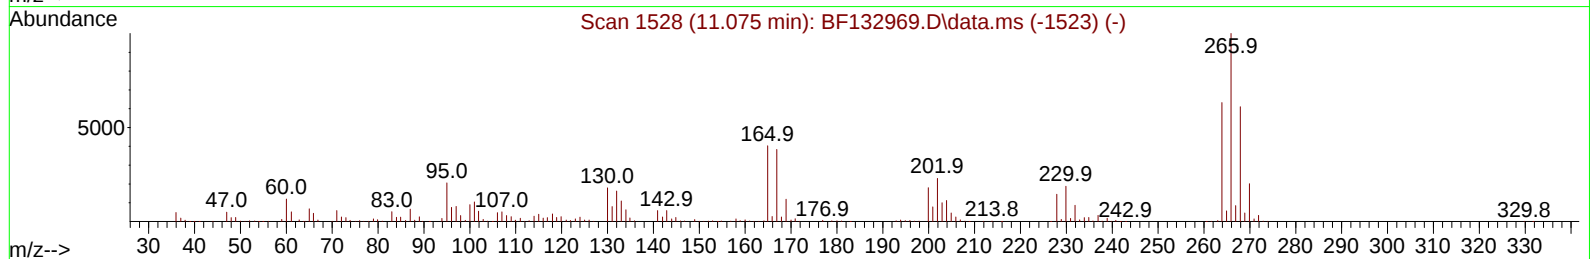
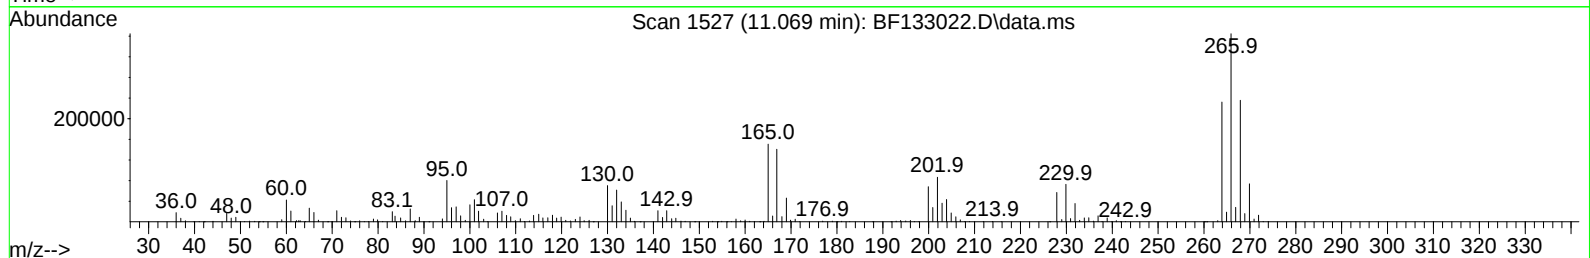


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042523\
Data File : BF133022.D
Acq On : 25 Apr 2023 09:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 07:23:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 25 18:24:07 2023
Response via : Initial Calibration

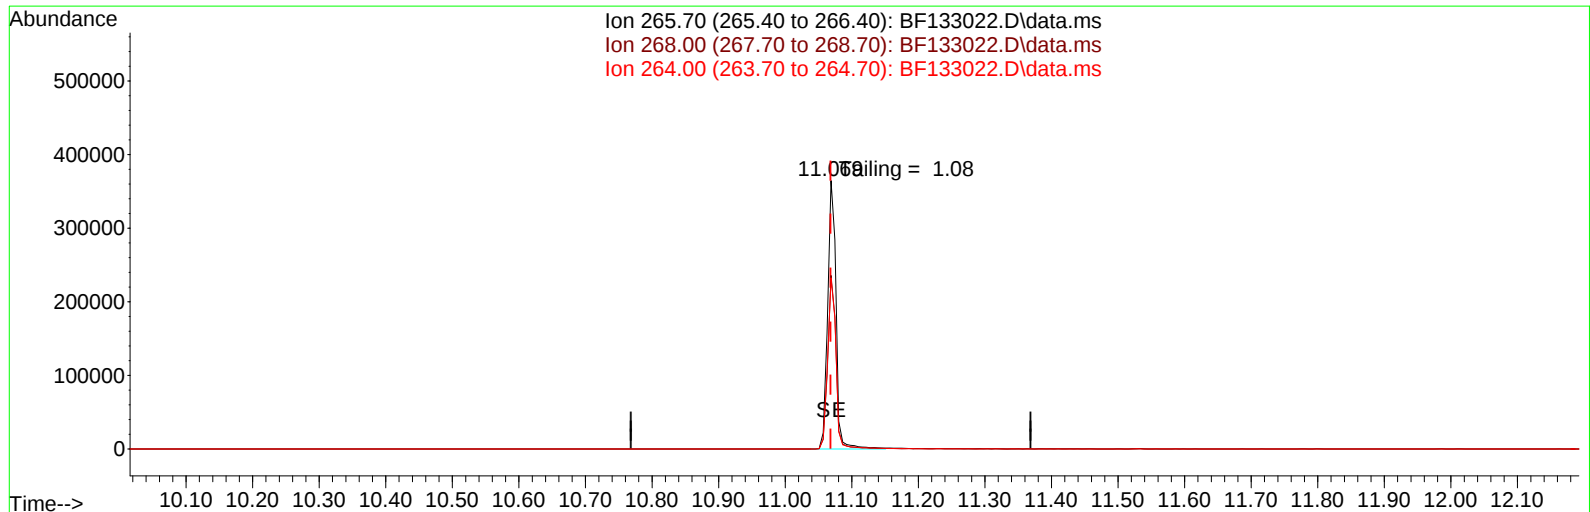

TIC: BF133022.D\data.ms

(70) Pentachlorophenol (C)




11.069min (+ 0.000) 582557.88 ng

response 322760

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	64.63
264.00	63.30	63.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042523\
 Data File : BF133022.D
 Acq On : 25 Apr 2023 09:59
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 07:23:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 25 18:24:07 2023
 Response via : Initial Calibration

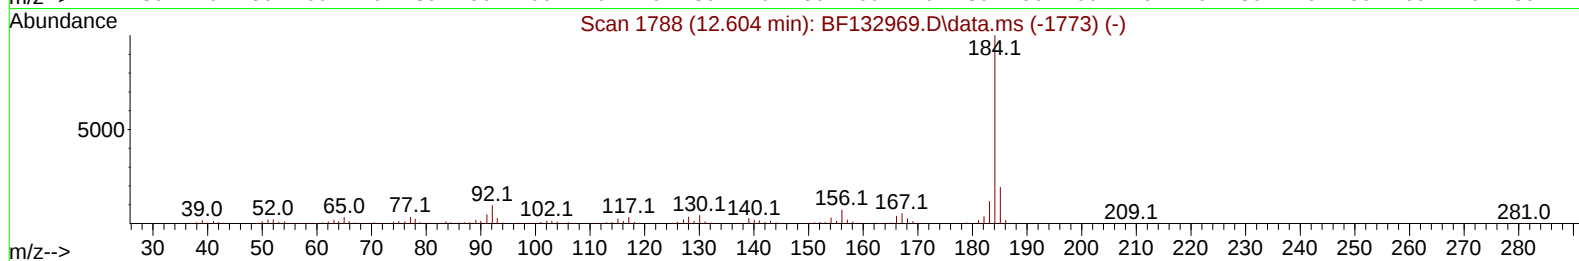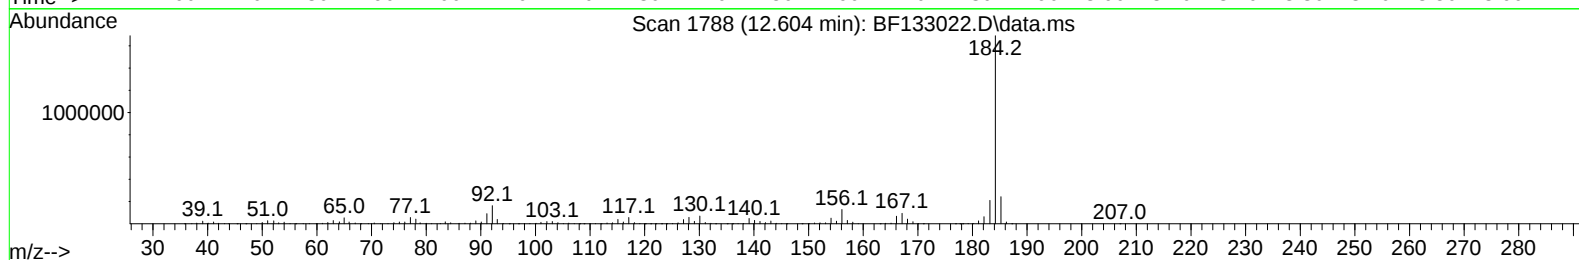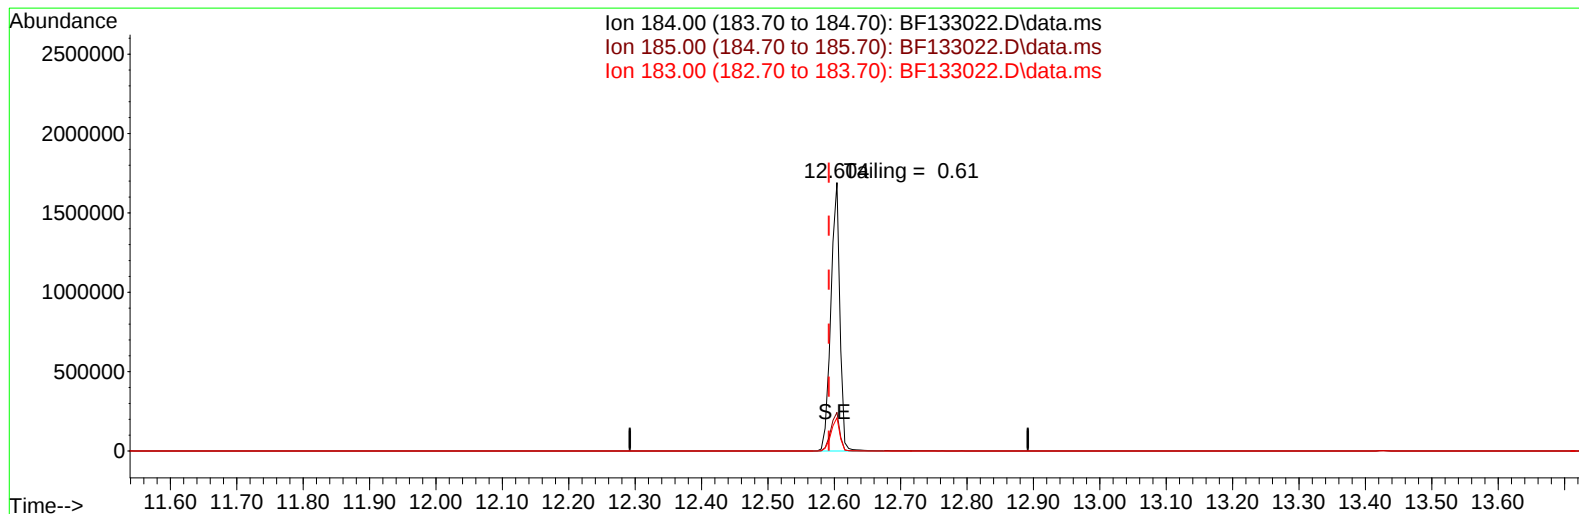

TIC: BF133022.D\data.ms

(77) Benzidine

12.604min (+ 0.012) 0.00 ng

response 1591448

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.37#
183.00	11.70	12.44
0.00	0.00	0.00