
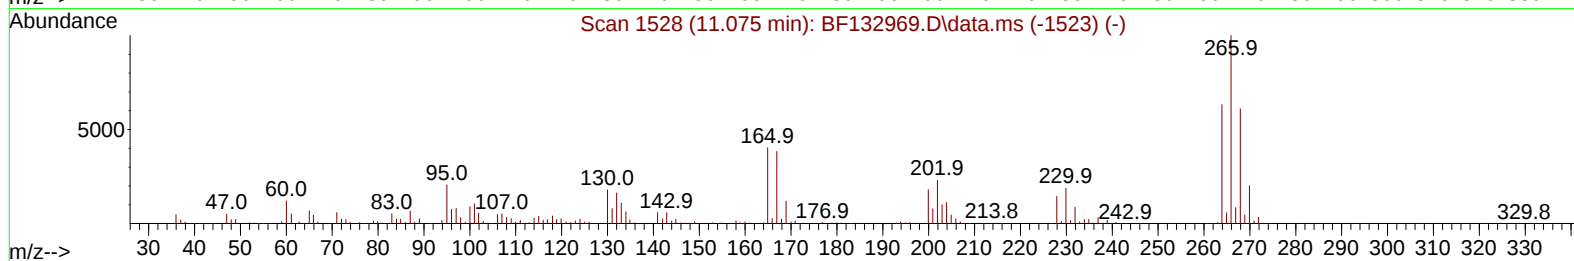
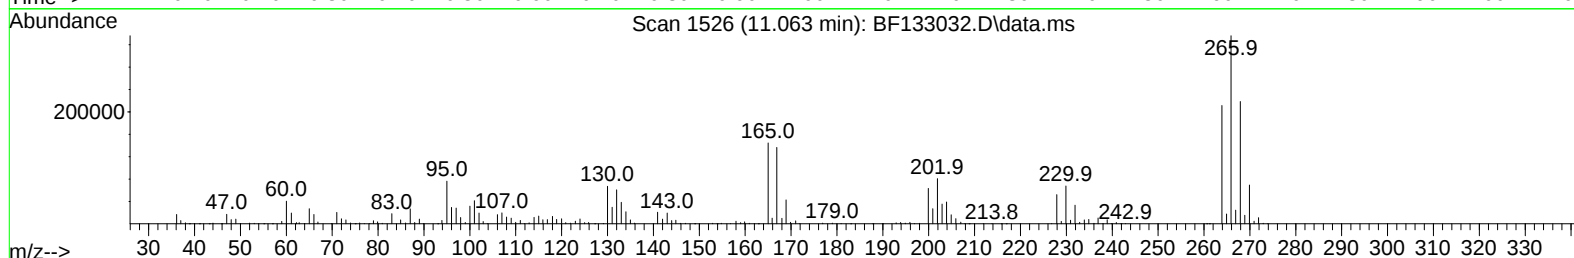


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042523\
Data File : BF133032.D
Acq On : 25 Apr 2023 17:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 07:25:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 25 18:24:07 2023
Response via : Initial Calibration

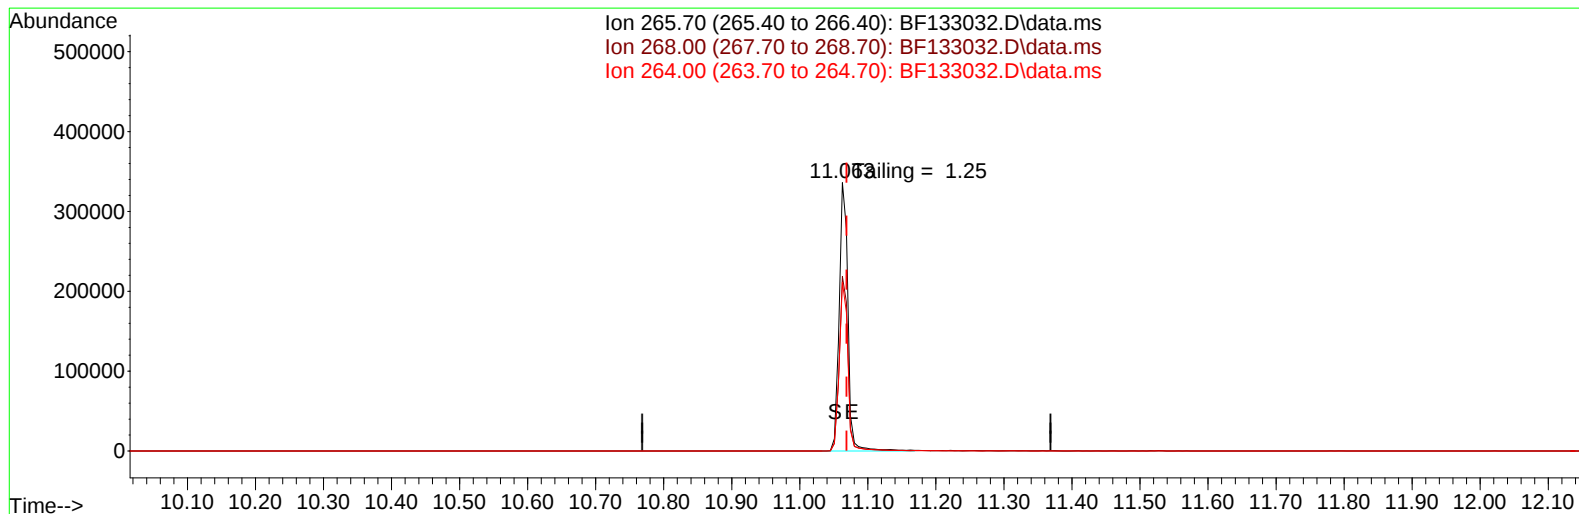

TIC: BF133032.D\data.ms

(70) Pentachlorophenol (C)




11.063min (-0.006) 178118.31 ng

response 300283

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	65.05
264.00	63.30	62.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042523\
Data File : BF133032.D
Acq On : 25 Apr 2023 17:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 07:25:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 25 18:24:07 2023
Response via : Initial Calibration

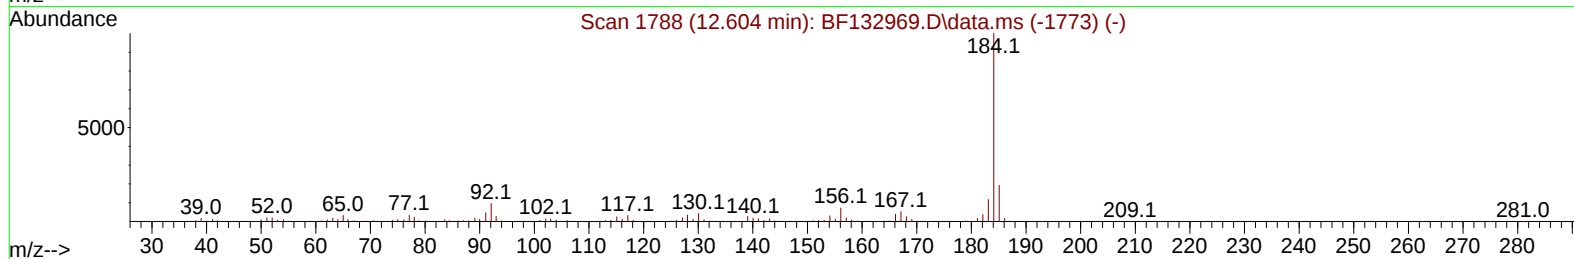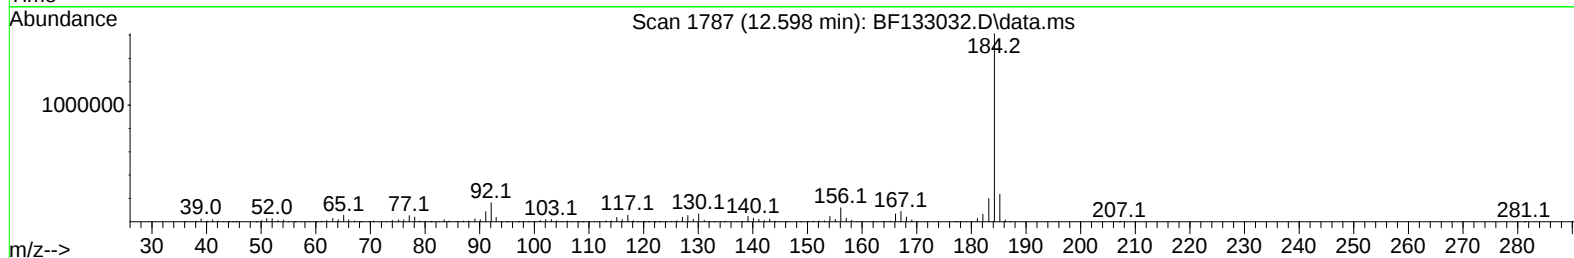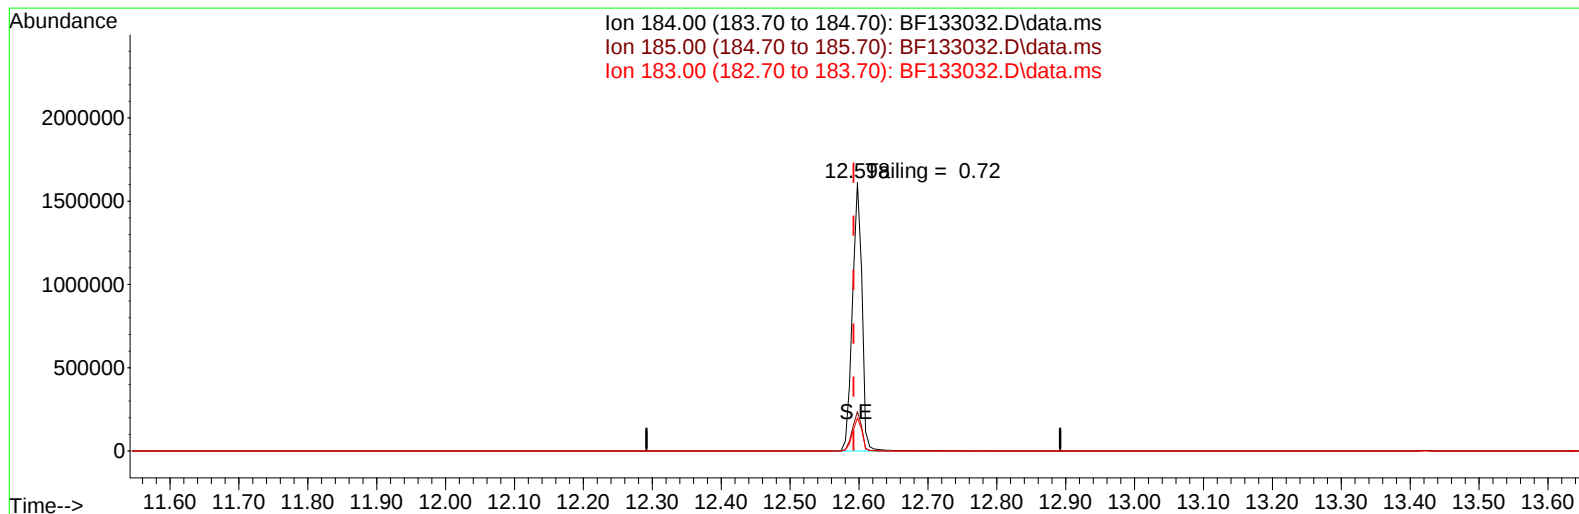

TIC: BF133032.D\data.ms

(77) Benzidine**12.598min (+ 0.006) 9139.99 ng****response 1542838**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.66#
183.00	11.70	12.34
0.00	0.00	0.00