

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042523\
 Data File : BF133041.D
 Acq On : 25 Apr 2023 22:29
 Operator : CG\JU
 Sample : 02483-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S2S-TP2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133041.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.934	479	484	489	rVB	85884	107605	2.69%	0.348%
2	5.351	550	555	558	rBV	3696809	3455675	86.31%	11.181%
3	6.375	724	729	732	rBV	3499496	3500494	87.43%	11.326%
4	6.739	787	791	794	rBV	1504461	1119776	27.97%	3.623%
5	7.304	882	887	890	rBV	2531550	2245665	56.09%	7.266%
6	8.022	1006	1009	1012	rBV	1958452	1459737	36.46%	4.723%
7	9.098	1188	1192	1195	rBV	4777631	3938350	98.37%	12.743%
8	9.774	1303	1307	1310	rBV	2197653	1730164	43.22%	5.598%
9	10.486	1425	1428	1431	rBV	1221087	918448	22.94%	2.972%
10	10.563	1436	1441	1444	rBV	2721682	2397361	59.88%	7.757%
11	10.792	1477	1480	1484	rVB	70476	55464	1.39%	0.179%
12	11.257	1555	1559	1561	rBV	2174613	1761850	44.01%	5.701%
13	11.274	1561	1562	1566	rVB	107393	83314	2.08%	0.270%
14	11.327	1566	1571	1574	rVB2	80155	66157	1.65%	0.214%
15	11.792	1646	1650	1654	rBV2	141092	154071	3.85%	0.499%
16	12.463	1760	1764	1768	rBV	390462	306026	7.64%	0.990%
17	12.574	1778	1783	1788	rBV5	30906	46963	1.17%	0.152%
18	12.692	1797	1803	1806	rBV	319037	317363	7.93%	1.027%
19	12.845	1824	1829	1832	rBV	4508837	4003591	100.00%	12.954%
20	13.886	2001	2006	2009	rBV	1417048	1486557	37.13%	4.810%
21	13.909	2009	2010	2017	rVB	151603	140424	3.51%	0.454%
22	14.904	2174	2179	2189	rBV2	101240	199570	4.98%	0.646%
23	15.192	2224	2228	2233	rVB	64391	79972	2.00%	0.259%
24	15.245	2233	2237	2243	rBV	80731	98637	2.46%	0.319%
25	15.309	2243	2248	2255	rBV	934301	1080783	27.00%	3.497%
26	16.680	2477	2481	2490	rVB3	45321	94565	2.36%	0.306%
27	17.086	2546	2550	2556	rVB	33718	57061	1.43%	0.185%




Sum of corrected areas: 30905643

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042523\
Data File : BF133041.D
Acq On : 25 Apr 2023 22:29
Operator : CG\JU
Sample : 02483-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S2S-TP2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

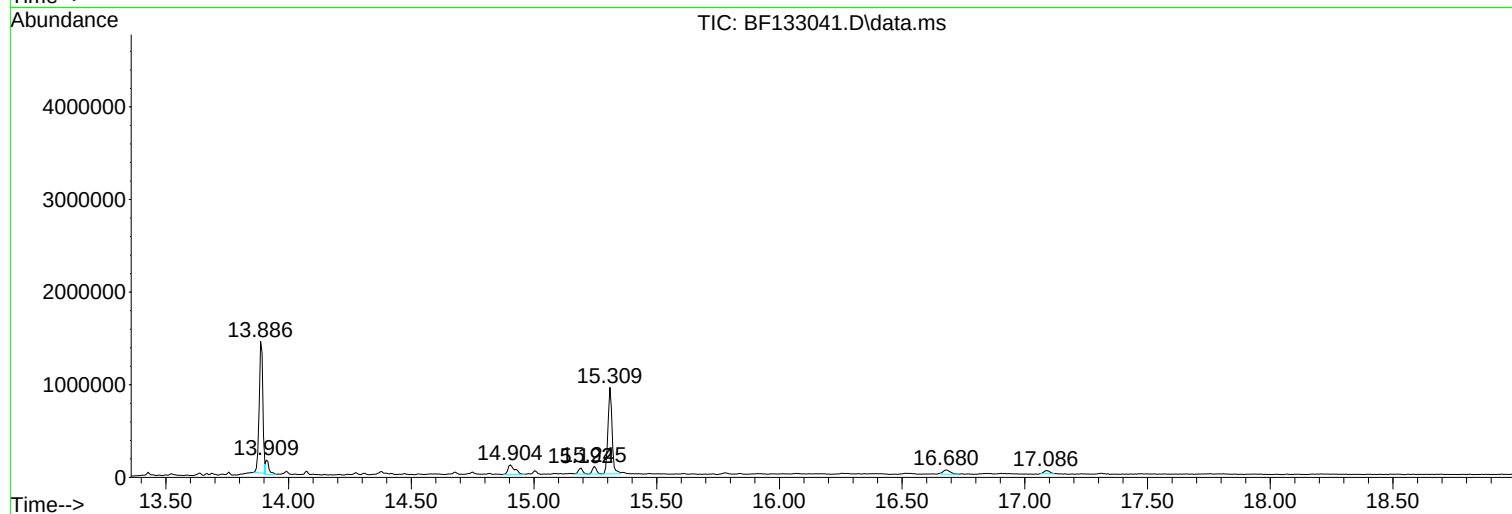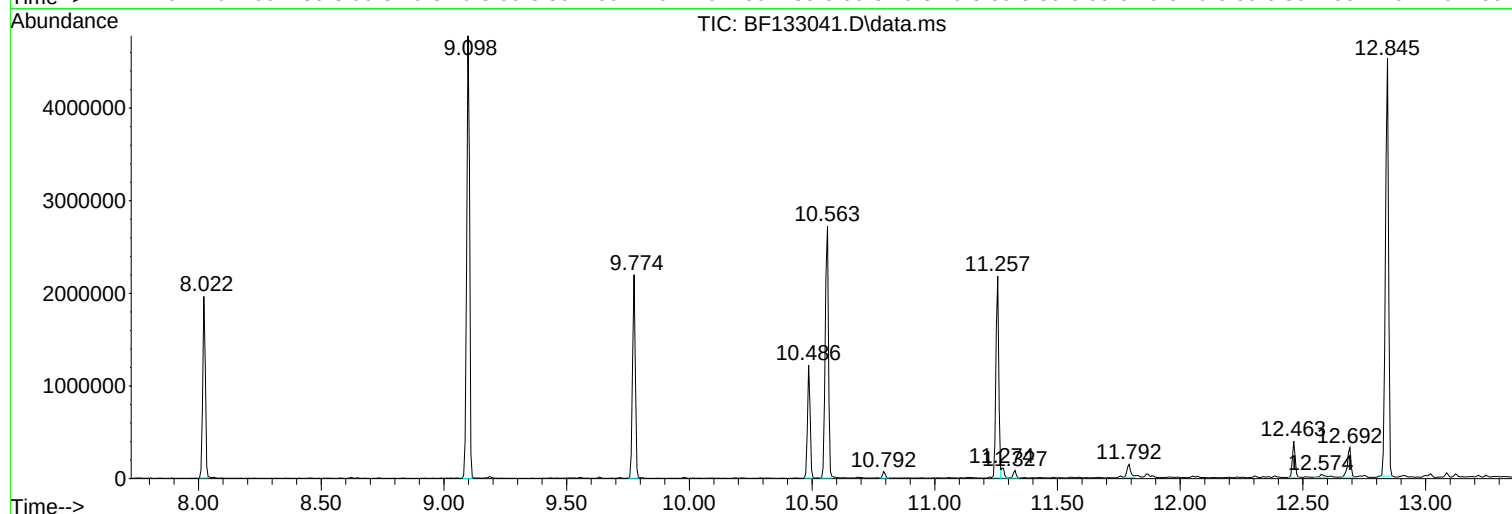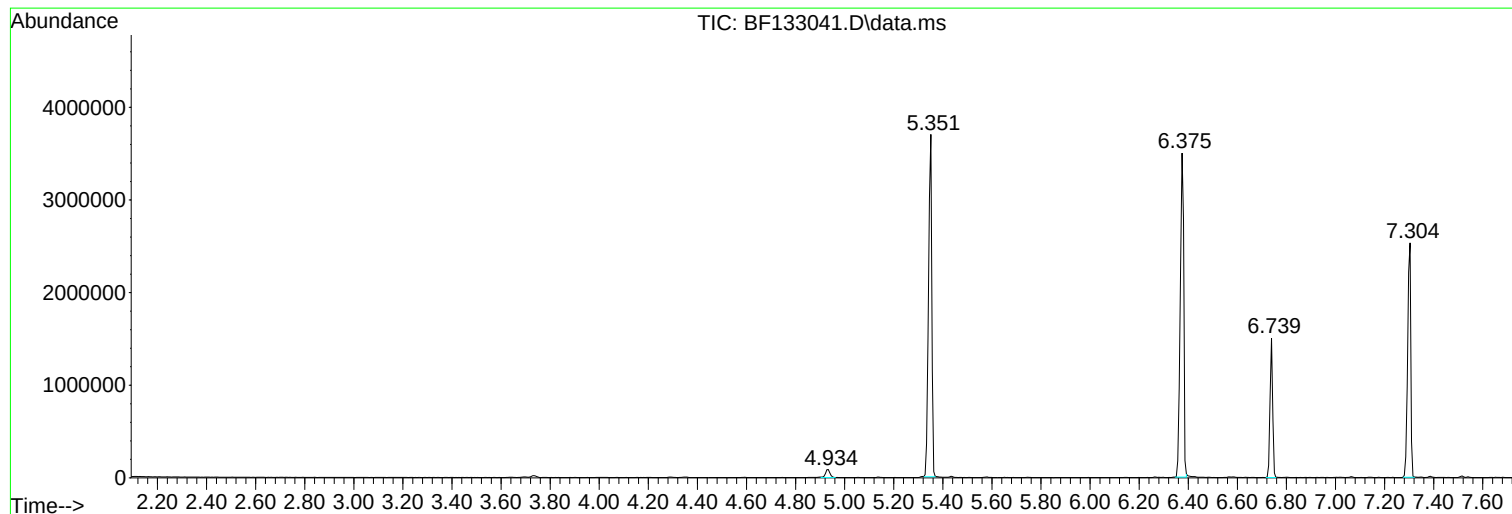

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042523\
Data File : BF133041.D
Acq On : 25 Apr 2023 22:29
Operator : CG\JU
Sample : 02483-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S2S-TP2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.486	10.62 ng	918448	Acenaphthene-d10	9.774

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	97
2			Acetophenone, 2-chloro-	154	C8H7ClO	000532-27-4	49
3			1,2-Propanedione, 1-phenyl-	148	C9H8O2	000579-07-7	47
4			Vinyl benzoate	148	C9H8O2	000769-78-8	47
5			N-Methylbenzamide, N-chlorodiflu...	247	C10H8ClF2NO2	1000446-98-2	47

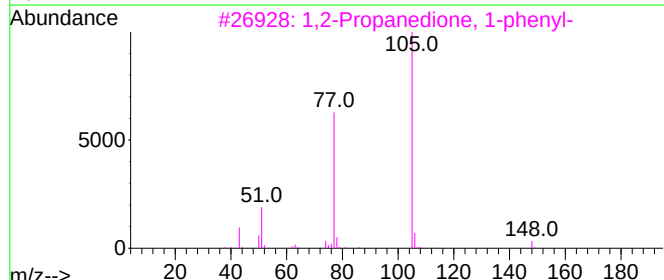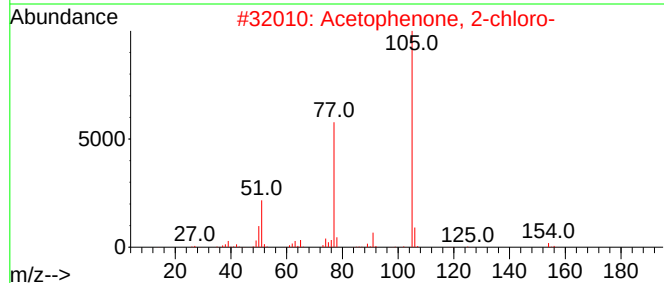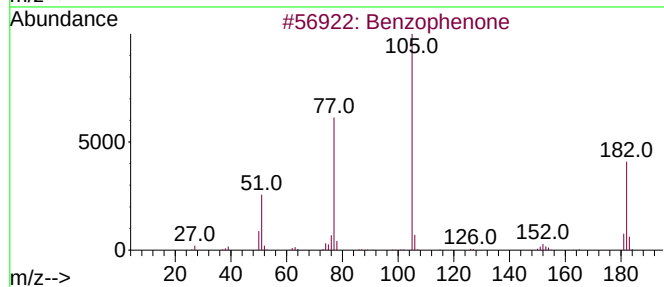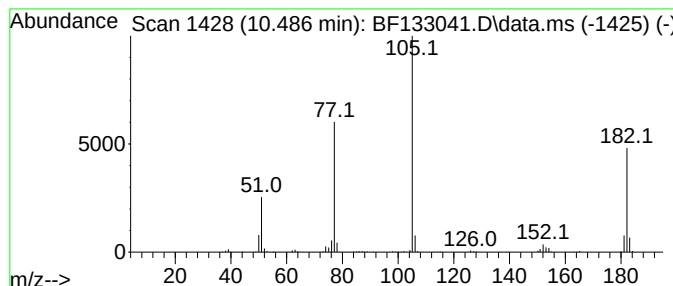

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042523\
Data File : BF133041.D
Acq On : 25 Apr 2023 22:29
Operator : CG\JU
Sample : 02483-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S2S-TP2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	10.486	10.6	ng	918448	3	9.774	1730160	20.0