
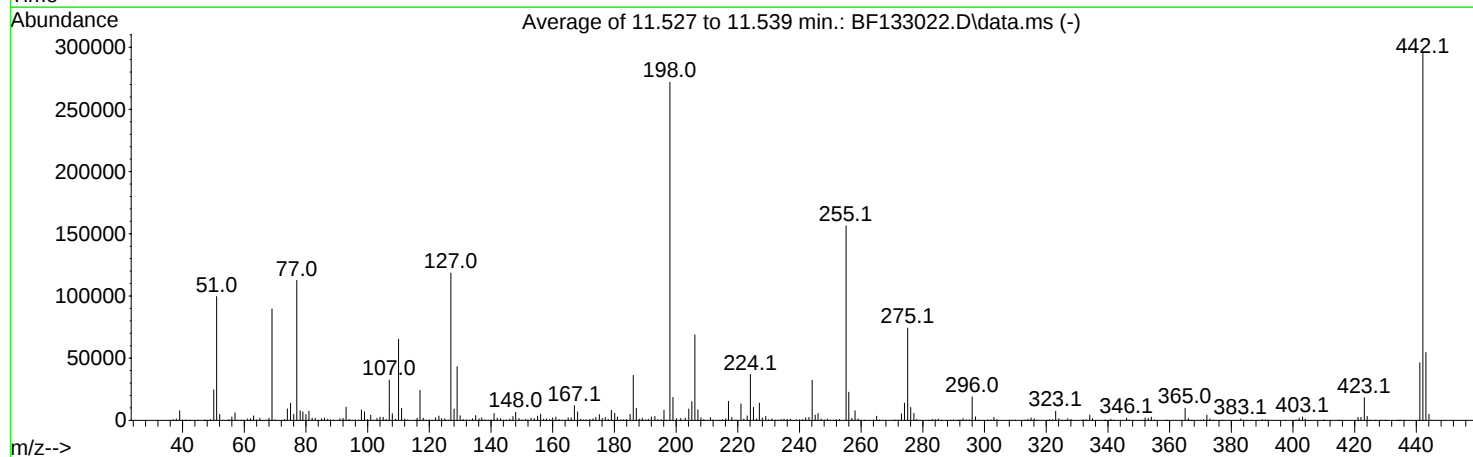


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042523\
 Data File : BF133022.D
 Acq On : 25 Apr 2023 09:59
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 25 18:24:07 2023

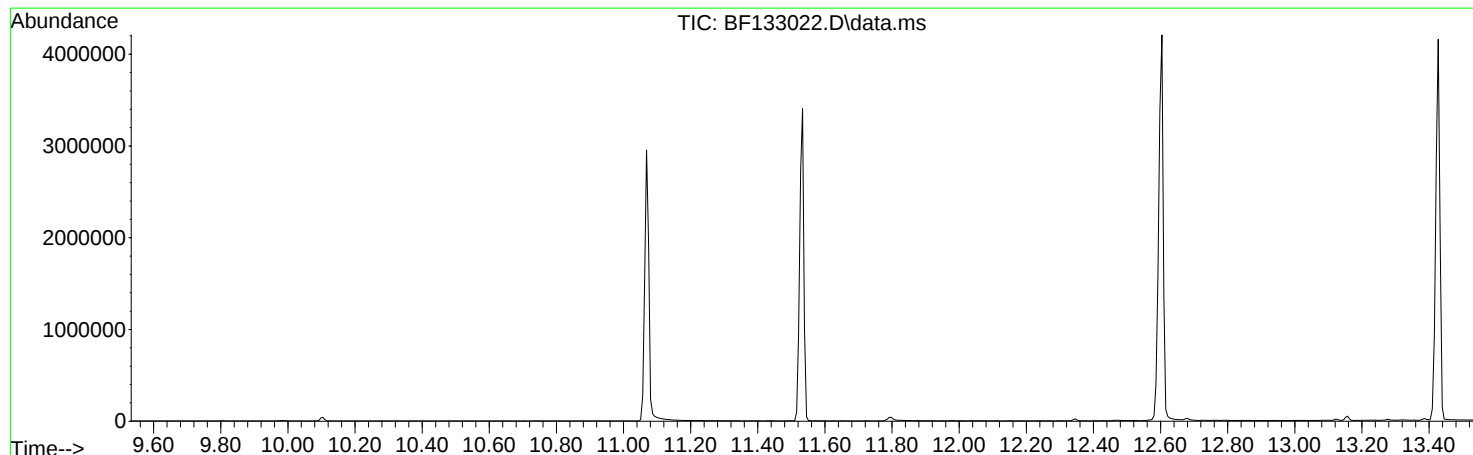

AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	99619	PASS
68	69	0.00	2	1.8	1620	PASS
69	198	0.00	100	33.0	89723	PASS
70	69	0.00	2	0.5	458	PASS
127	198	10	80	43.6	118368	PASS
197	198	0.00	2	0.1	262	PASS
198	198	100	100	100.0	271731	PASS
199	198	5	9	6.8	18371	PASS
275	198	10	60	27.3	74227	PASS
365	198	1	100	3.6	9754	PASS
441	198	0.01	100	17.0	46328	PASS
442	442	50	100	100.0	295701	PASS
443	442	15	24	18.4	54539	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/25/2023	BNA_F	<u>BF133022.D</u>
Compound Name	Response	Retention Time
DDT	713029	13.427
DDD	9472	13.157
DDE	473	12.792
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9945	722974	1.38

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042523\
Data File : BF133022.D
Acq On : 25 Apr 2023 09:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 26 07:23:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 25 18:24:07 2023
Response via : Initial Calibration

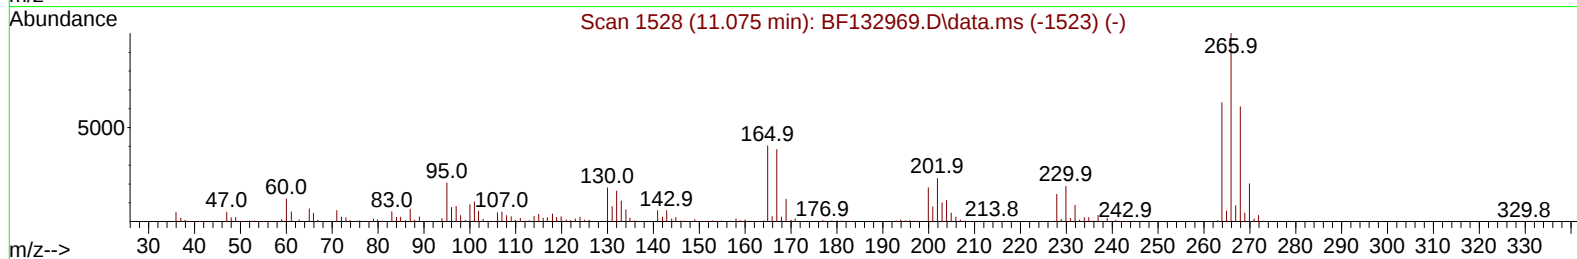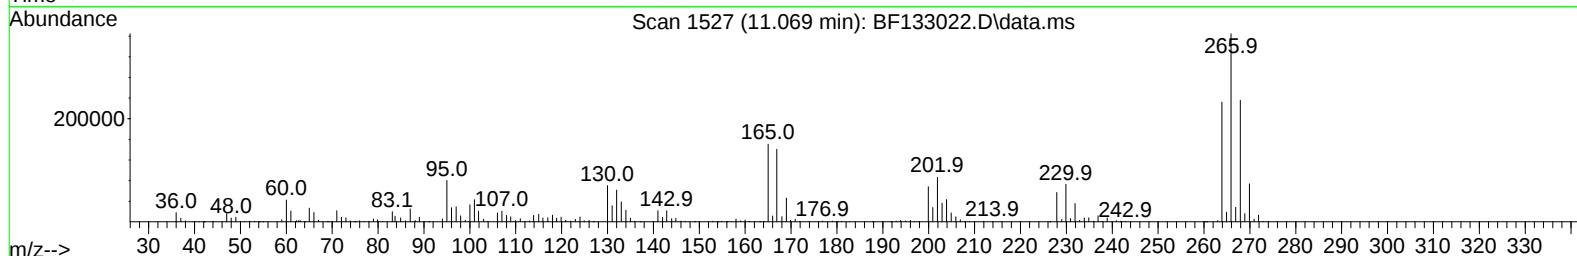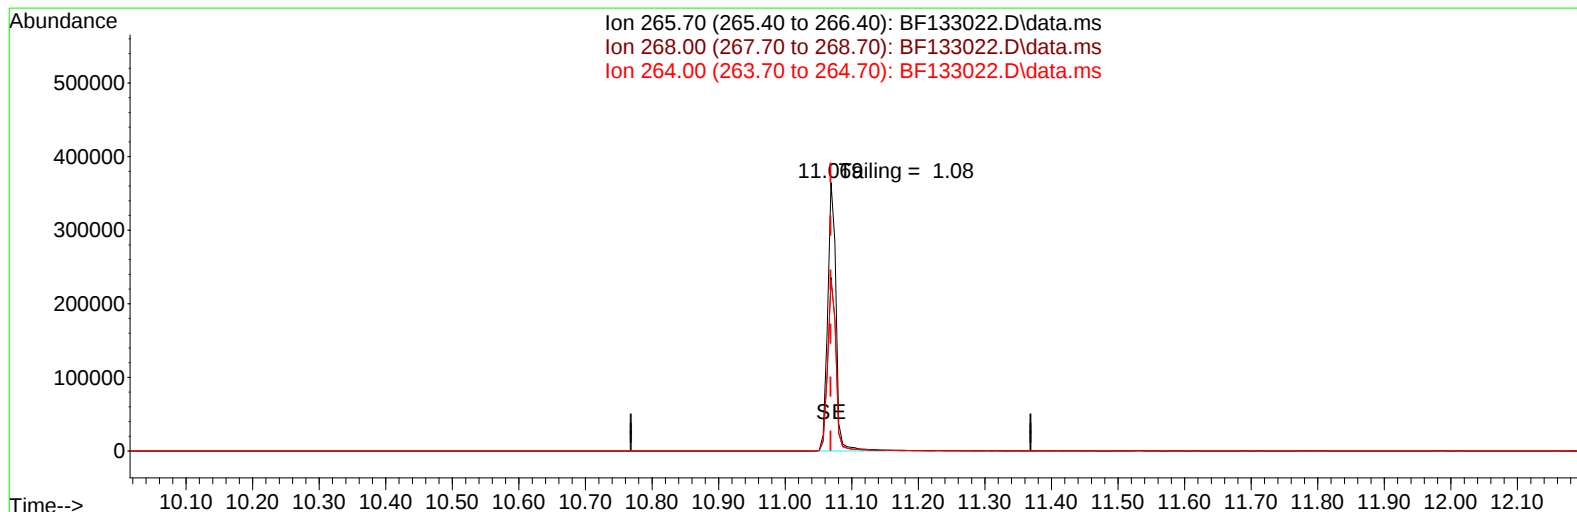

TIC: BF133022.D\data.ms

(70) Pentachlorophenol (C)

11.069min (+ 0.000) 582557.88 ng




response 322760

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	64.63
264.00	63.30	63.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042523\
Data File : BF133022.D
Acq On : 25 Apr 2023 09:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 26 07:23:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 25 18:24:07 2023
Response via : Initial Calibration

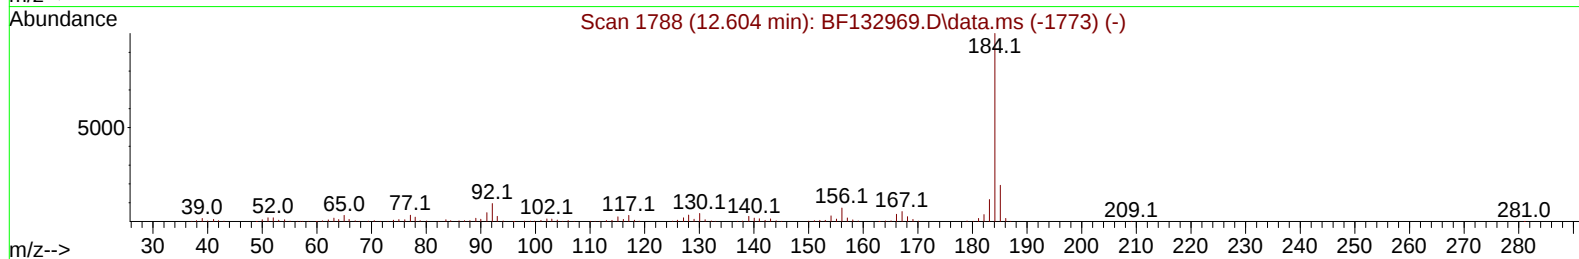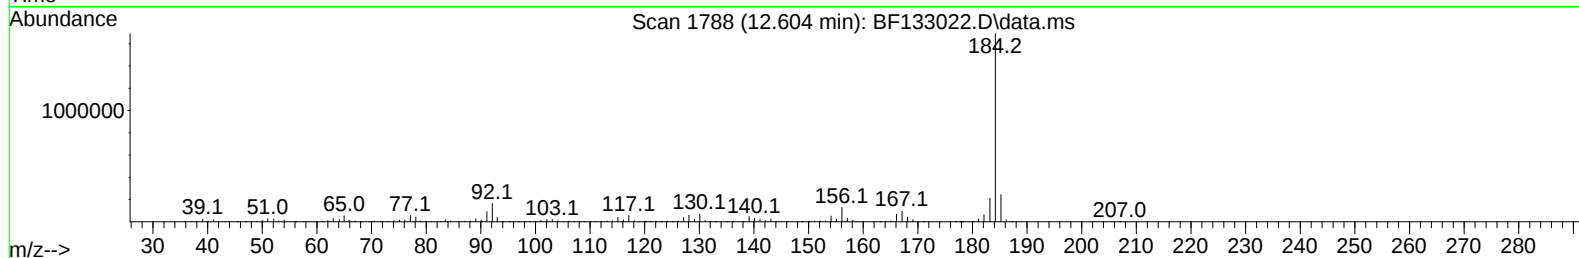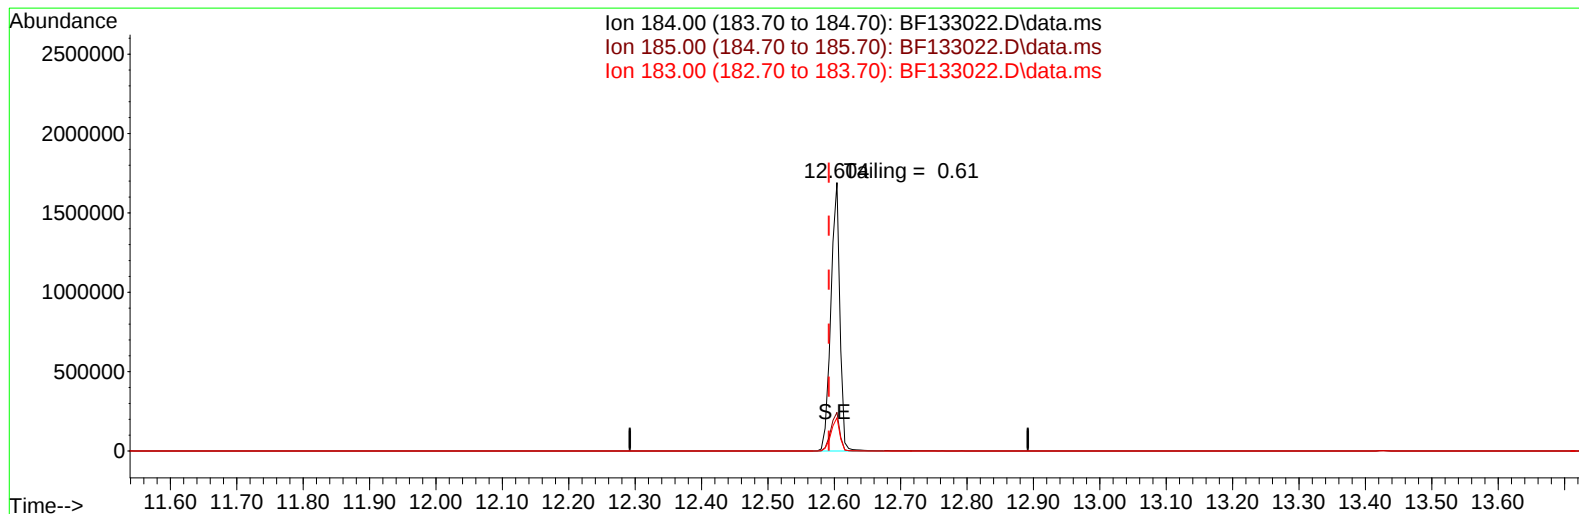

TIC: BF133022.D\data.ms

(77) Benzidine

12.604min (+ 0.012) 0.00 ng

response 1591448

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.37#
183.00	11.70	12.44
0.00	0.00	0.00