


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042523\
 Data File : BF133032.D
 Acq On : 25 Apr 2023 17:53
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 25 18:24:07 2023

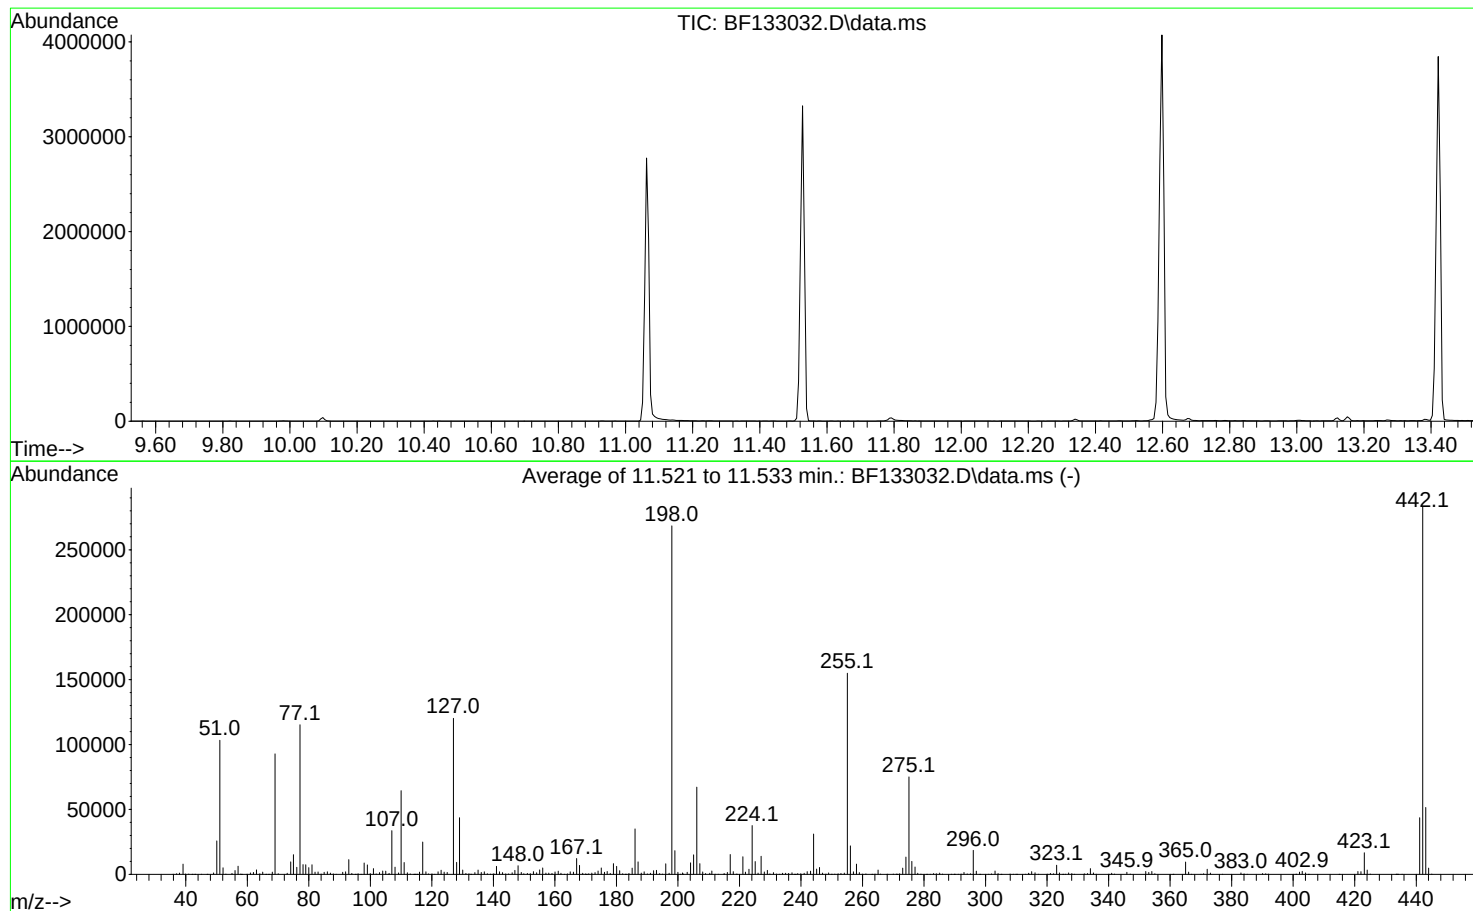

AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	103243	PASS
68	69	0.00	2	1.9	1731	PASS
69	198	0.00	100	34.6	92819	PASS
70	69	0.00	2	0.5	472	PASS
127	198	10	80	44.8	120203	PASS
197	198	0.00	2	0.3	854	PASS
198	198	100	100	100.0	268480	PASS
199	198	5	9	6.8	18272	PASS
275	198	10	60	28.0	75043	PASS
365	198	1	100	3.5	9447	PASS
441	198	0.01	100	16.3	43677	PASS
442	442	50	100	100.0	283355	PASS
443	442	15	24	18.2	51507	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/25/2023	BNA_F	<u>BF133032.D</u>
Compound Name	Response	Retention Time
DDT	644595	13.421
DDD	11770	13.151
DDE	418	12.792
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12188	656783	1.86

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042523\
 Data File : BF133032.D
 Acq On : 25 Apr 2023 17:53
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 26 07:25:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 25 18:24:07 2023
 Response via : Initial Calibration

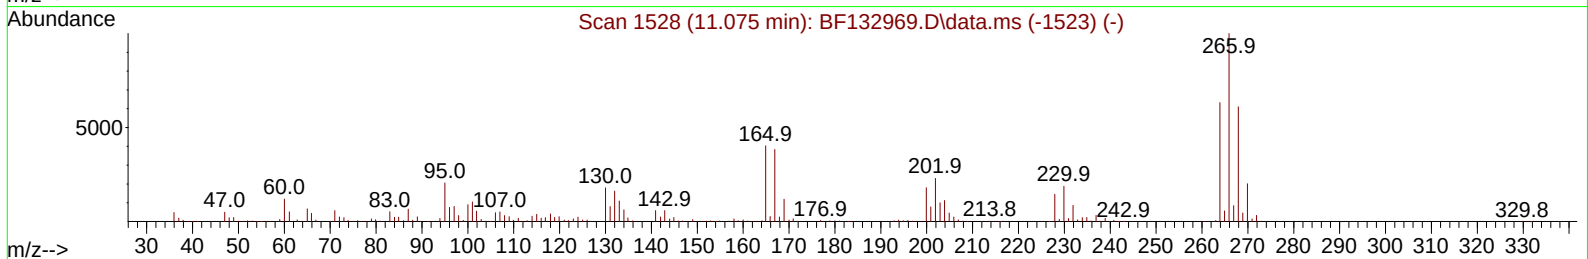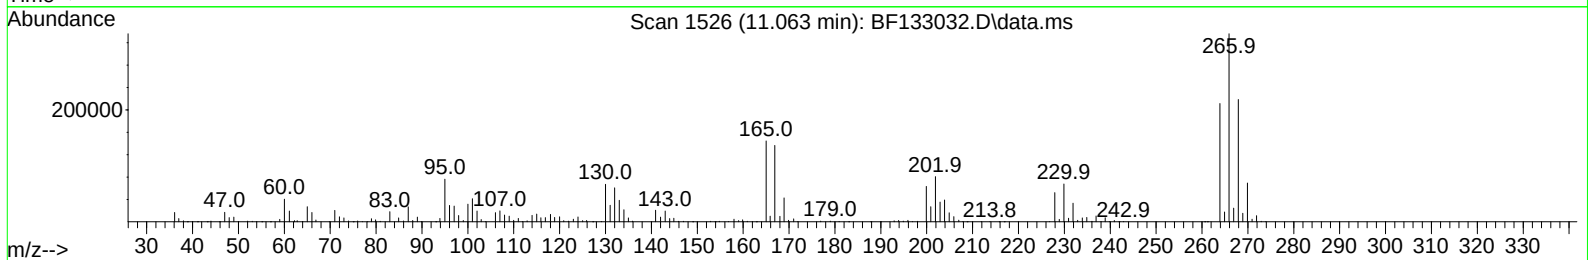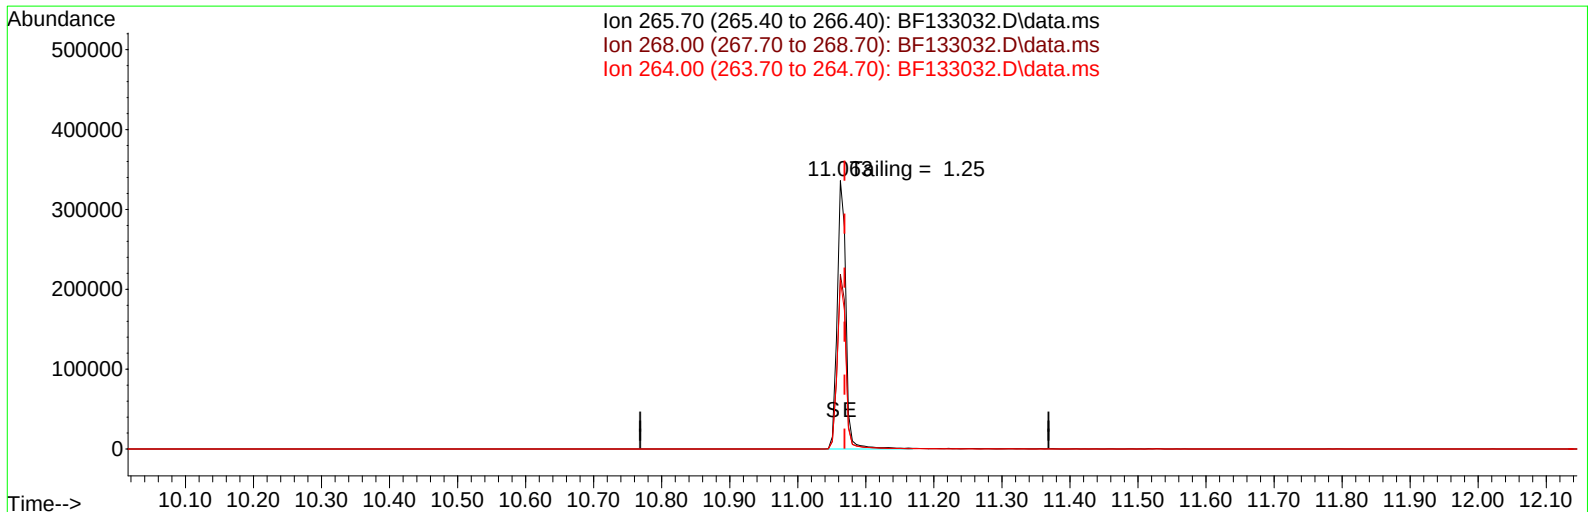

TIC: BF133032.D\data.ms

(70) Pentachlorophenol (C)

11.063min (-0.006) 178118.31 ng




response 300283

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	65.05
264.00	63.30	62.88
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042523\  
Data File : BF133032.D  
Acq On    : 25 Apr 2023  17:53  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 26 07:25:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 25 18:24:07 2023
Response via : Initial Calibration

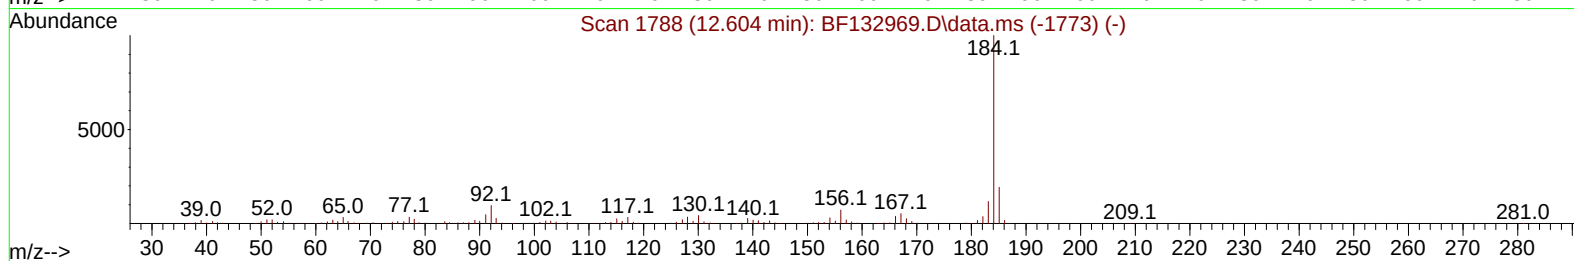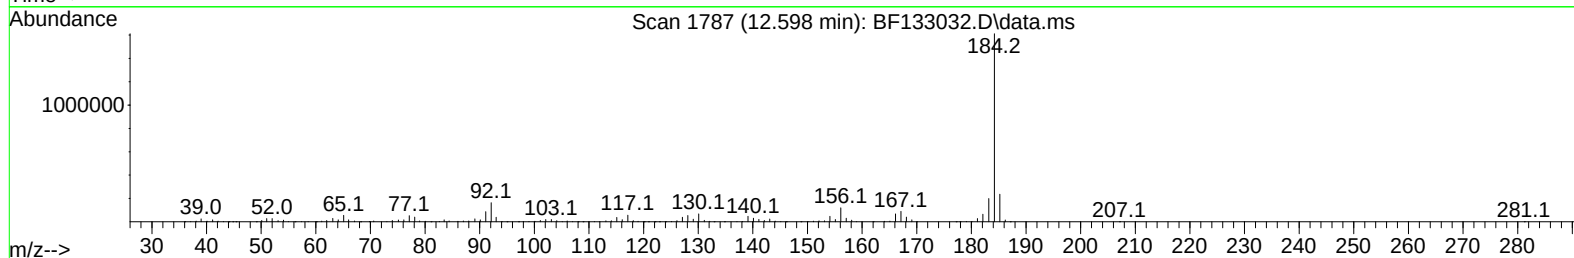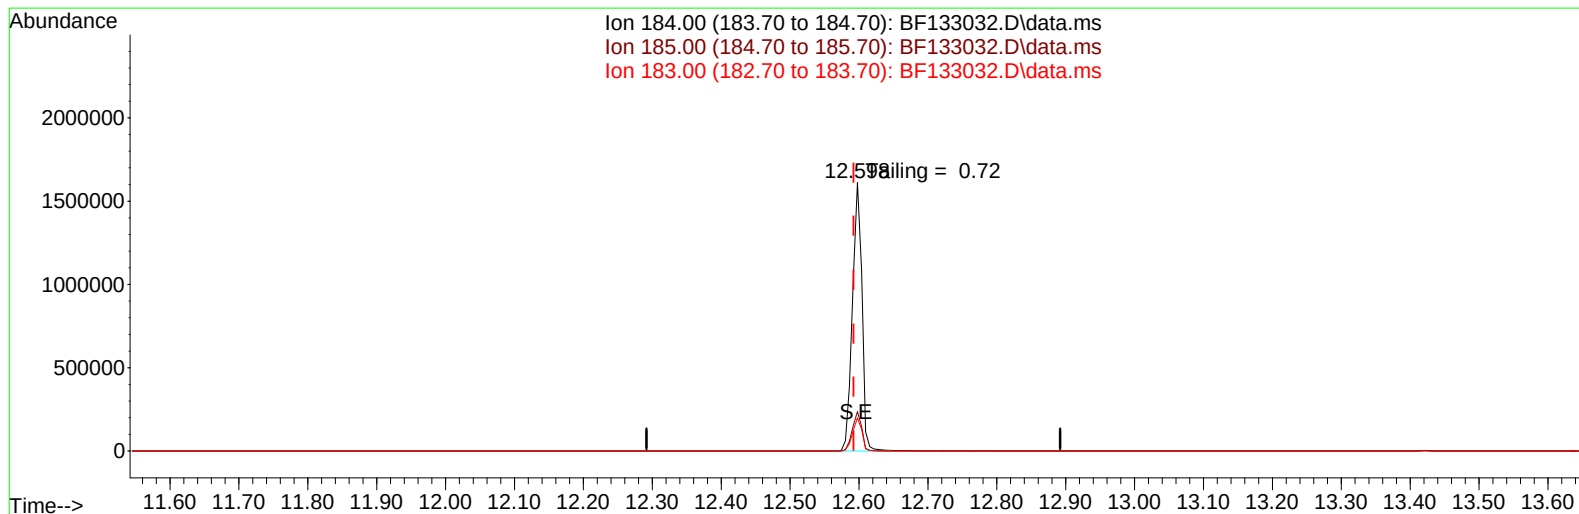

TIC: BF133032.D\data.ms

(77) Benzidine

12.598min (+ 0.006) 9139.99 ng

response **1542838**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.66#
183.00	11.70	12.34
0.00	0.00	0.00