
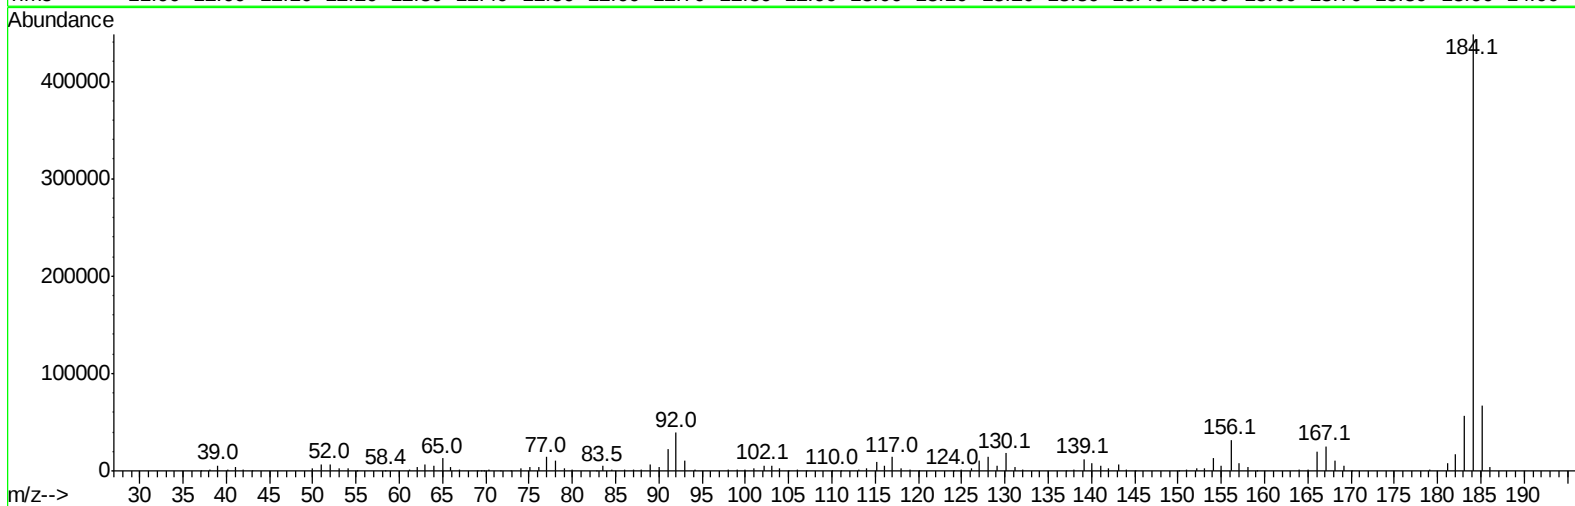


Data Path : Z:\HPCHEM1\BNA F\DATA\BF042617\
Data File : BF094639.D
Acq On : 26 Apr 2017 11:35
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 08:19:20 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

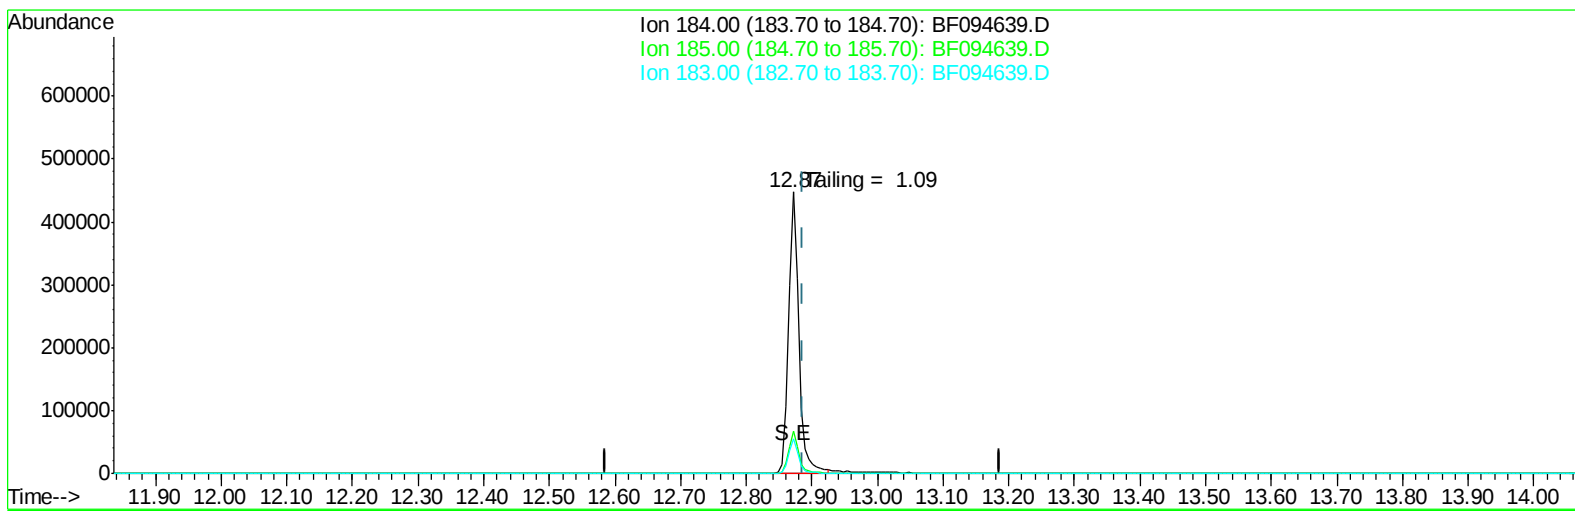

TIC: BF094639.D

(76) Benzidine



12.872min (-0.014) 30329.22ng

response 505946

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	15.07#
183.00	12.20	12.50
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042617\
Data File : BF094639.D
Acq On : 26 Apr 2017 11:35
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 08:19:20 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

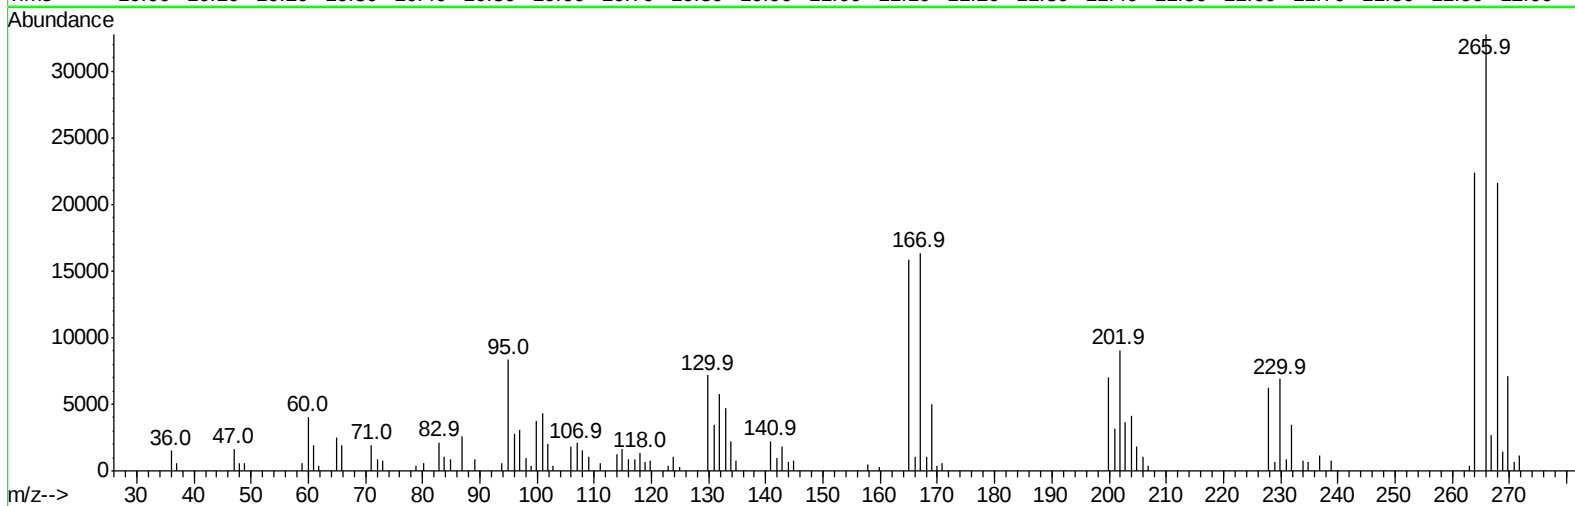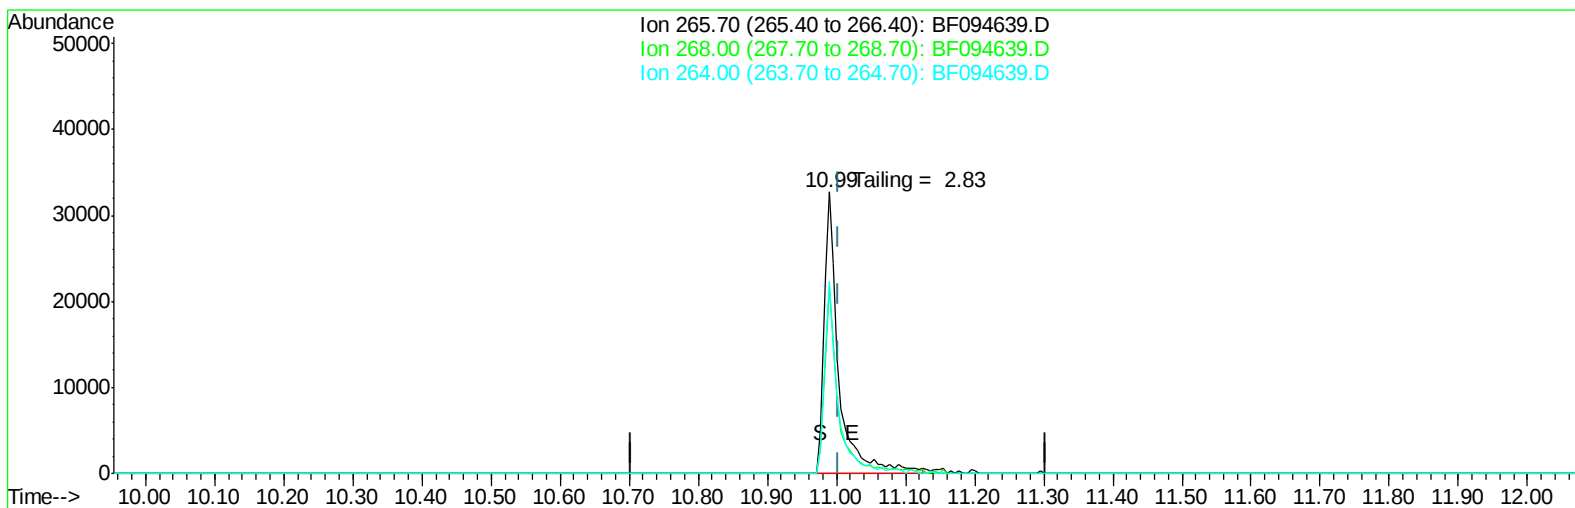

TIC: BF094639.D

(69) Pentachlorophenol (C)

10.989min (-0.014) 20945.81ng m

response 47939

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.12
264.00	64.60	68.20
0.00	0.00	0.00