


Data Path : Z:\HPCHEM1\BNA F\Data\BF042618\
Data File : BF104830.D
Acq On : 26 Apr 2018 11:41
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 25 14:01:50 2018

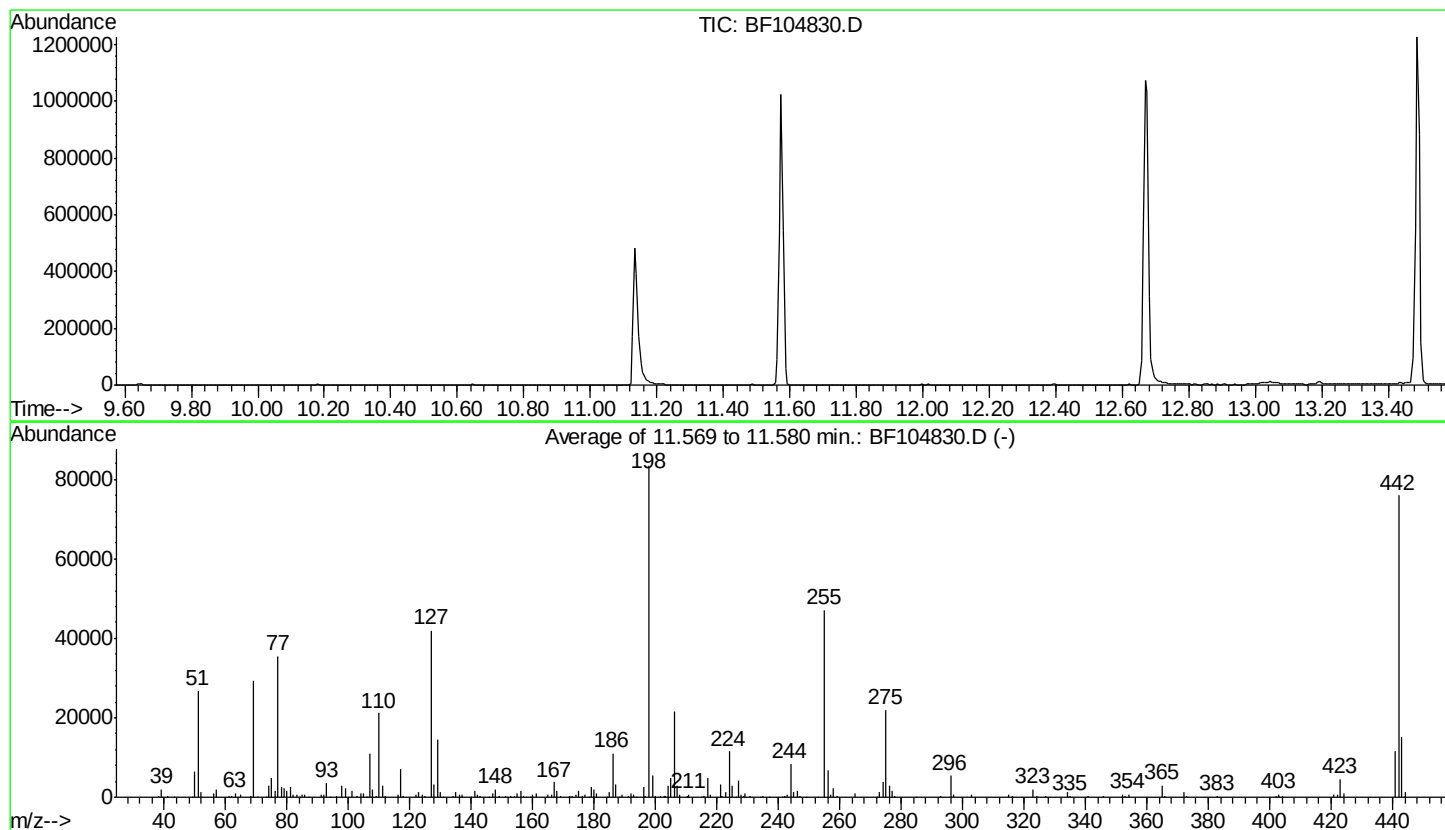

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	26874	PASS
68	69	0.00	2	1.6	457	PASS
69	198	0.00	100	35.3	29465	PASS
70	69	0.00	2	0.4	128	PASS
127	198	10	80	50.3	41936	PASS
197	198	0.00	2	0.2	194	PASS
198	198	100	100	100.0	83440	PASS
199	198	5	9	6.5	5452	PASS
275	198	10	60	26.3	21945	PASS
365	198	1	100	3.5	2946	PASS
441	443	0.01	100	77.1	11739	PASS
442	198	50	100	91.1	76002	PASS
443	442	15	24	20.0	15216	PASS