
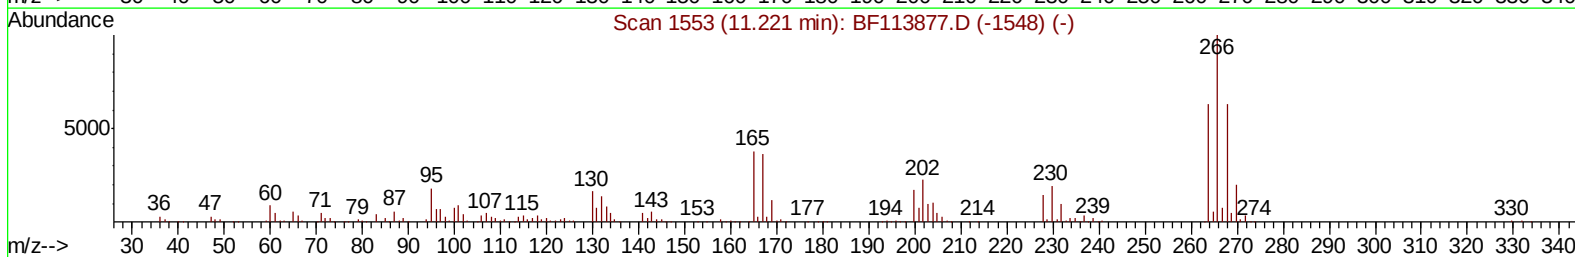
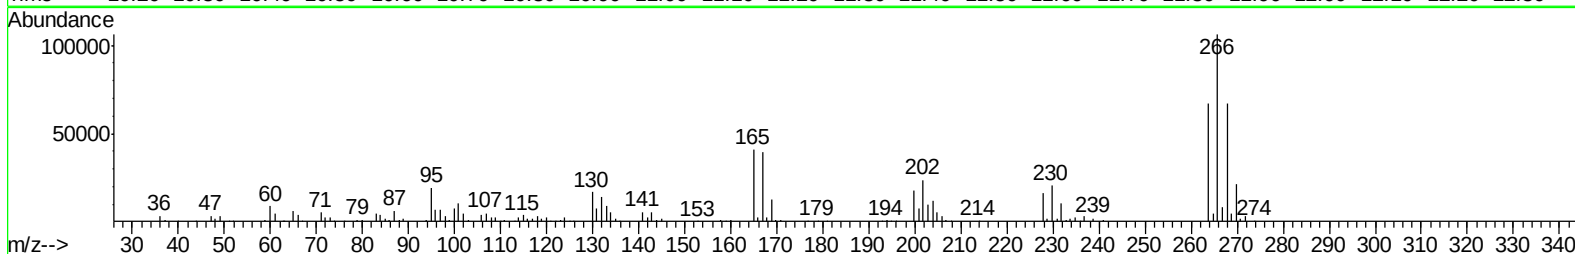


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042619\
Data File : BF113999.D
Acq On : 26 Apr 2019 9:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 06:26:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 23 03:32:35 2019
Response via : Initial Calibration

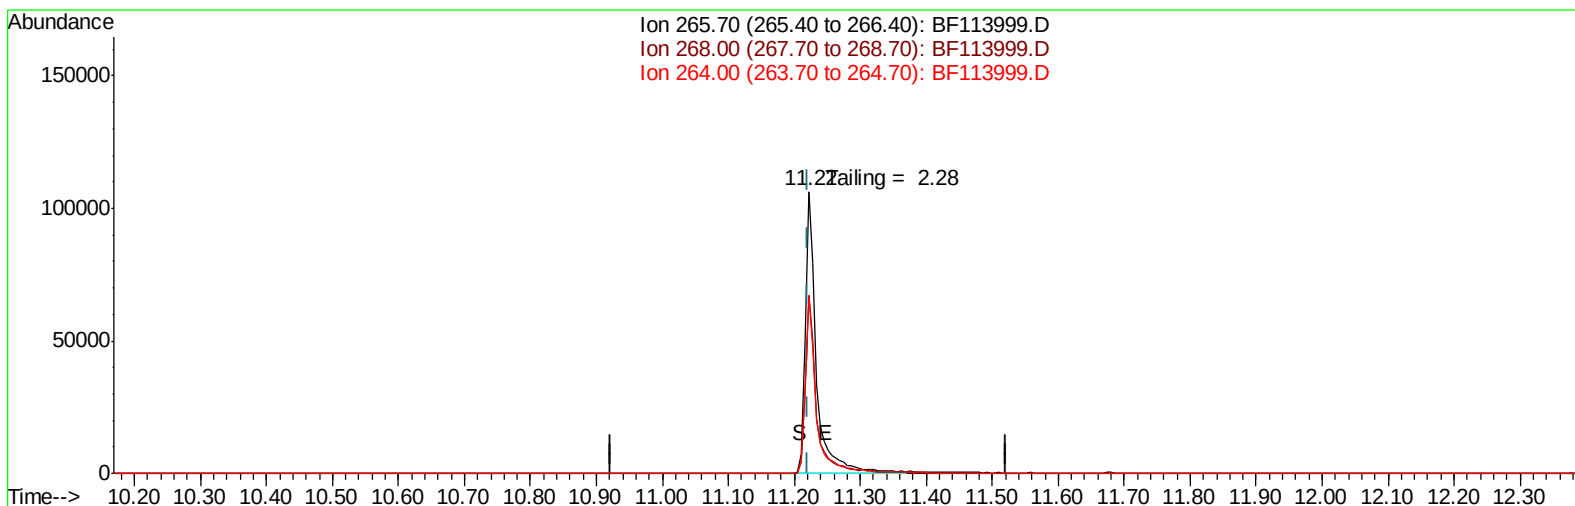

TIC: BF113999.D

(70) Pentachlorophenol (C)




11.221min (0.000) 55591.71ng

response 127441

Ion	Exp%	Act%
265.70	100	100
268.00	66.90	63.15
264.00	63.80	62.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042619\
 Data File : BF113999.D
 Acq On : 26 Apr 2019 9:52
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 06:26:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 23 03:32:35 2019
 Response via : Initial Calibration

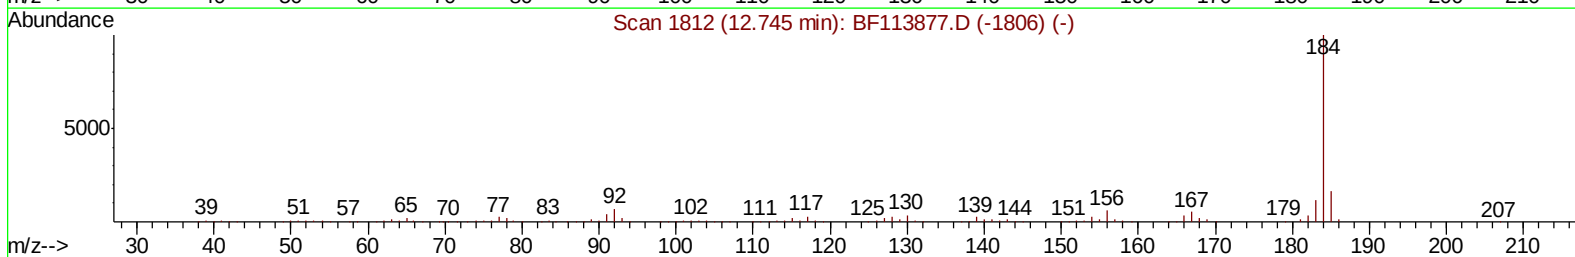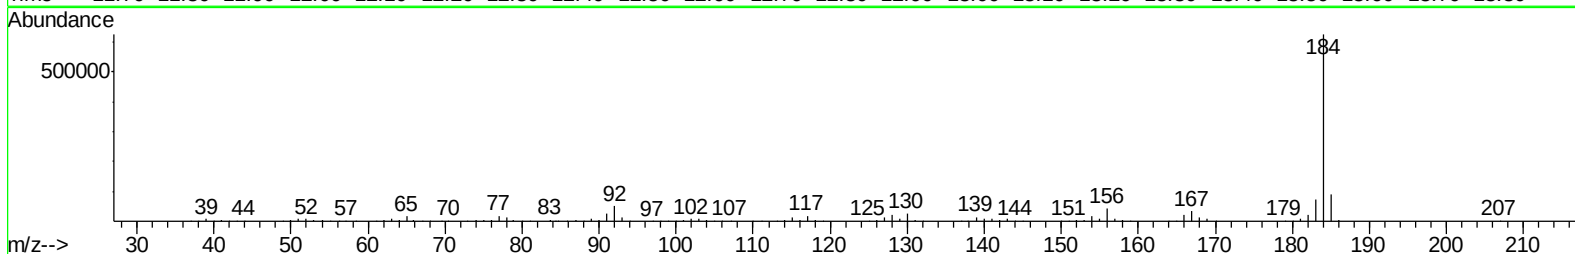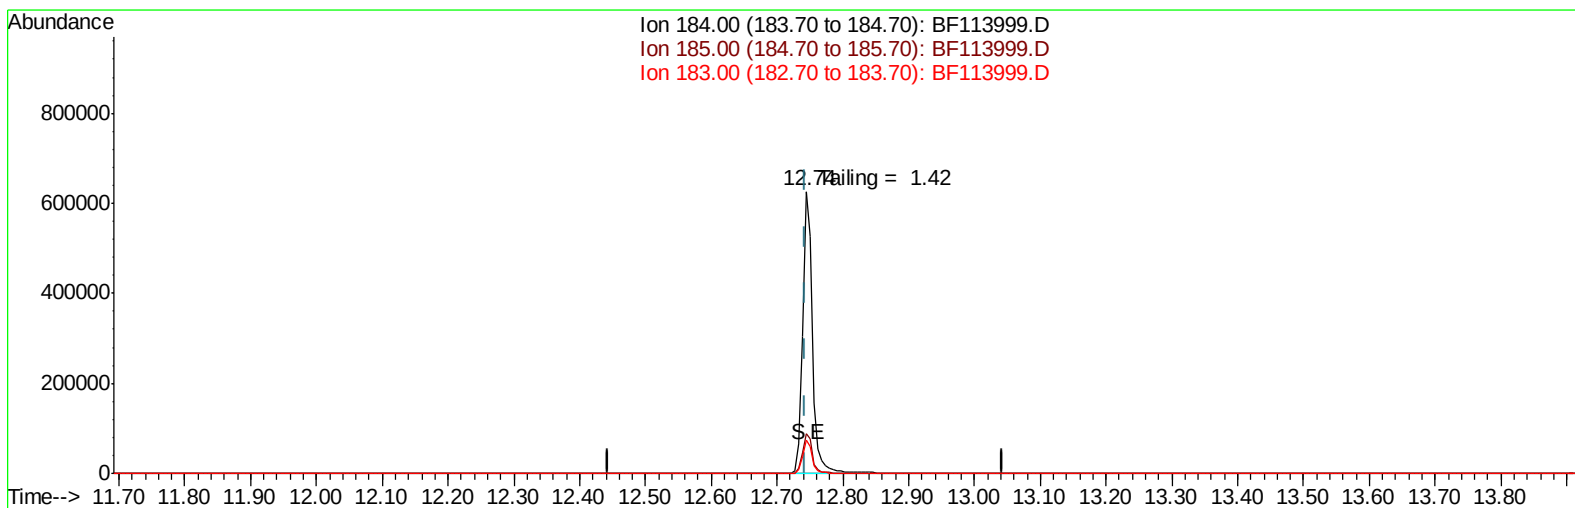

TIC: BF113999.D

(77) Benzidine

12.745min (+0.001) 0.00ng

response 650356

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.18
183.00	11.70	11.82
0.00	0.00	0.00