

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042619\
 Data File : BF114005.D
 Acq On : 26 Apr 2019 13:06
 Operator : JU/SJ
 Sample : PB119131BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB119131BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.534	580	586	589	rBV	2830531	2906783	60.70%	8.888%
2	6.528	748	755	757	rBV	2544183	2994784	62.54%	9.157%
3	6.669	774	779	782	rBV	3225726	3178568	66.37%	9.719%
4	6.892	814	817	821	rBV	953819	844696	17.64%	2.583%
5	7.051	840	844	848	rBV	2754596	2606096	54.42%	7.969%
6	7.451	906	912	915	rBV	1735368	1942107	40.55%	5.938%
7	8.175	1030	1035	1050	rBV	1092408	1083595	22.63%	3.313%
8	9.251	1212	1218	1221	rBV	4064017	4086657	85.33%	12.496%
9	9.933	1328	1334	1349	rBV	1289716	1340961	28.00%	4.100%
10	10.721	1462	1468	1501	rBV	2380155	2660426	55.55%	8.135%
11	11.415	1580	1586	1601	rBV	1572610	1501876	31.36%	4.592%
12	13.004	1851	1856	1859	rBV	4873421	4788972	100.00%	14.643%
13	14.057	2031	2035	2046	rBV	1411345	1408089	29.40%	4.305%
14	15.198	2225	2229	2234	rVB	49467	55019	1.15%	0.168%
15	15.551	2284	2289	2306	rBV	672932	1164608	24.32%	3.561%
16	16.033	2366	2371	2376	rBV	45887	68995	1.44%	0.211%
17	16.550	2453	2459	2467	rBV2	37099	72326	1.51%	0.221%


Sum of corrected areas: 32704558

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042619\
Data File : BF114005.D
Acq On : 26 Apr 2019 13:06
Operator : JU/SJ
Sample : PB119131BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB119131BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

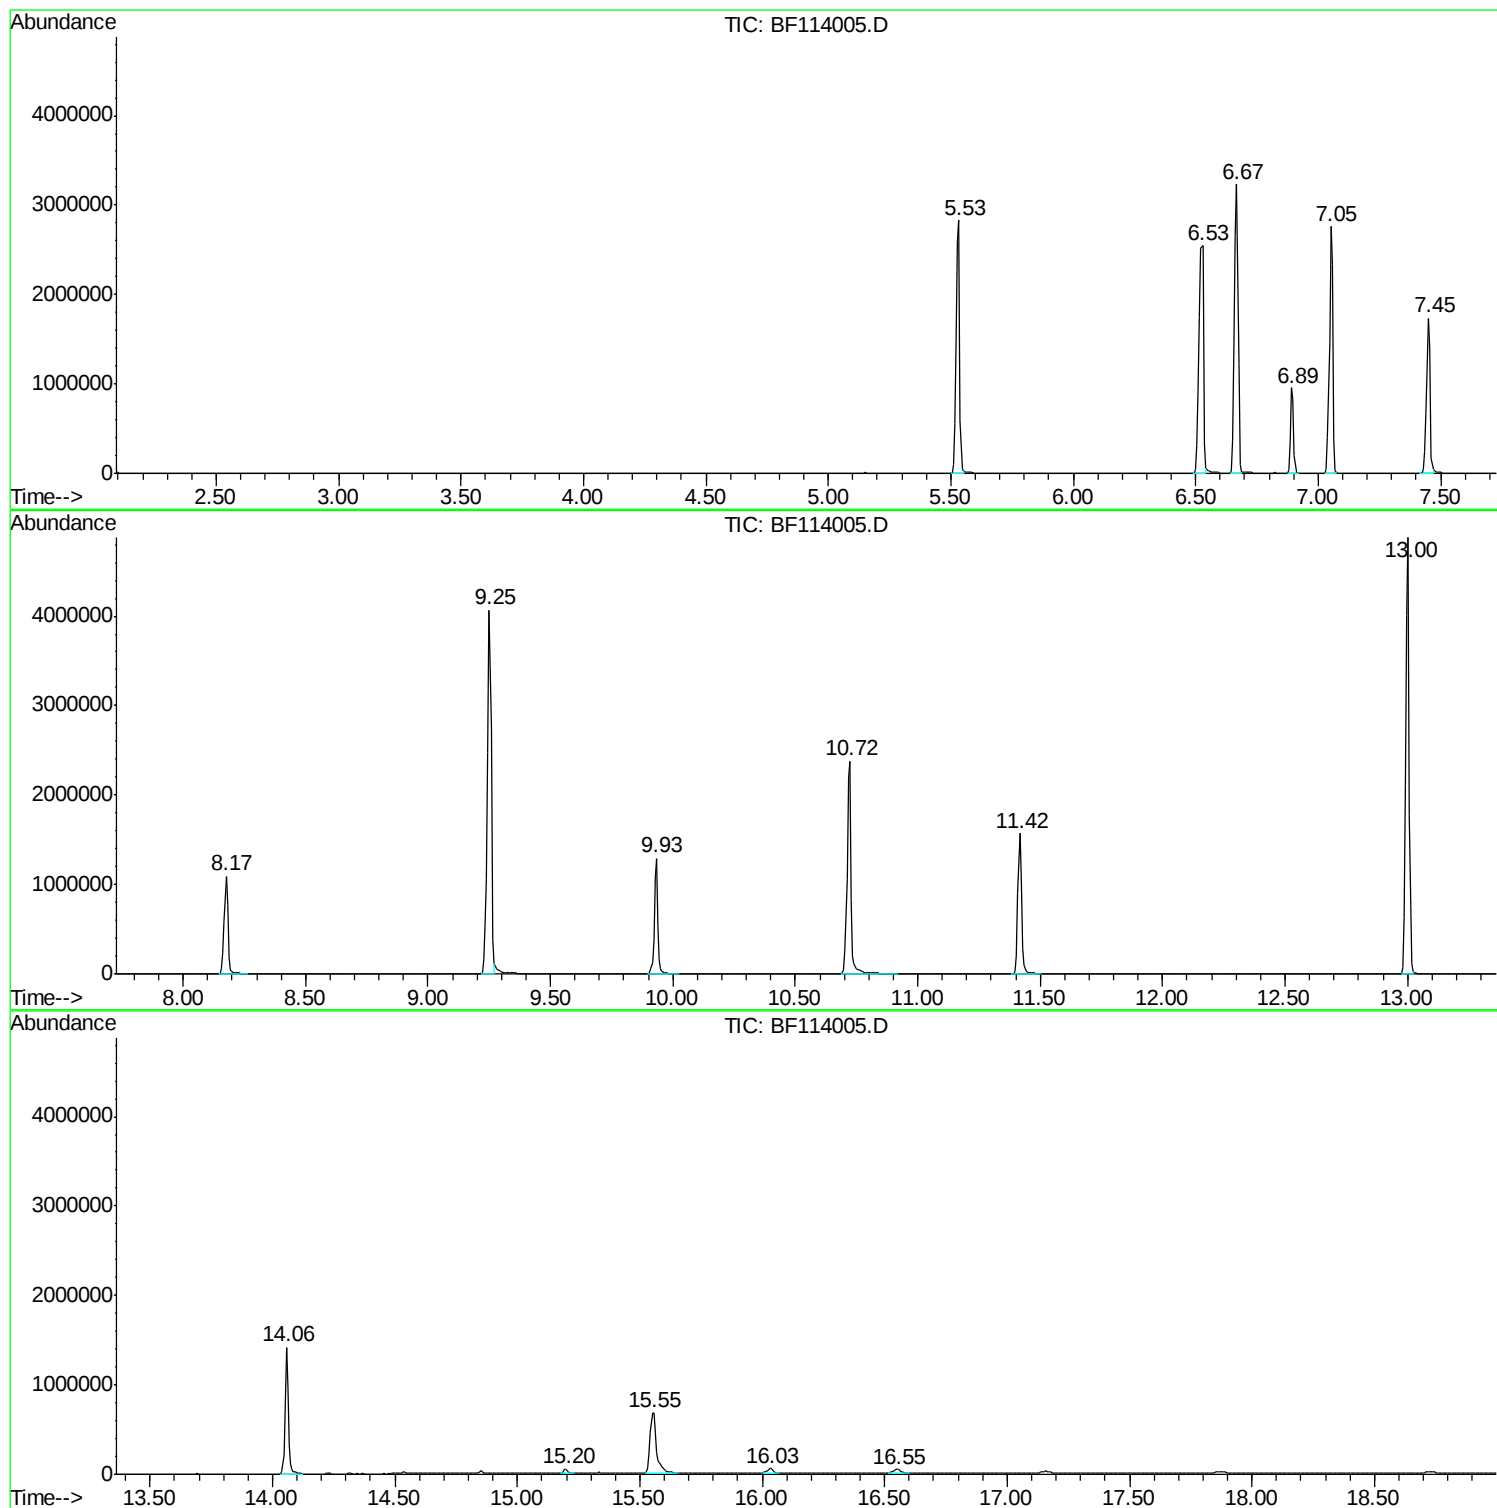

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042619\
Data File : BF114005.D
Acq On : 26 Apr 2019 13:06
Operator : JU/SJ
Sample : PB119131BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB119131BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.67 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.67	75.26 ng	3178570	1,4-Dichlorobenzene-d4	6.89

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
3		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
4		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

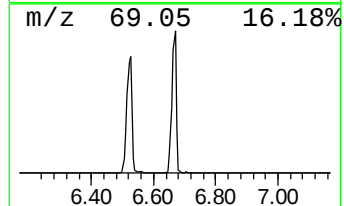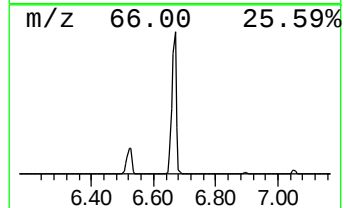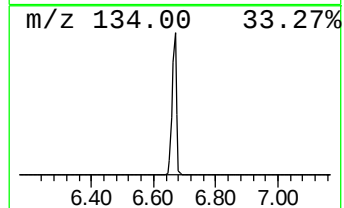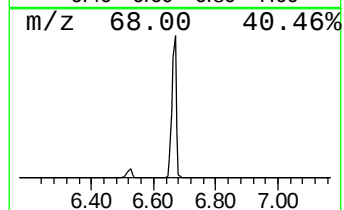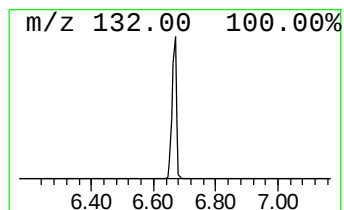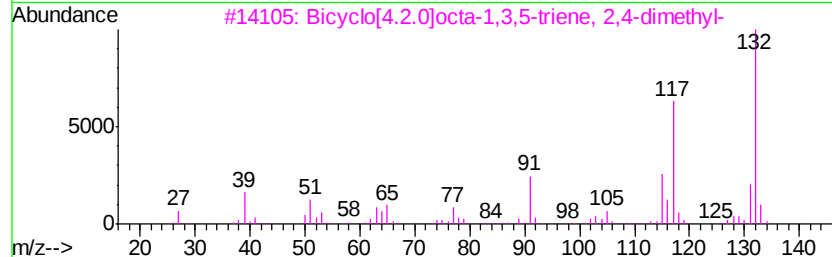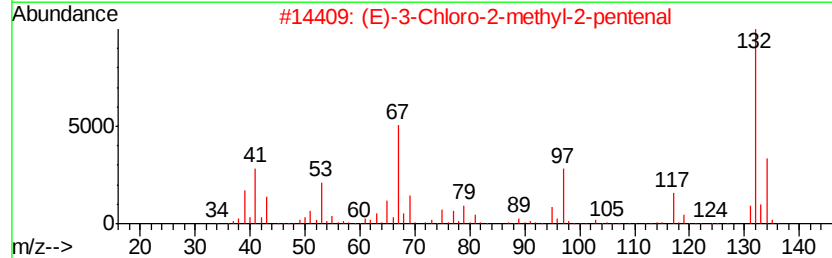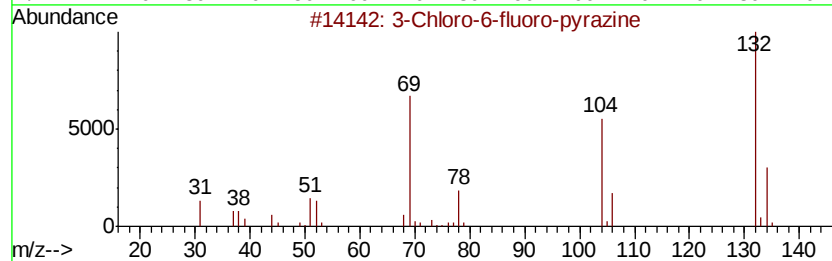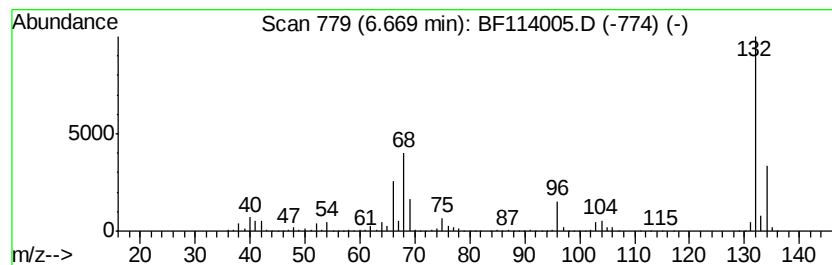

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042619\
Data File : BF114005.D
Acq On : 26 Apr 2019 13:06
Operator : JU/SJ
Sample : PB119131BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB119131BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.67	6.67	75.3	ng	3178570	1	6.89	844696	20.0