

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042619\
 Data File : BF114006.D
 Acq On : 26 Apr 2019 13:32
 Operator : JU/SJ
 Sample : PB119206BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB119206BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.534	580	586	589	rBV	3306000	3333575	59.94%	9.107%
2	6.528	748	755	758	rBV	3097650	3432215	61.71%	9.376%
3	6.669	774	779	782	rBV	3559438	3626724	65.21%	9.908%
4	6.893	813	817	821	rBV	958585	854429	15.36%	2.334%
5	7.051	840	844	848	rBV	3033656	2962915	53.28%	8.094%
6	7.451	906	912	916	rBV	1871153	2242354	40.32%	6.126%
7	8.175	1030	1035	1047	rBV	1043273	1093598	19.66%	2.988%
8	9.251	1212	1218	1221	rBV	4341572	4671887	84.01%	12.763%
9	9.933	1328	1334	1347	rBV	1281854	1360700	24.47%	3.717%
10	10.722	1461	1468	1492	rBV	2907303	3130234	56.28%	8.552%
11	11.416	1580	1586	1594	rBV	1603132	1533339	27.57%	4.189%
12	13.004	1848	1856	1859	rBV	5345771	5561405	100.00%	15.193%
13	14.057	2030	2035	2048	rBV	1522821	1513356	27.21%	4.134%
14	15.545	2282	2288	2305	rBV	795587	1287740	23.15%	3.518%


Sum of corrected areas: 36604471

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042619\
Data File : BF114006.D
Acq On : 26 Apr 2019 13:32
Operator : JU/SJ
Sample : PB119206BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB119206BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

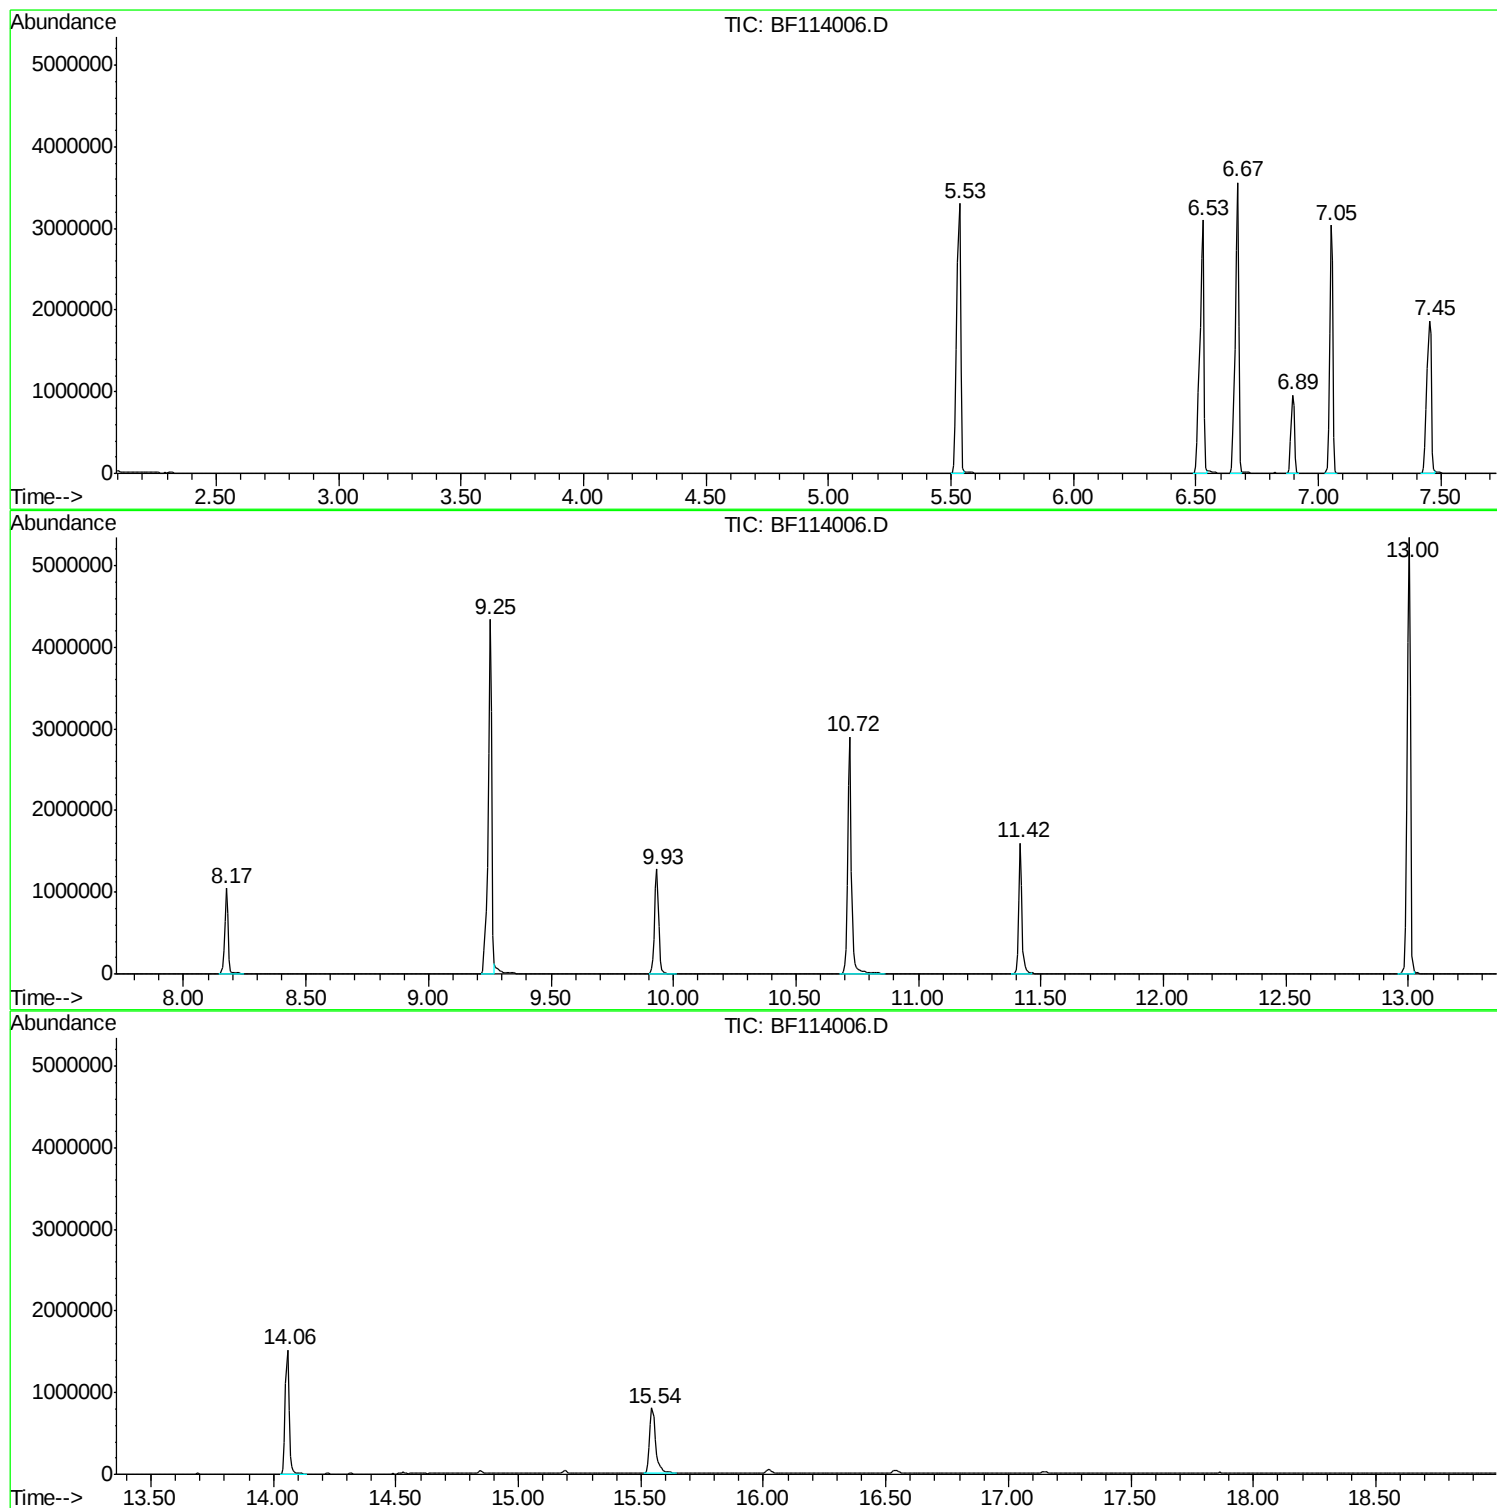

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042619\
Data File : BF114006.D
Acq On : 26 Apr 2019 13:32
Operator : JU/SJ
Sample : PB119206BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB119206BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.67 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.67	84.89 ng	3626720	1,4-Dichlorobenzene-d4	6.89

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
3		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

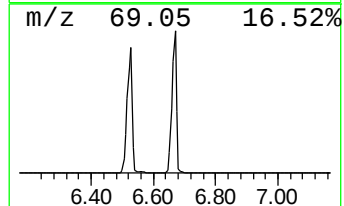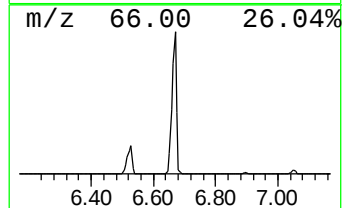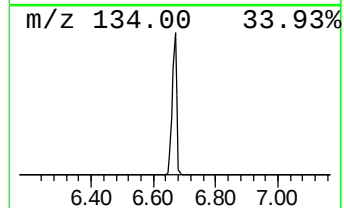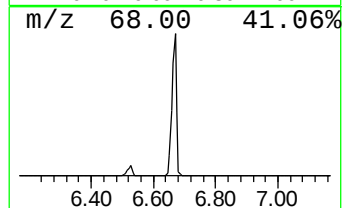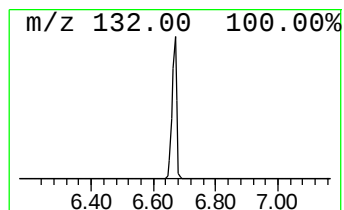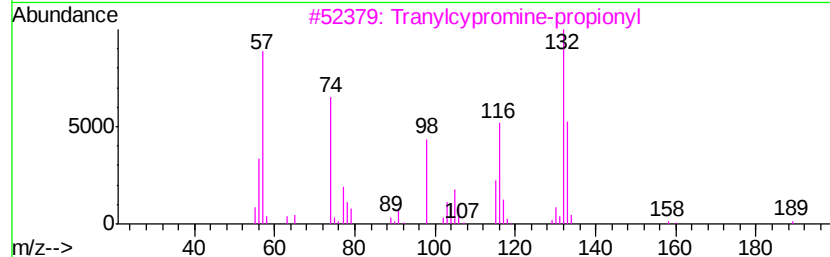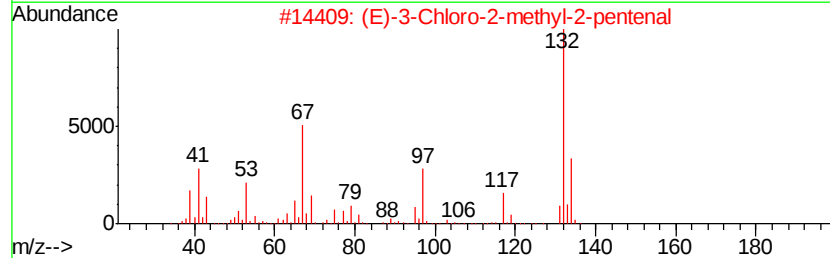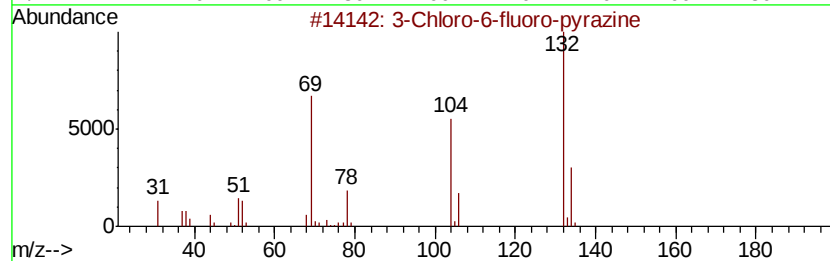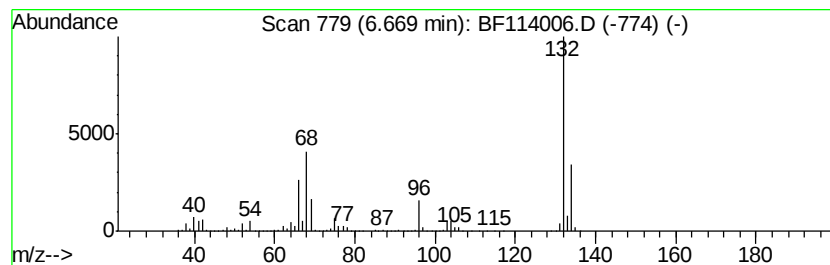

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042619\
Data File : BF114006.D
Acq On : 26 Apr 2019 13:32
Operator : JU/SJ
Sample : PB119206BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB119206BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.67	6.67	84.9	ng	3626720	1	6.89	854429	20.0