
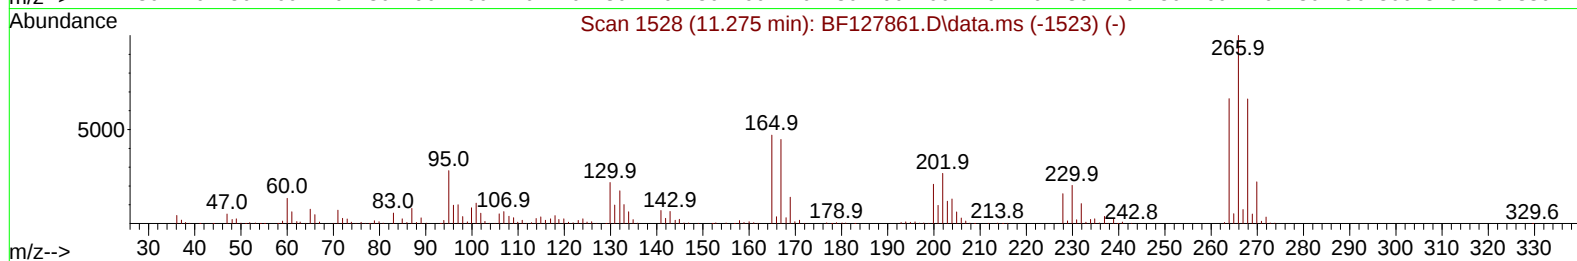
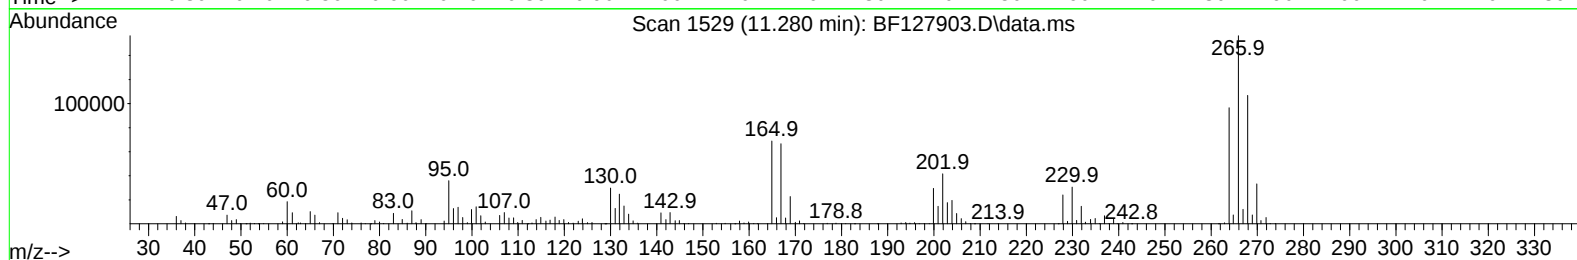


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\
Data File : BF127903.D
Acq On : 26 Apr 2022 09:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 05:38:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 00:43:03 2022
Response via : Initial Calibration

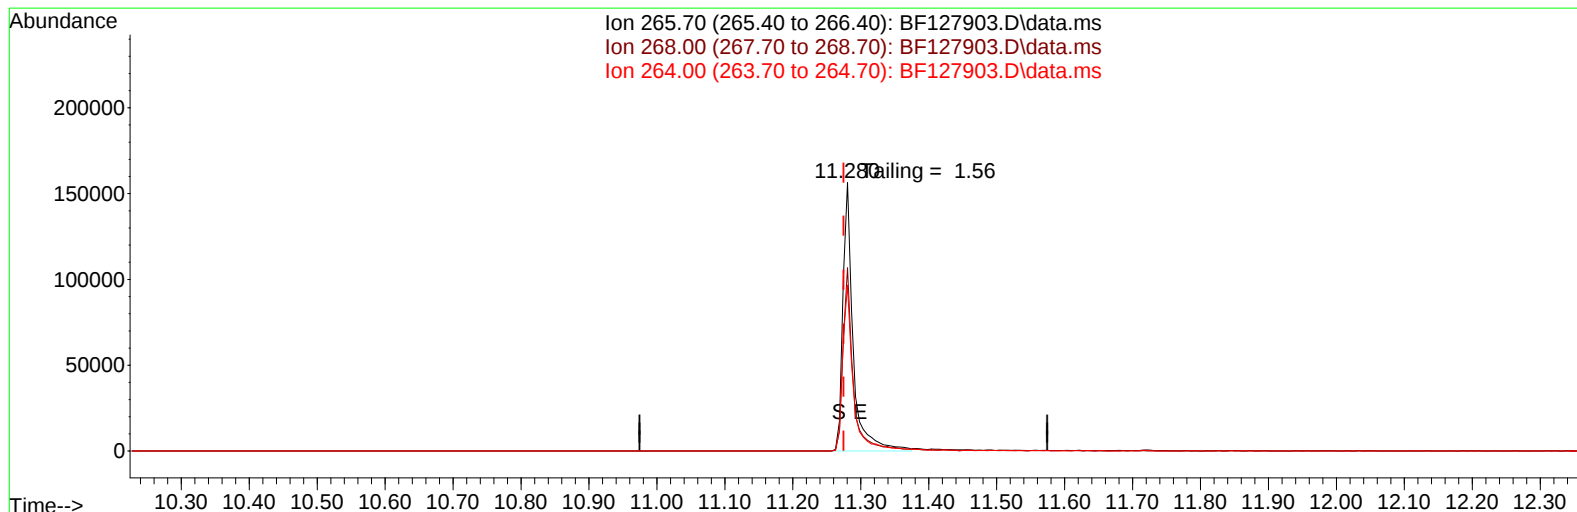

TIC: BF127903.D\data.ms

(70) Pentachlorophenol (C)




11.280min (+ 0.006) 361396.70 ng

response 163892

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	68.26
264.00	66.40	61.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\
Data File : BF127903.D
Acq On : 26 Apr 2022 09:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 05:38:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 00:43:03 2022
Response via : Initial Calibration

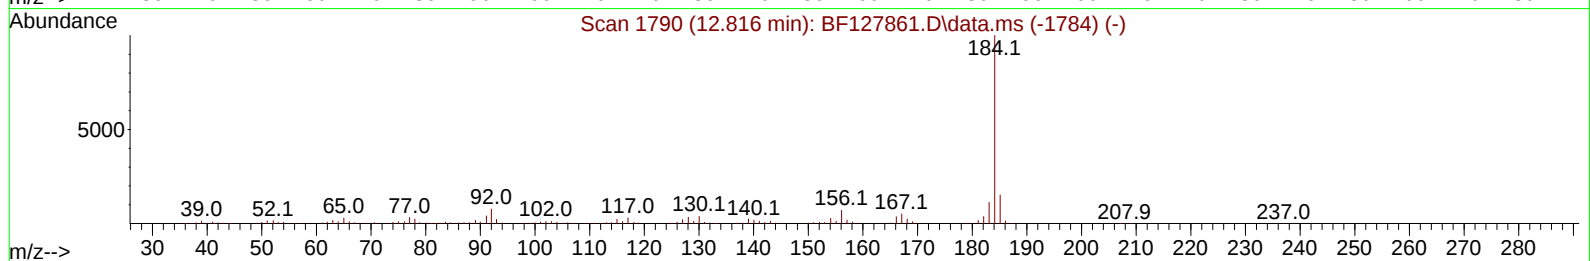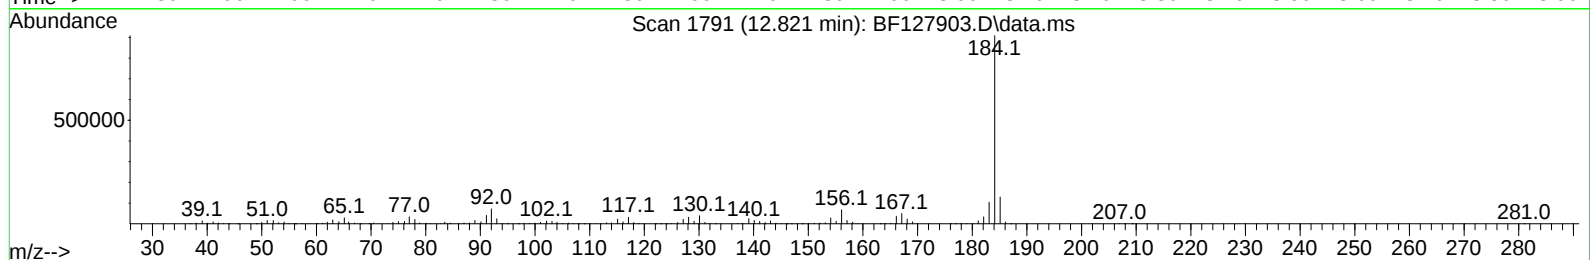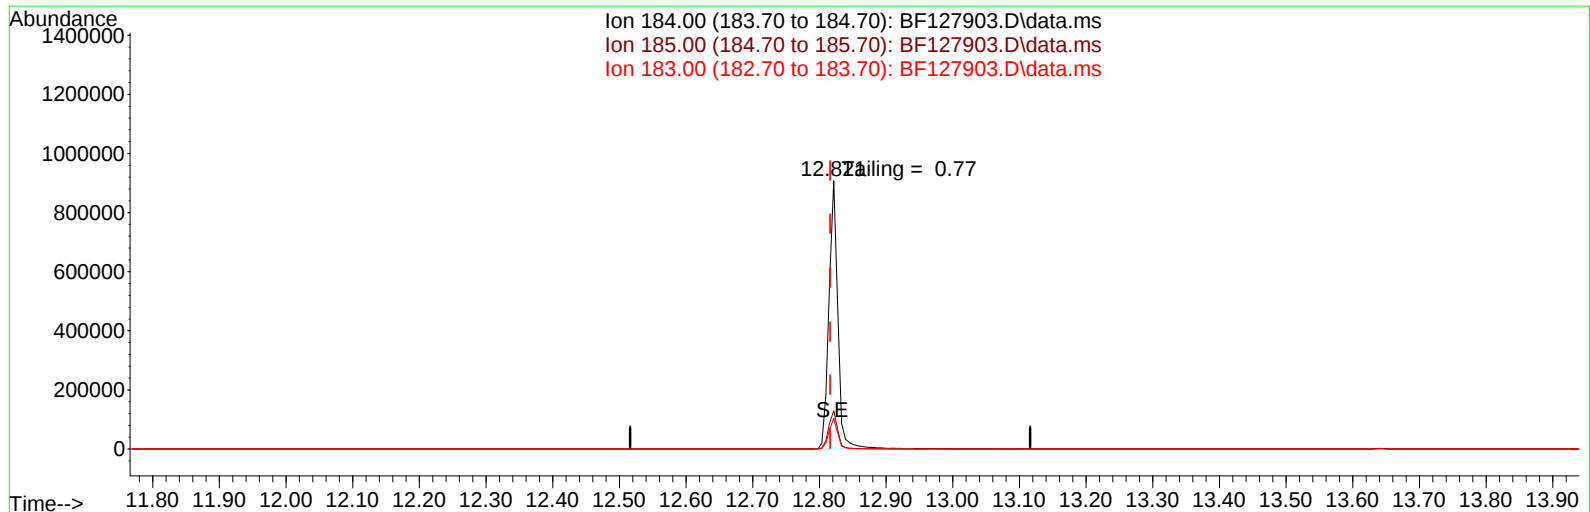

TIC: BF127903.D\data.ms

(77) Benzidine**12.821min (+ 0.005) 196990.64 ng****response 849835**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.26
183.00	11.20	11.47
0.00	0.00	0.00