
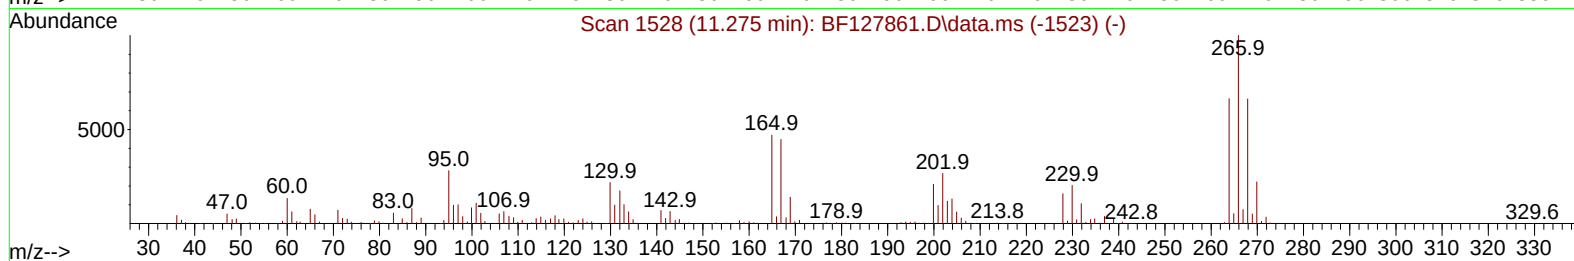
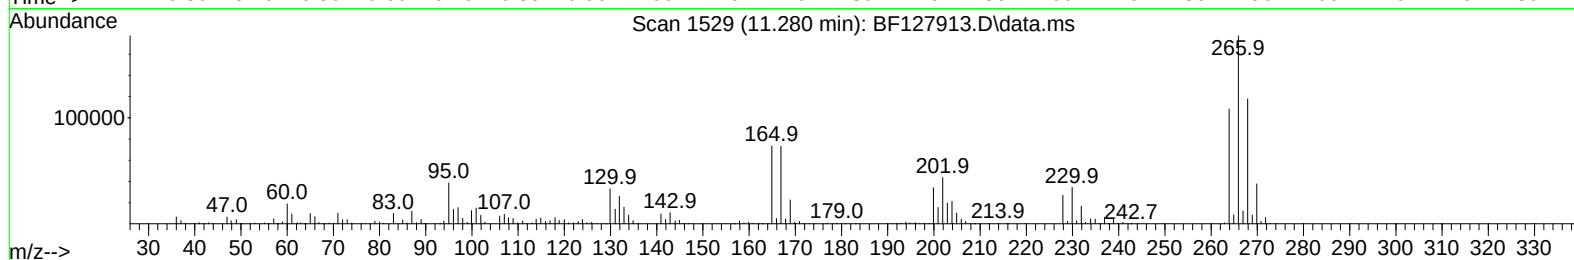


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\
Data File : BF127913.D
Acq On : 26 Apr 2022 15:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 05:42:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 00:43:03 2022
Response via : Initial Calibration

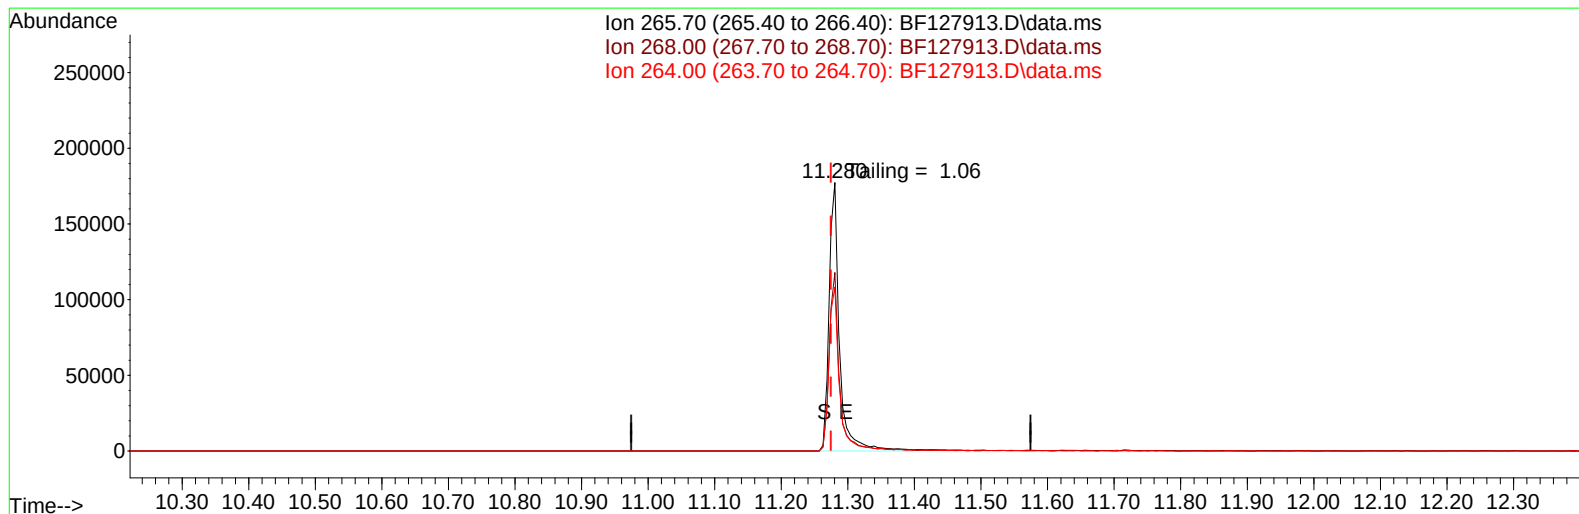

TIC: BF127913.D\data.ms

(70) Pentachlorophenol (C)




11.280min (+ 0.006) 471509.88 ng

response 194389

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	66.51
264.00	66.40	61.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\
 Data File : BF127913.D
 Acq On : 26 Apr 2022 15:11
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 05:42:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Apr 24 00:43:03 2022
 Response via : Initial Calibration

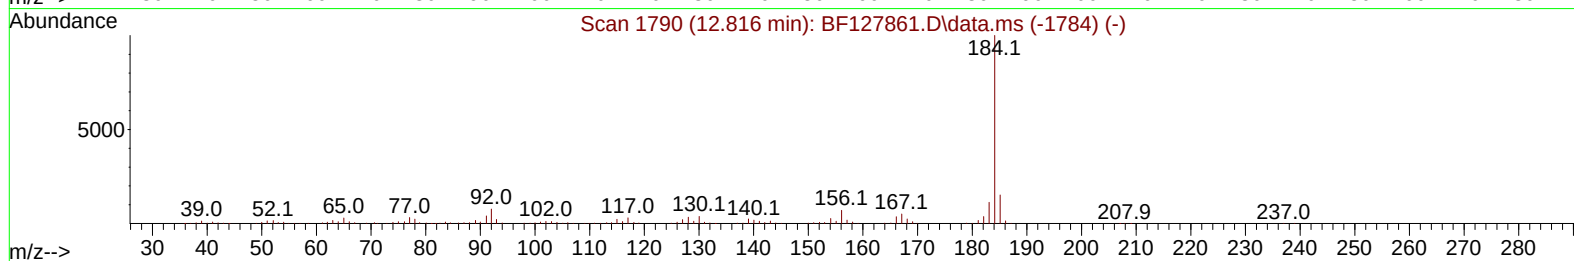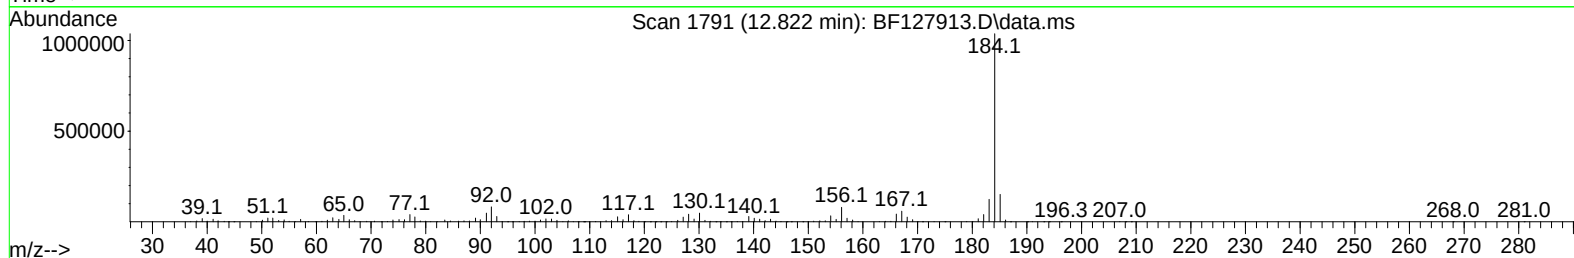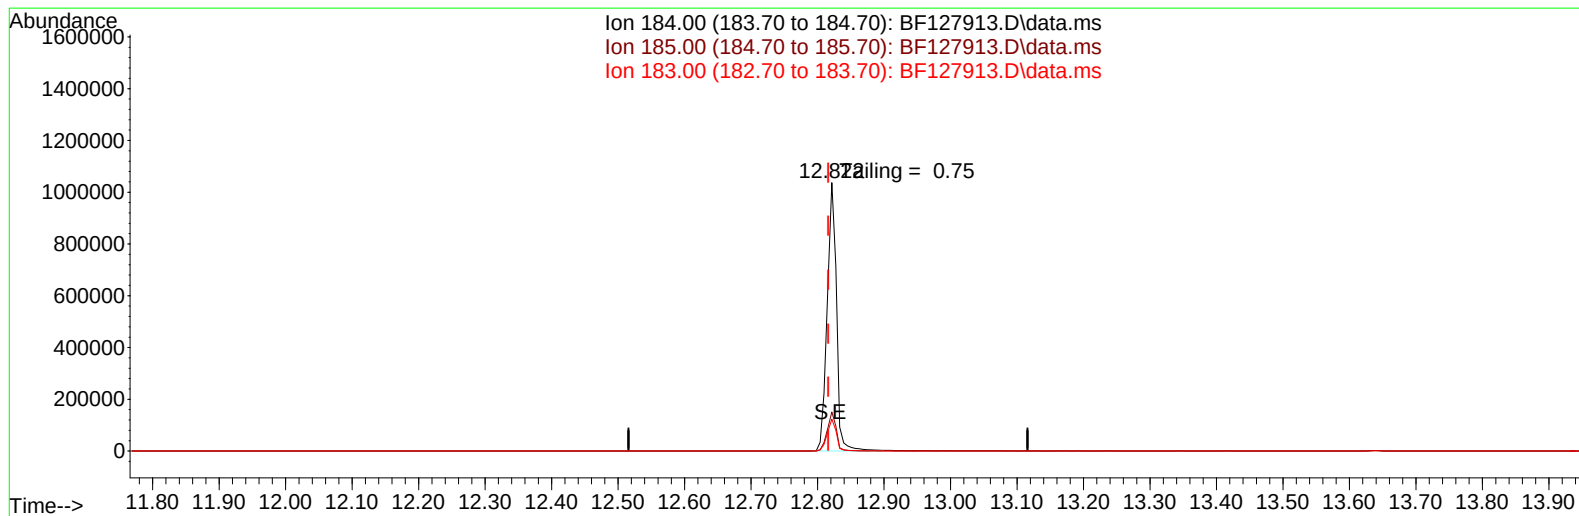

TIC: BF127913.D\data.ms

(77) Benzidine**12.822min (+ 0.006) 192128.30 ng****response 1014261**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.57
183.00	11.20	11.89
0.00	0.00	0.00