

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\
 Data File : BF127905.D
 Acq On : 26 Apr 2022 10:21
 Operator : CG\JU
 Sample : PB144215BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144215BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127905.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.122	307	312	317	rVB	88371	106873	1.82%	0.317%
2	5.204	492	496	503	rBV	49033	59450	1.01%	0.177%
3	5.581	555	560	563	rBV	3250348	3303332	56.31%	9.808%
4	6.569	722	728	731	rBV	3163925	3385413	57.71%	10.052%
5	6.939	788	791	795	rVB	1225860	1098269	18.72%	3.261%
6	7.510	881	888	891	rBV	2775104	3387862	57.75%	10.059%
7	8.228	1004	1010	1013	rBV	1378135	1516076	25.84%	4.501%
8	9.304	1186	1193	1196	rBV	5195832	5866293	100.00%	17.418%
9	9.986	1302	1309	1312	rBV	1878381	1807181	30.81%	5.366%
10	10.780	1437	1444	1465	rBV	2334837	2617966	44.63%	7.773%
11	11.480	1556	1563	1566	rBV	2061500	1849803	31.53%	5.492%
12	13.068	1828	1833	1837	rBV	5218696	5669445	96.64%	16.833%
13	14.127	2009	2013	2016	rBV	1586387	1429945	24.38%	4.246%
14	14.215	2023	2028	2033	rBV	49870	70508	1.20%	0.209%
15	15.251	2201	2204	2208	rVB	54942	67328	1.15%	0.200%
16	15.645	2265	2271	2282	rBV2	883449	1264085	21.55%	3.753%
17	16.115	2347	2351	2357	rVB	60330	89163	1.52%	0.265%
18	16.651	2438	2442	2451	rVB	47643	91454	1.56%	0.272%




Sum of corrected areas: 33680446

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\
Data File : BF127905.D
Acq On : 26 Apr 2022 10:21
Operator : CG\JU
Sample : PB144215BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144215BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

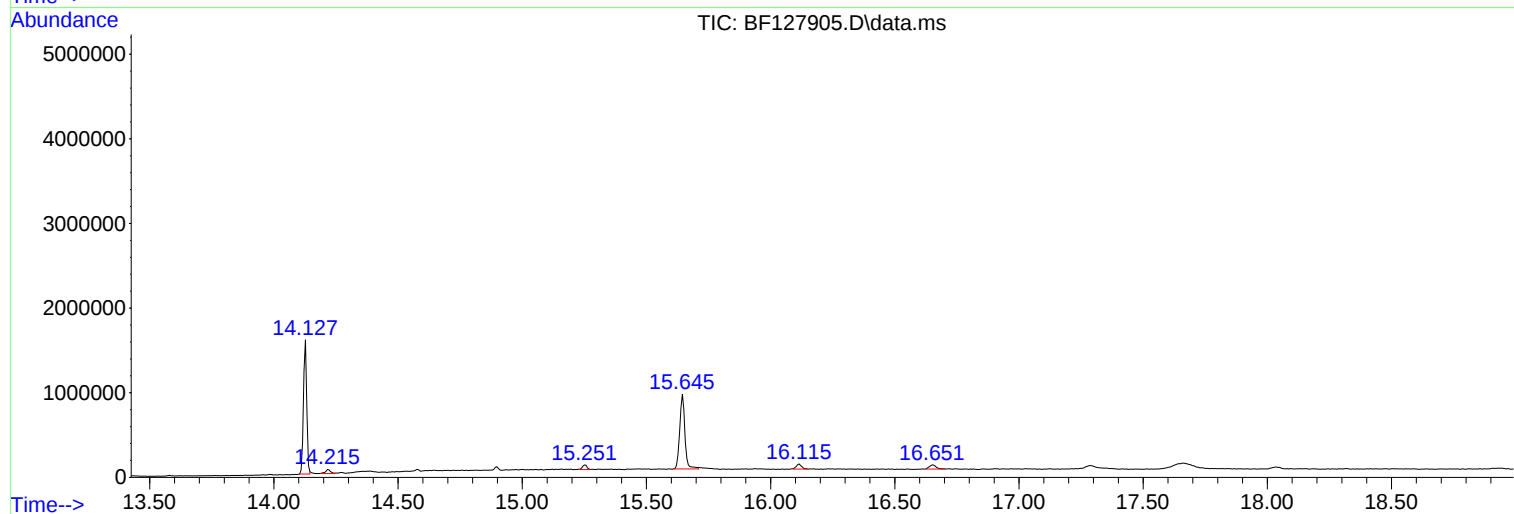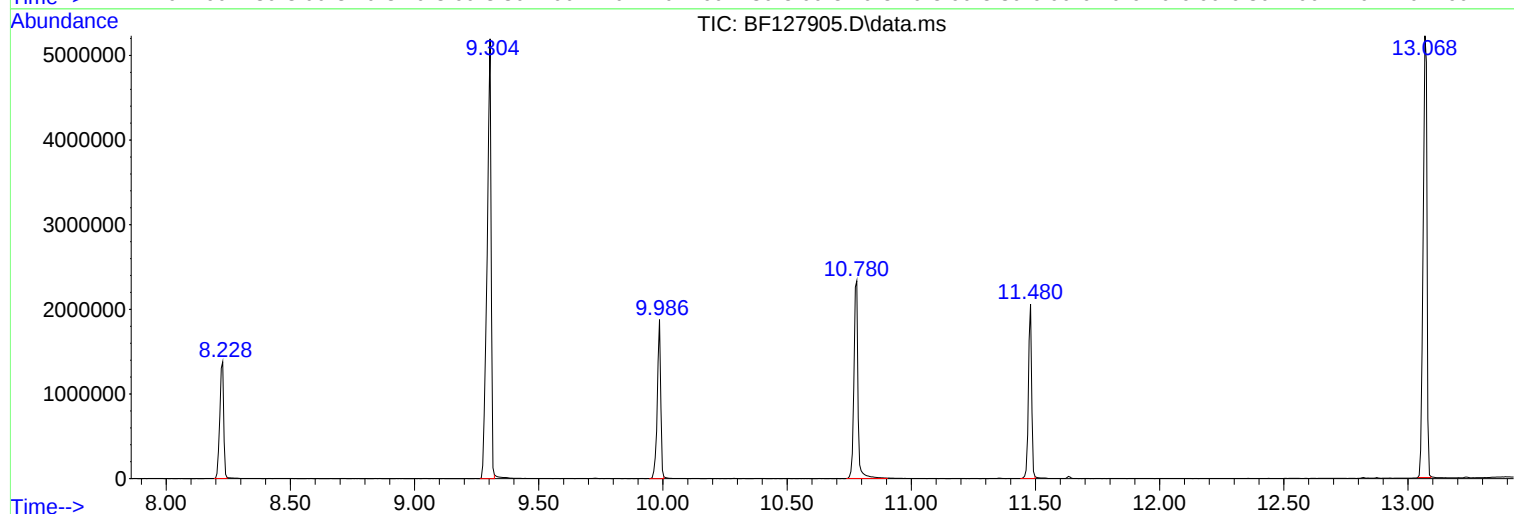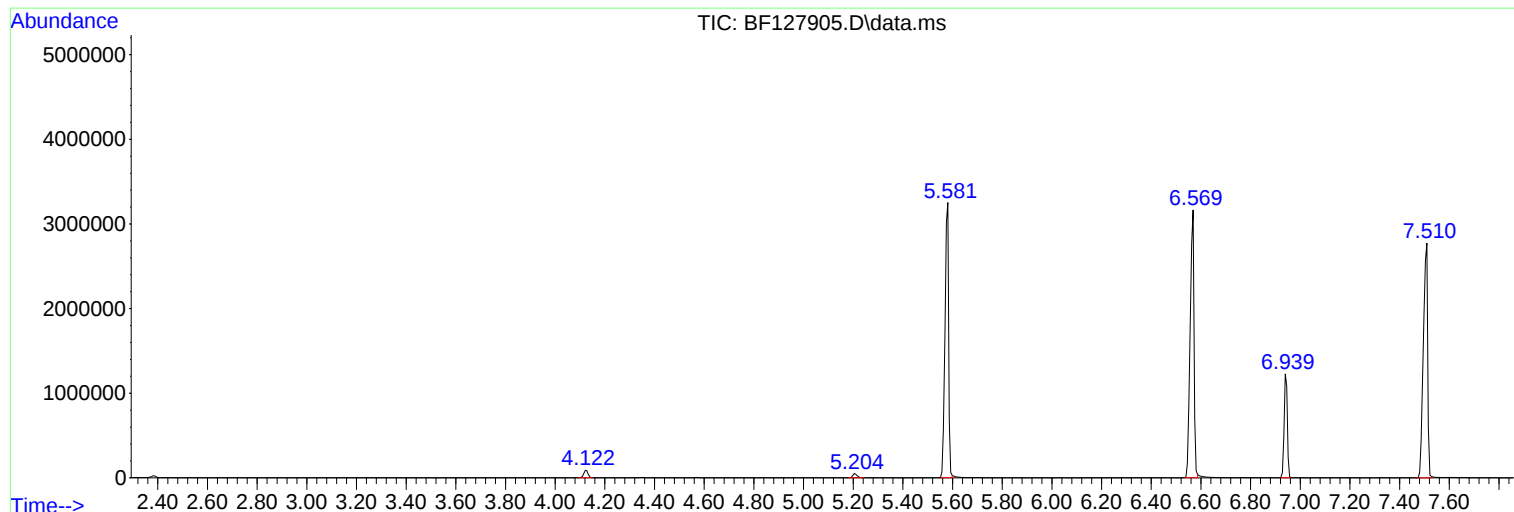

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\
Data File : BF127905.D
Acq On : 26 Apr 2022 10:21
Operator : CG\JU
Sample : PB144215BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144215BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\
Data File : BF127905.D
Acq On : 26 Apr 2022 10:21
Operator : CG\JU
Sample : PB144215BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144215BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------