

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\
 Data File : BF127915.D
 Acq On : 26 Apr 2022 16:08
 Operator : CG\JU
 Sample : PB144337BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144337BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127915.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.581	554	560	563	rBV	4210669	4667854	73.63%	12.475%
2	6.575	722	729	732	rBV	3924497	4796227	75.65%	12.819%
3	6.939	787	791	795	rBV	1237631	1034465	16.32%	2.765%
4	7.510	881	888	891	rBV	2811921	3374909	53.23%	9.020%
5	8.222	1004	1009	1013	rBV	1357775	1370207	21.61%	3.662%
6	9.304	1186	1193	1196	rBV	5276446	5787445	91.29%	15.468%
7	9.986	1303	1309	1312	rBV	1639894	1632486	25.75%	4.363%
8	10.780	1437	1444	1447	rBV	3579022	3715134	58.60%	9.929%
9	11.474	1556	1562	1566	rBV	1785568	1766999	27.87%	4.723%
10	13.069	1828	1833	1836	rBV	5580123	6339846	100.00%	16.944%
11	14.121	2008	2012	2016	rBV	1602473	1580557	24.93%	4.224%
12	15.645	2265	2271	2279	rBV	921049	1350178	21.30%	3.609%




Sum of corrected areas: 37416307

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\
Data File : BF127915.D
Acq On : 26 Apr 2022 16:08
Operator : CG\JU
Sample : PB144337BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144337BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

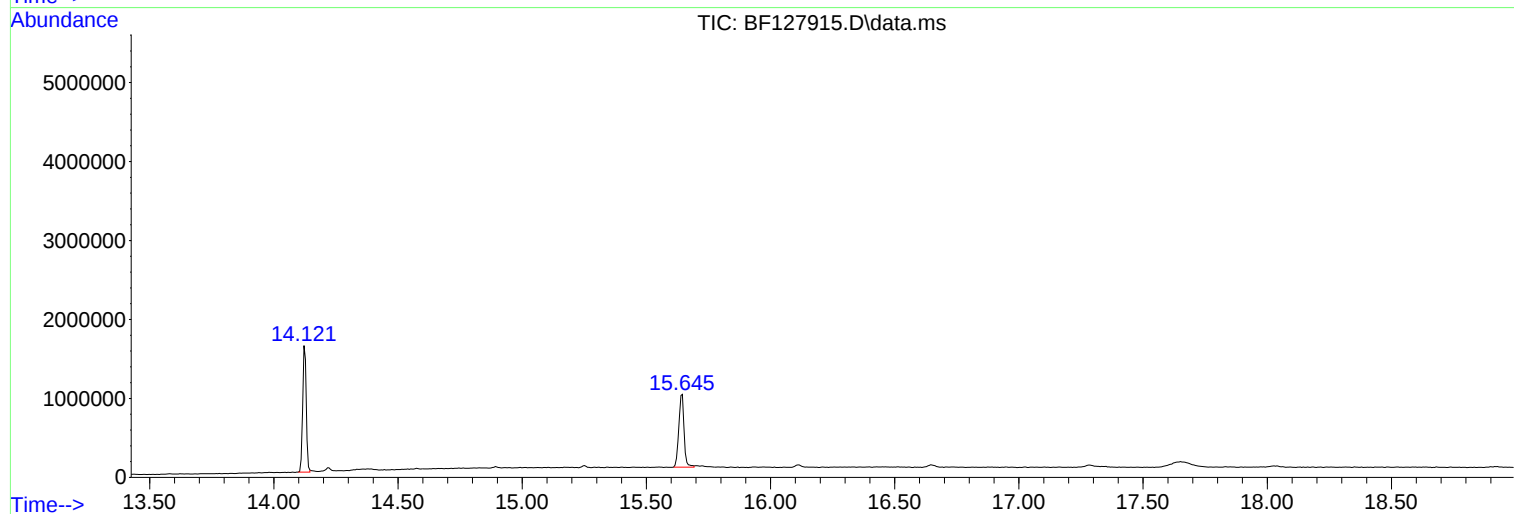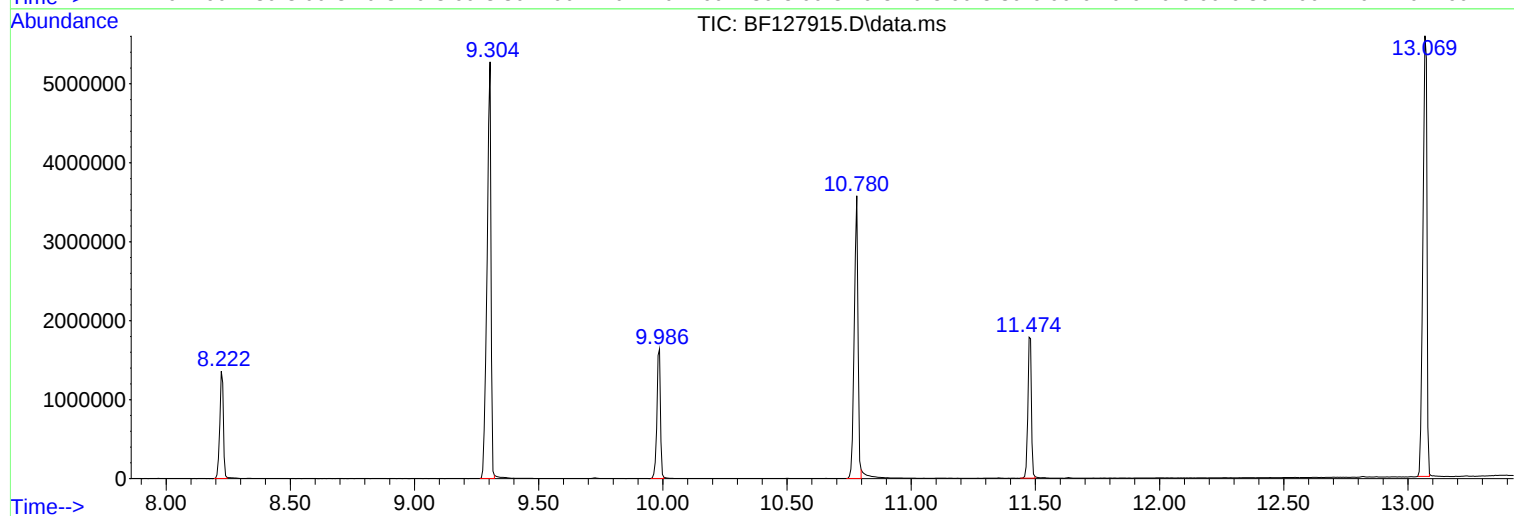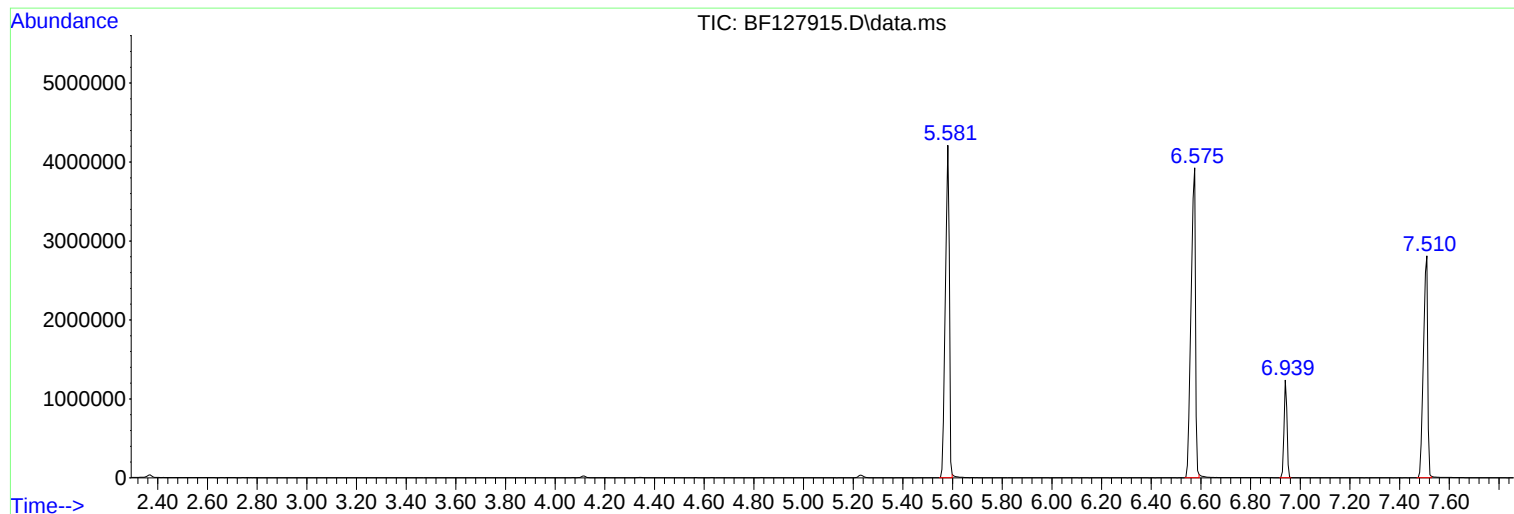

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\
Data File : BF127915.D
Acq On : 26 Apr 2022 16:08
Operator : CG\JU
Sample : PB144337BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144337BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\
Data File : BF127915.D
Acq On : 26 Apr 2022 16:08
Operator : CG\JU
Sample : PB144337BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144337BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------