

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\
 Data File : BF127928.D
 Acq On : 26 Apr 2022 22:36
 Operator : CG\JU
 Sample : N2551-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 20220376-096-21-02-ELUTRIATE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127928.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.557	552	556	563	rBV	1311830	1148376	37.05%	5.363%
2	6.557	722	726	733	rBV	938476	836831	27.00%	3.908%
3	6.940	787	791	795	rBV	1091577	884937	28.55%	4.133%
4	7.504	879	887	890	rBV	1867943	1736897	56.03%	8.111%
5	7.610	901	905	912	rVV	39995	42715	1.38%	0.199%
6	7.669	912	915	919	rVB	108191	91562	2.95%	0.428%
7	8.222	1005	1009	1013	rBV	1316446	1144268	36.91%	5.344%
8	8.804	1103	1108	1112	rBV	75300	84416	2.72%	0.394%
9	9.298	1187	1192	1195	rBV	3452449	3011562	97.15%	14.064%
10	9.369	1200	1204	1207	rVB	132287	111385	3.59%	0.520%
11	9.981	1302	1308	1312	rBV	1513216	1362080	43.94%	6.361%
12	10.775	1438	1443	1450	rBV	1907533	1809866	58.39%	8.452%
13	11.475	1558	1562	1572	rBV	1566147	1324279	42.72%	6.184%
14	11.633	1585	1589	1592	rBV	3570712	3099824	100.00%	14.476%
15	11.851	1624	1626	1630	rVB	67702	57487	1.85%	0.268%
16	11.986	1646	1649	1654	rBV	196421	188484	6.08%	0.880%
17	12.610	1750	1755	1759	rBV5	17260	35482	1.14%	0.166%
18	12.710	1766	1772	1775	rBV	46198	47594	1.54%	0.222%
19	13.057	1827	1831	1835	rBV	1861661	1651873	53.29%	7.714%
20	14.027	1990	1996	2008	rBV5	253114	844920	27.26%	3.946%
21	14.121	2008	2012	2021	rVV	812555	830792	26.80%	3.880%
22	14.216	2024	2028	2033	rBV	41770	50183	1.62%	0.234%
23	14.886	2138	2142	2147	rBV7	24403	47041	1.52%	0.220%
24	14.968	2153	2156	2161	rVB	108930	114689	3.70%	0.536%
25	15.633	2264	2269	2277	rBV2	631839	856022	27.62%	3.998%




Sum of corrected areas: 21413565

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\
Data File : BF127928.D
Acq On : 26 Apr 2022 22:36
Operator : CG\JU
Sample : N2551-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20220376-096-21-02-ELUTRIATE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

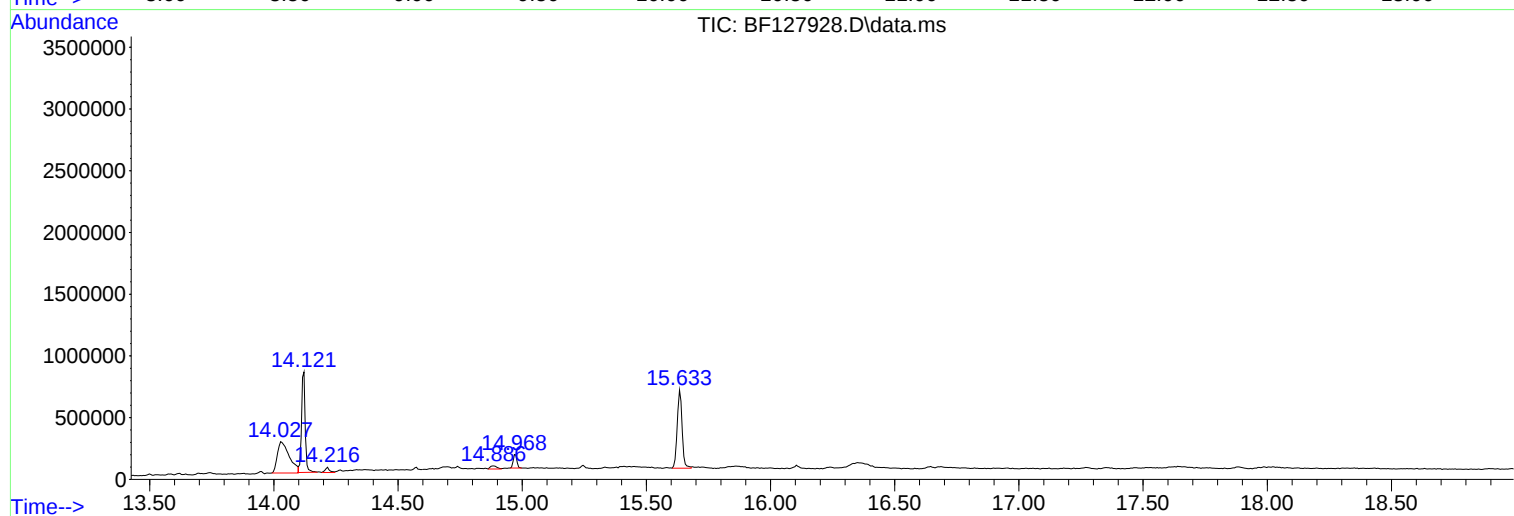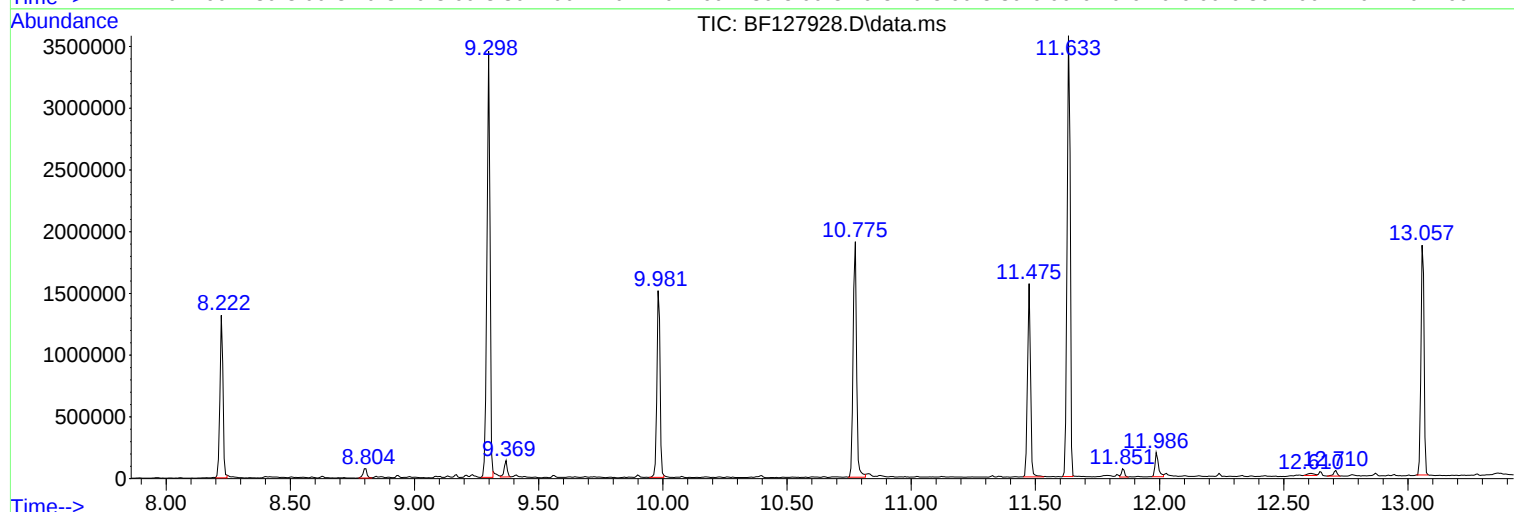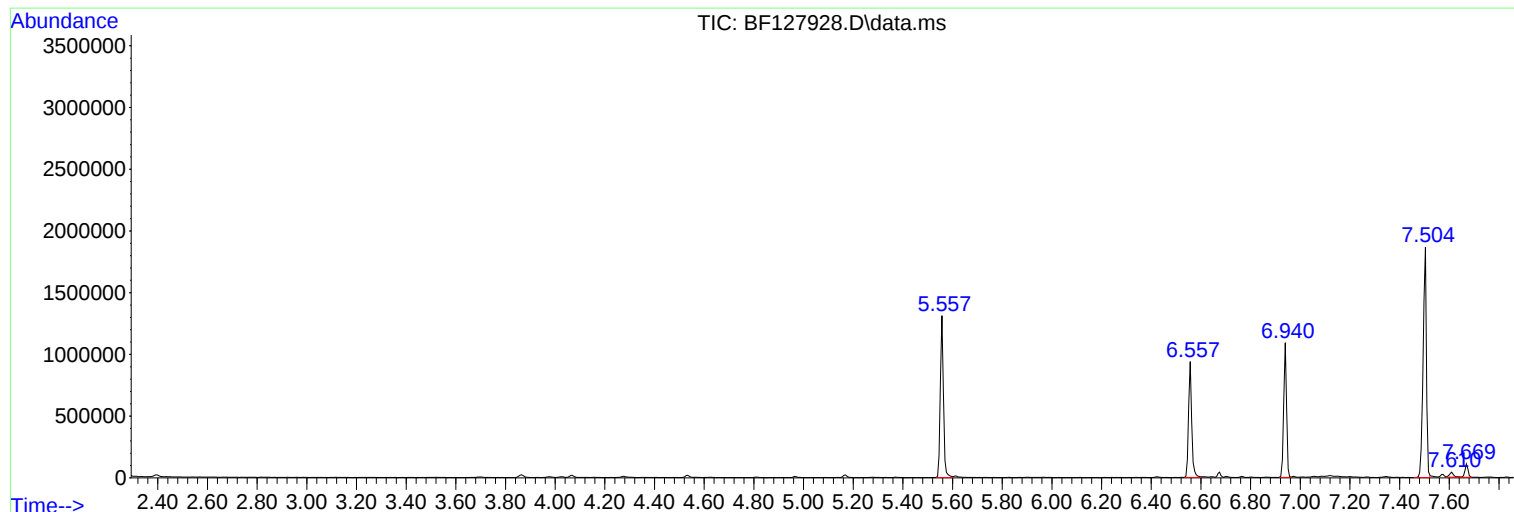

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\
Data File : BF127928.D
Acq On : 26 Apr 2022 22:36
Operator : CG\JU
Sample : N2551-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20220376-096-21-02-ELUTRIATE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\
Data File : BF127928.D
Acq On : 26 Apr 2022 22:36
Operator : CG\JU
Sample : N2551-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20220376-096-21-02-ELUTRIATE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc