
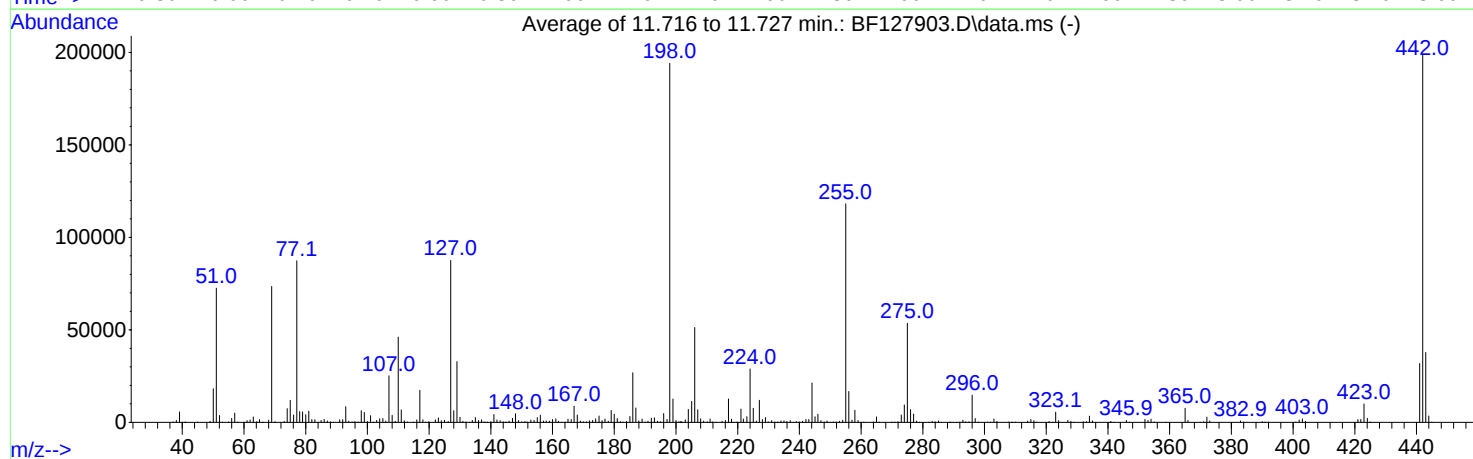


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\
 Data File : BF127903.D
 Acq On : 26 Apr 2022 09:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Apr 24 00:43:03 2022

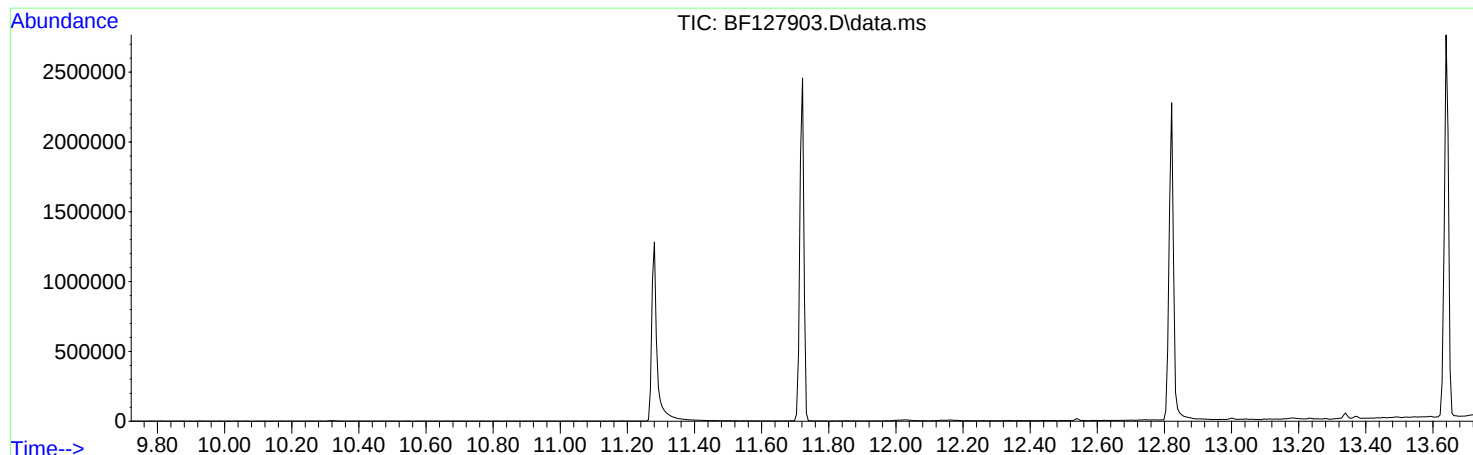




AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	72544	PASS
68	69	0.00	2	1.7	1214	PASS
69	198	0.00	100	37.8	73413	PASS
70	69	0.00	2	0.5	378	PASS
127	198	10	80	45.1	87573	PASS
197	198	0.00	2	0.9	1693	PASS
198	198	100	100	100.0	194123	PASS
199	198	5	9	6.5	12599	PASS
275	198	10	60	27.6	53571	PASS
365	198	1	100	3.9	7662	PASS
441	198	0.01	100	16.4	31819	PASS
442	442	50	100	100.0	198843	PASS
443	442	15	24	19.0	37771	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\
Data File : BF127903.D
Acq On : 26 Apr 2022 09:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 27 05:38:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 00:43:03 2022
Response via : Initial Calibration

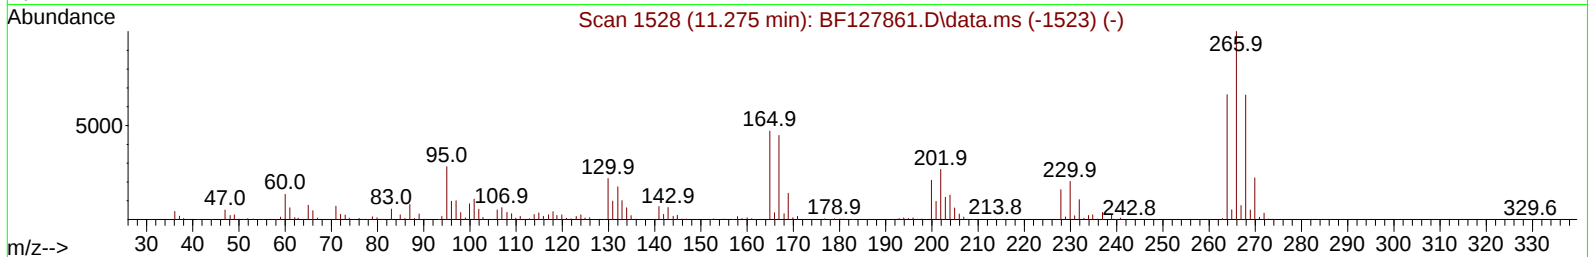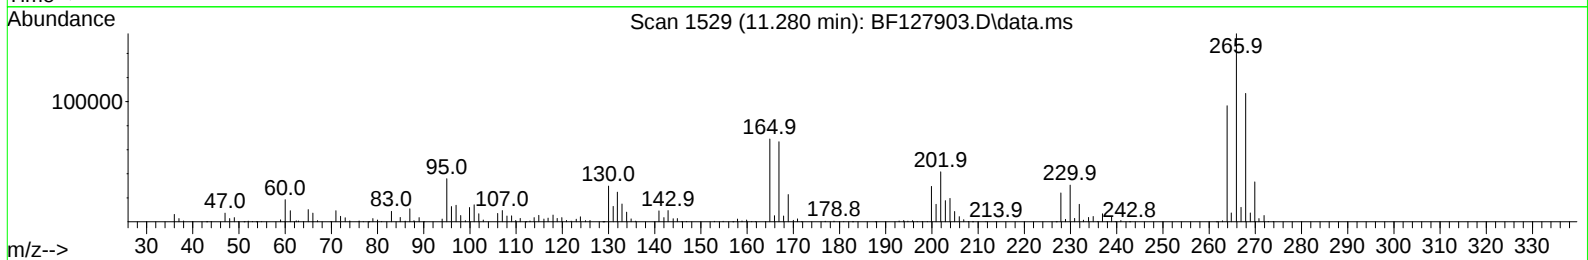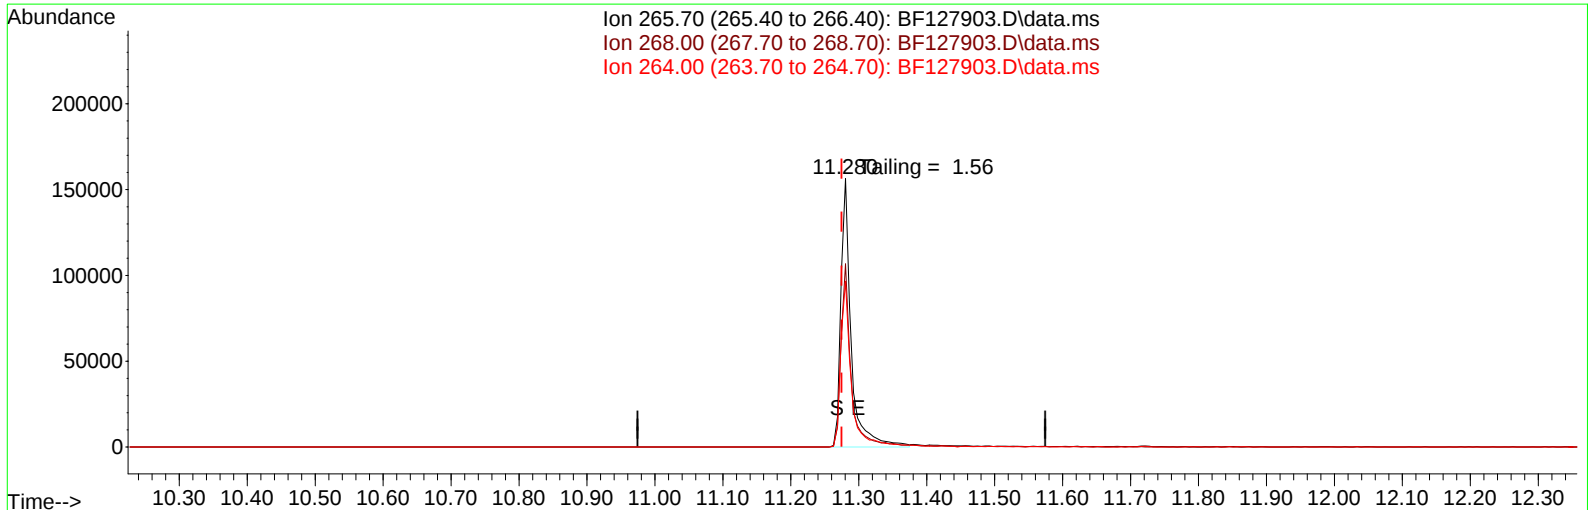

TIC: BF127903.D\data.ms

(70) Pentachlorophenol (C)

11.280min (+ 0.006) 361396.70 ng




response 163892

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	68.26
264.00	66.40	61.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\
Data File : BF127903.D
Acq On : 26 Apr 2022 09:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 27 05:38:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 00:43:03 2022
Response via : Initial Calibration

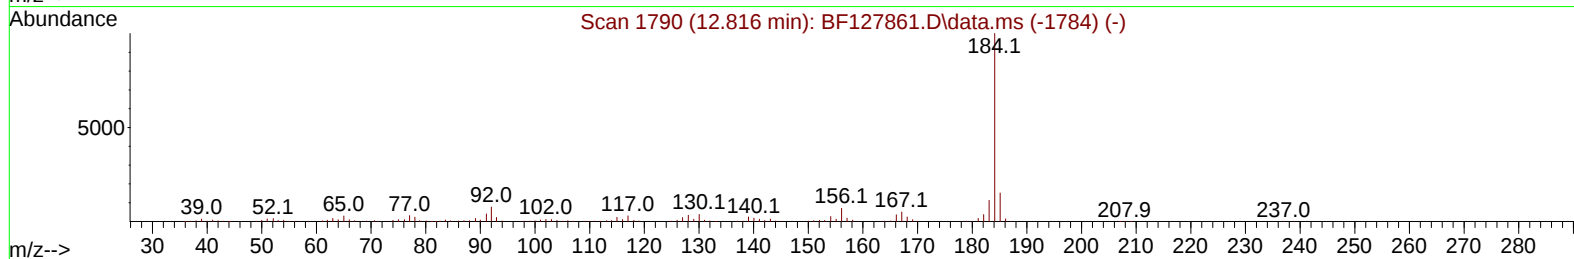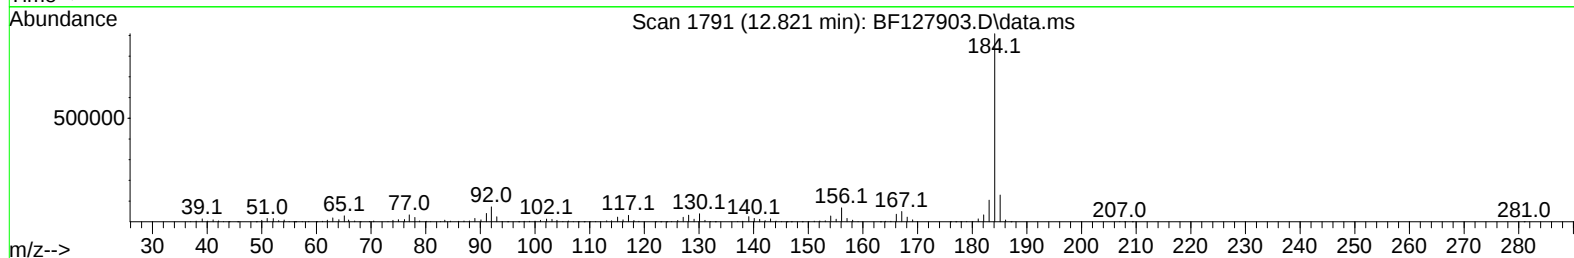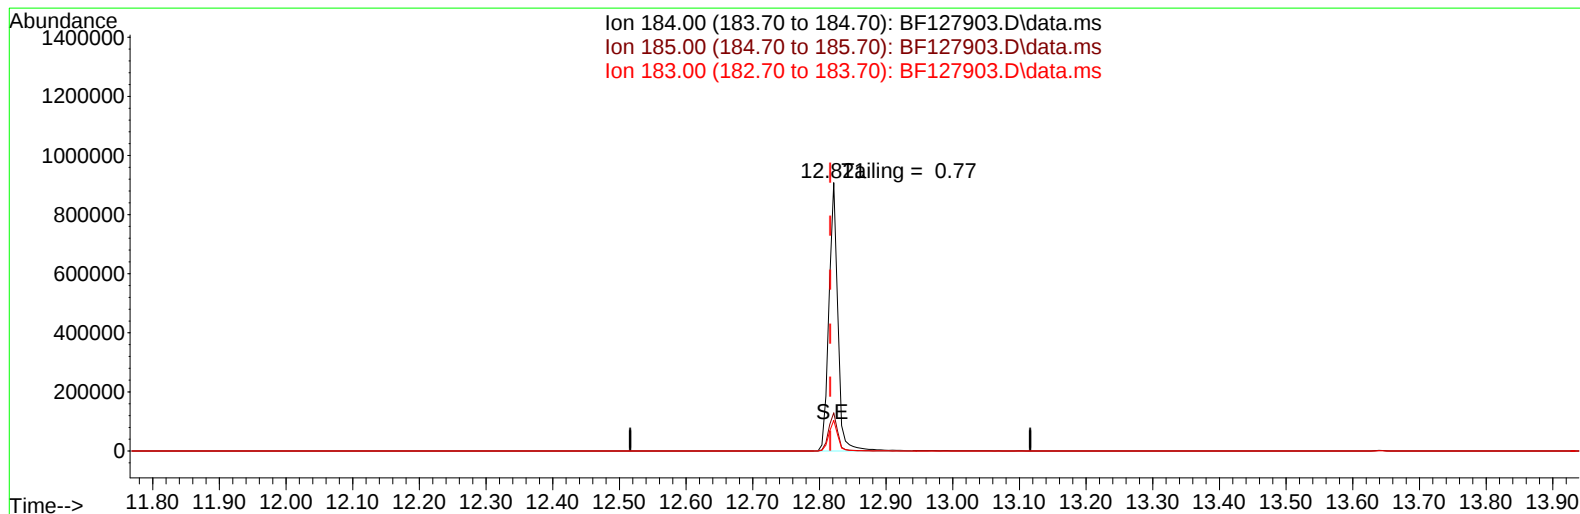

TIC: BF127903.D\data.ms

(77) Benzidine

12.821min (+ 0.005) 196990.64 ng

response 849835

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.26
183.00	11.20	11.47
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/26/2022	BNA_F	<u>BF127903.D</u>
Compound Name	Response	Retention Time
DDT	463386	13.639
DDD	10105	13.339
DDE	1097	13.004
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11202	474588	2.36

Instrument :
BNA_F
ClientSampleId :
DFTPP