
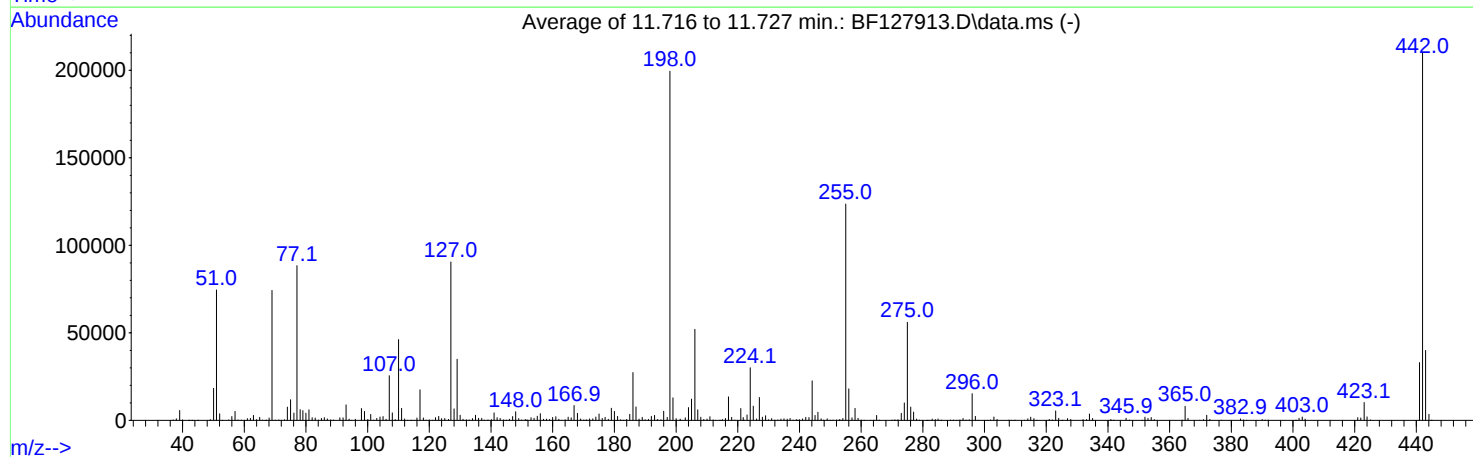


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\
 Data File : BF127913.D
 Acq On : 26 Apr 2022 15:11
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Apr 24 00:43:03 2022

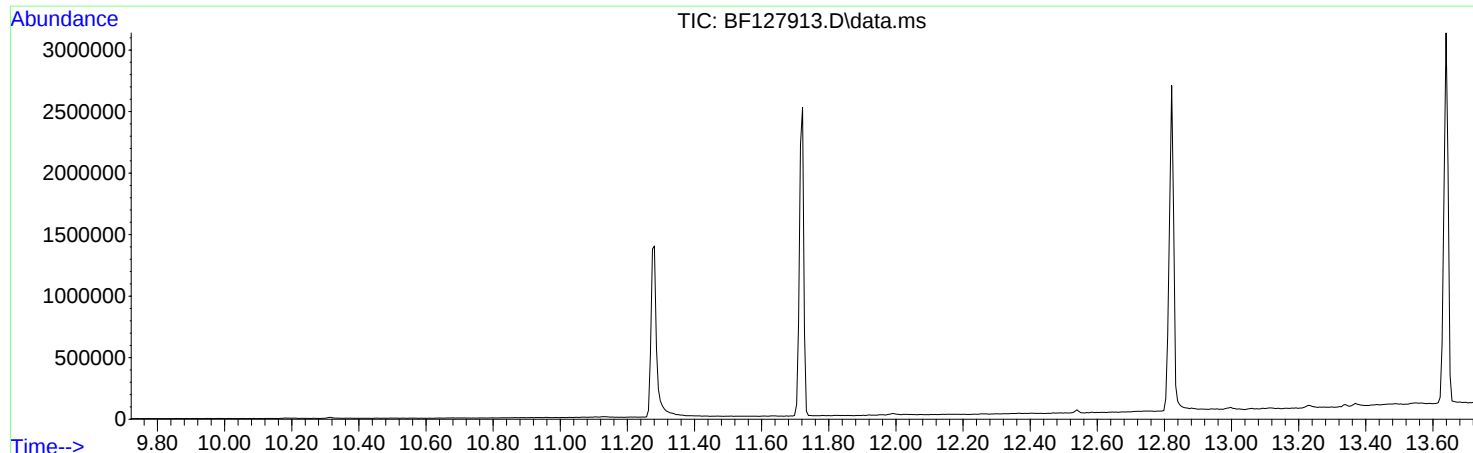




AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	74476	PASS
68	69	0.00	2	1.9	1421	PASS
69	198	0.00	100	37.2	74259	PASS
70	69	0.00	2	0.3	226	PASS
127	198	10	80	45.4	90496	PASS
197	198	0.00	2	0.9	1737	PASS
198	198	100	100	100.0	199523	PASS
199	198	5	9	6.5	12922	PASS
275	198	10	60	28.1	56021	PASS
365	198	1	100	4.0	8021	PASS
441	198	0.01	100	16.5	33011	PASS
442	442	50	100	100.0	210197	PASS
443	442	15	24	19.0	39965	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\  
Data File : BF127913.D  
Acq On    : 26 Apr 2022  15:11  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 27 05:42:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 00:43:03 2022
Response via : Initial Calibration

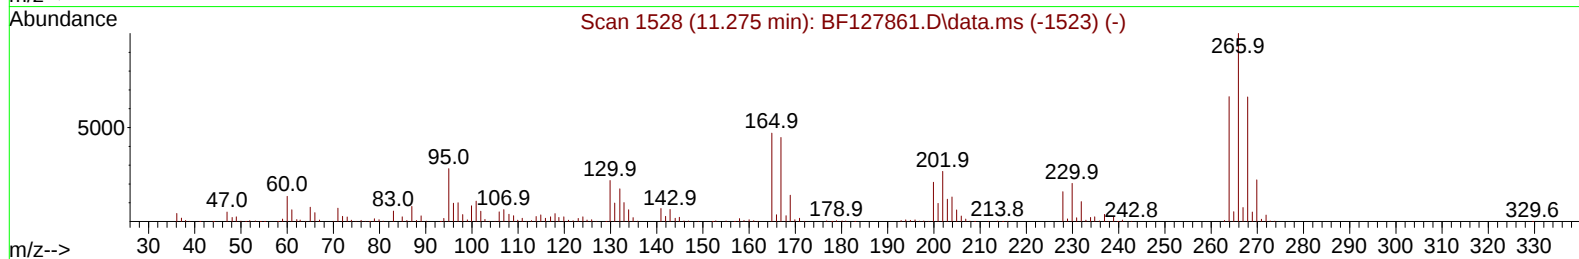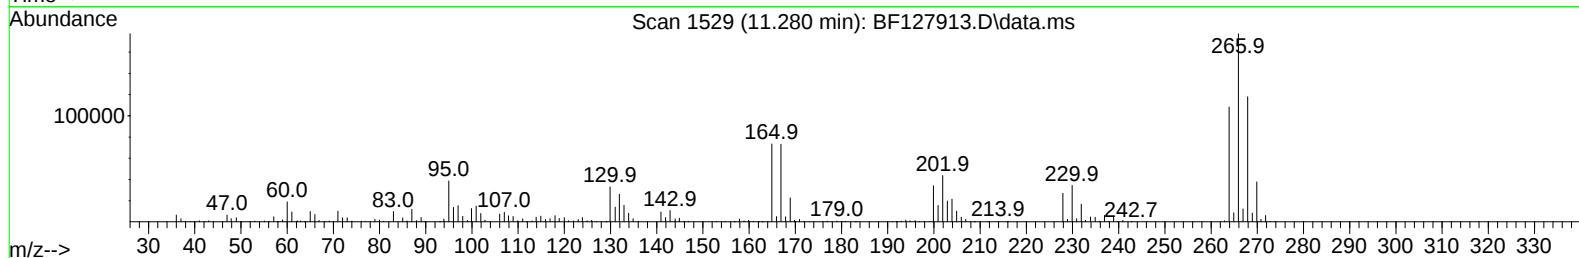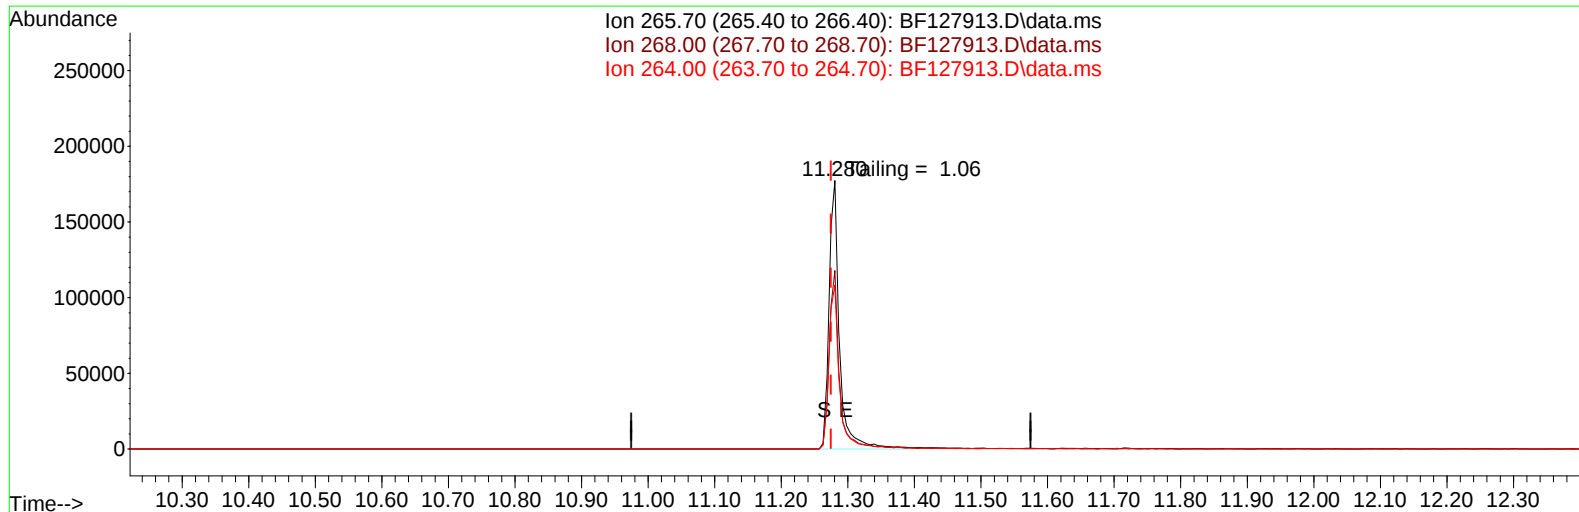

TIC: BF127913.D\data.ms

(70) Pentachlorophenol (C)

11.280min (+ 0.006) 471509.88 ng




response	194389
----------	--------

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	66.51
264.00	66.40	61.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042622\
 Data File : BF127913.D
 Acq On : 26 Apr 2022 15:11
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 27 05:42:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Apr 24 00:43:03 2022
 Response via : Initial Calibration

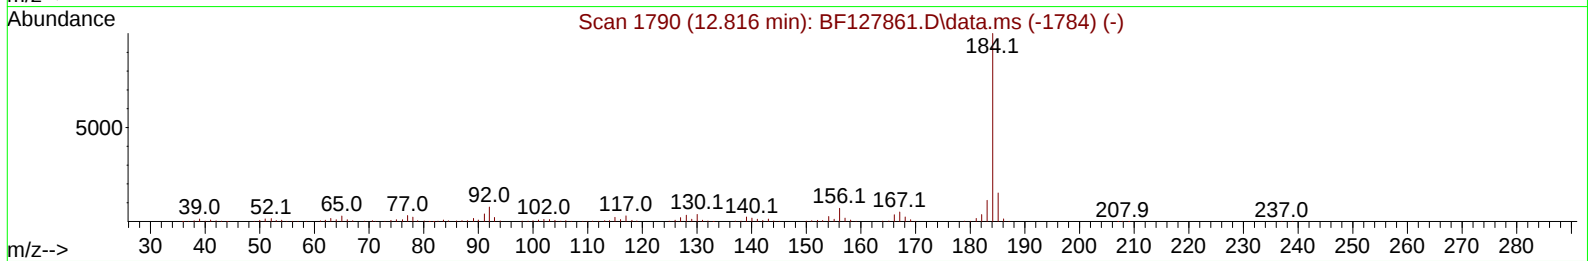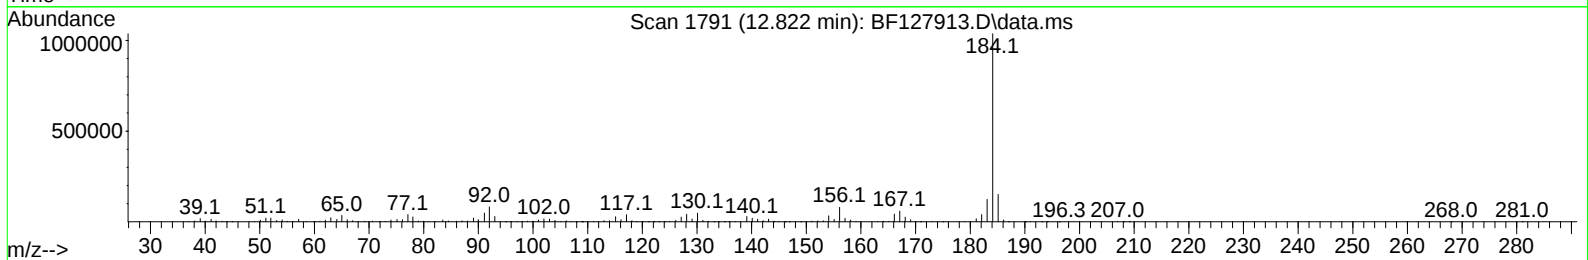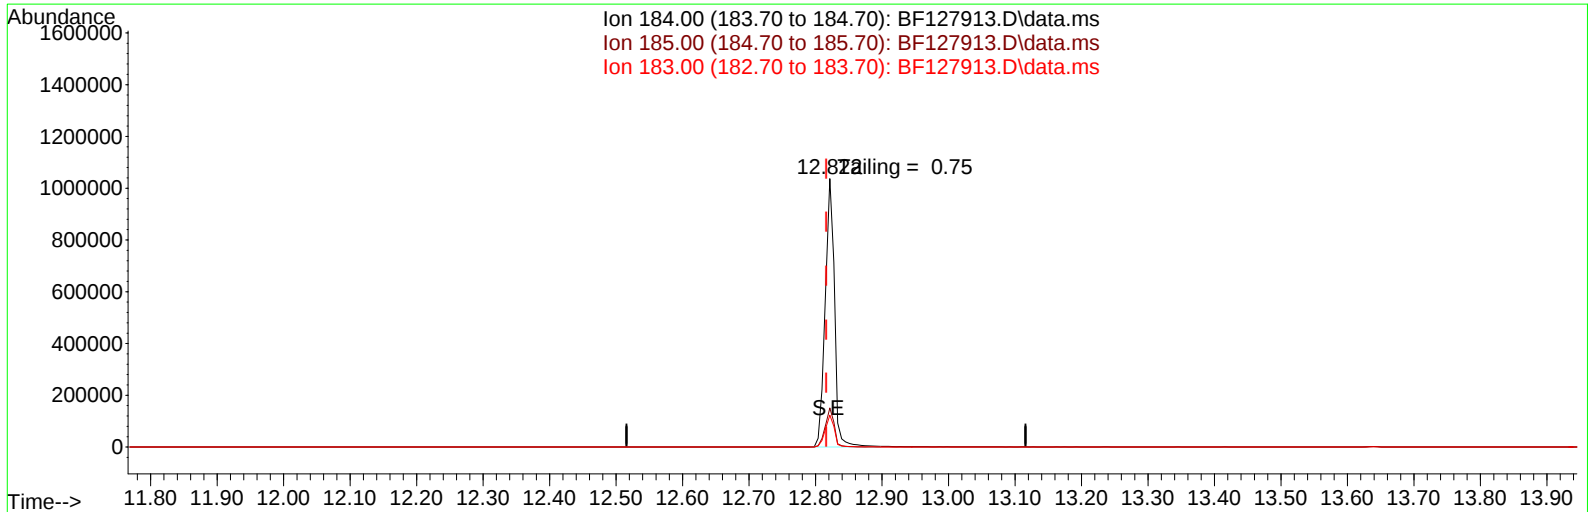

TIC: BF127913.D\data.ms

(77) Benzidine

12.822min (+ 0.006) 192128.30 ng

response 1014261

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.57
183.00	11.20	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/26/2022	BNA_F	<u>BF127913.D</u>
Compound Name	Response	Retention Time
DDT	522223	13.639
DDD	6867	13.339
DDE	1169	12.998
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8036	530259	1.52

Instrument :
BNA_F
ClientSampleId :
DFTPP