
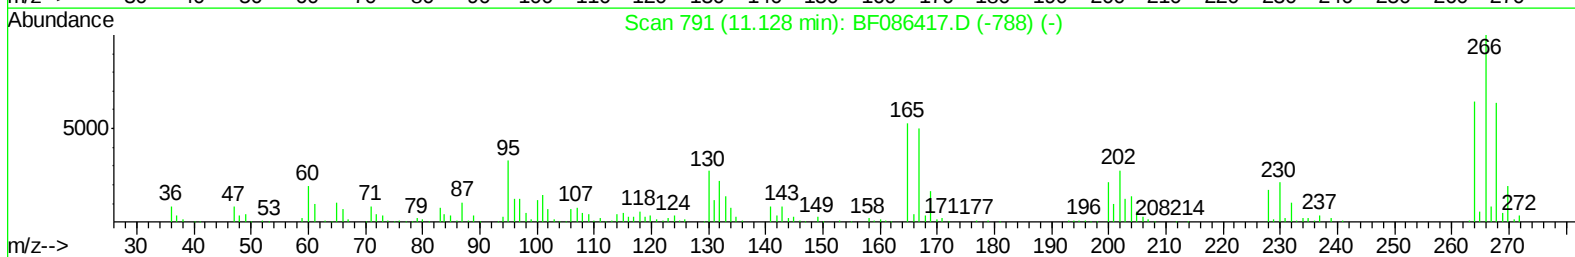
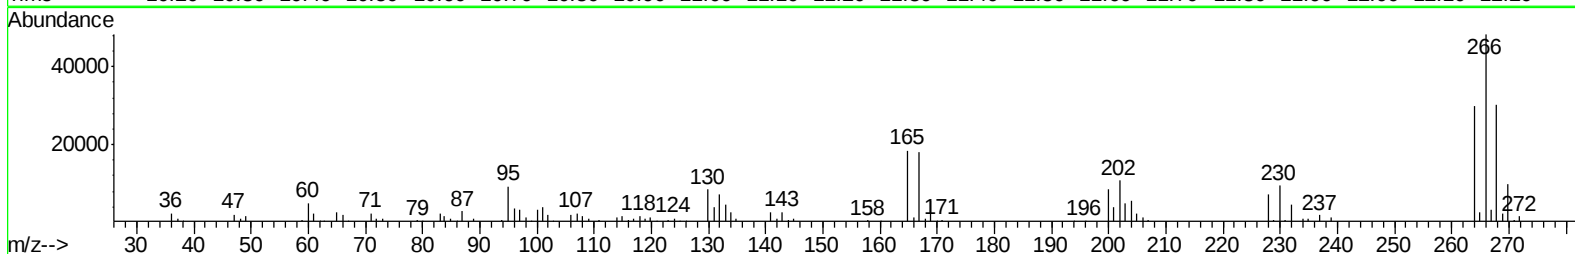


Data Path : Z:\HPCHEM1\BNA F\DATA\BF042716\
Data File : BF086413.D
Acq On : 27 Apr 2016 9:59
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 12:36:18 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 27 11:18:22 2016
Response via : Initial Calibration

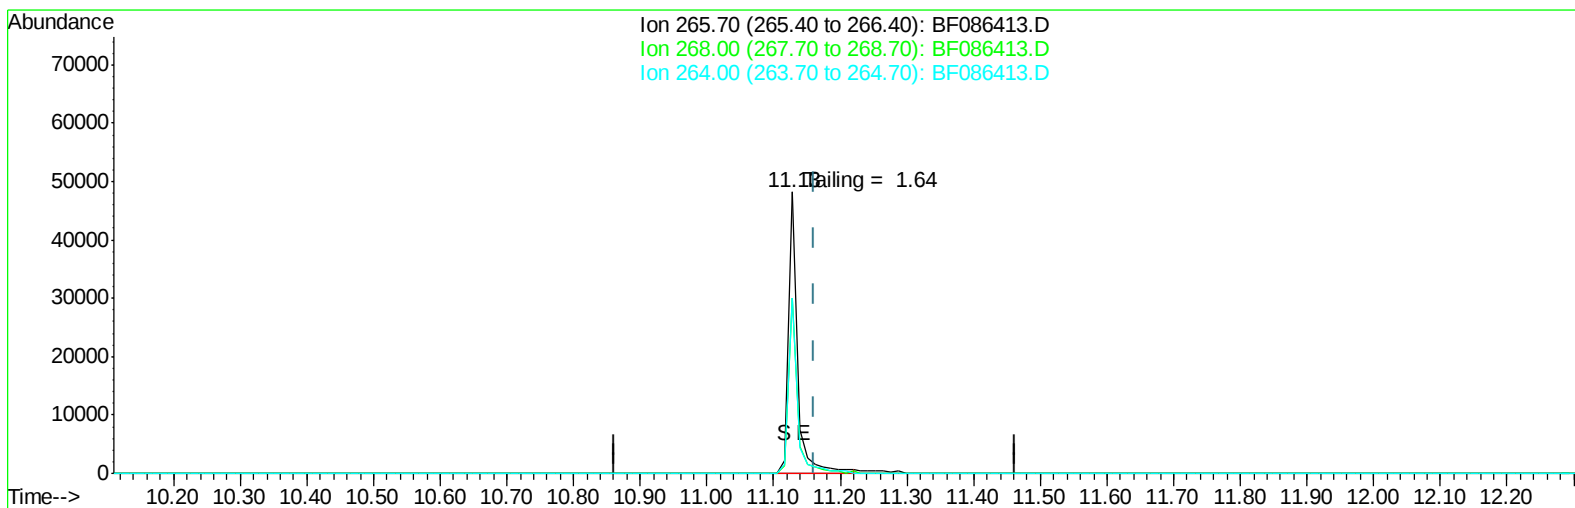

TIC: BF086413.D

(69) Pentachlorophenol (C)




11.128min (-0.034) 22627.33ng

response 46781

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	62.31
264.00	66.10	62.11
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042716\
Data File : BF086413.D
Acq On : 27 Apr 2016 9:59
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 12:36:18 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 27 11:18:22 2016
Response via : Initial Calibration

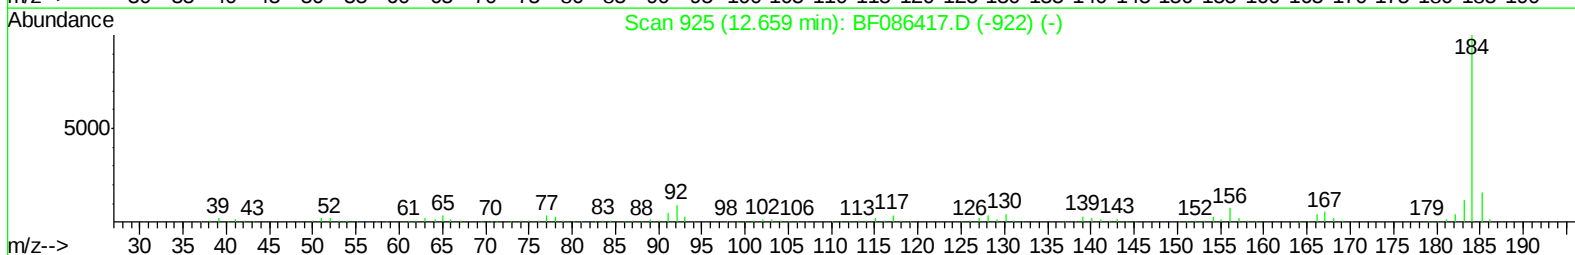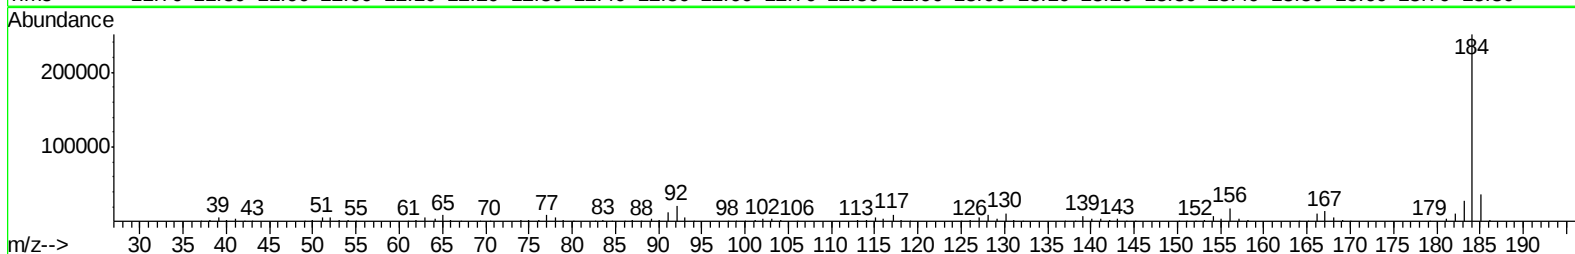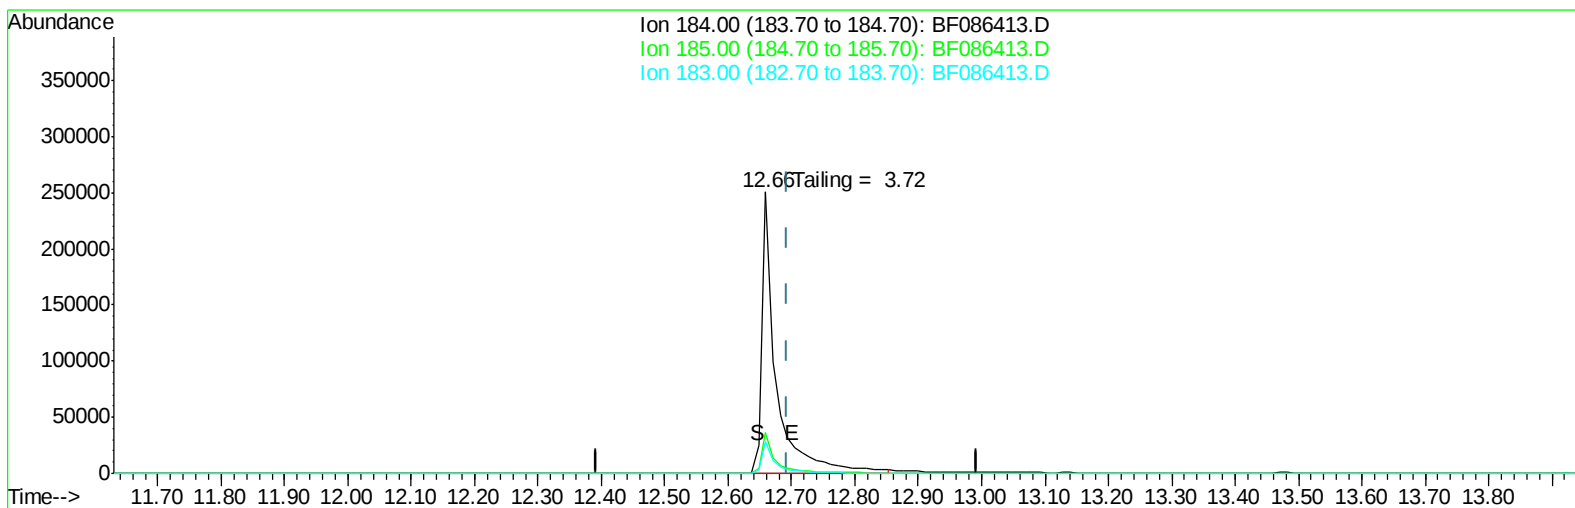

TIC: BF086413.D

(76) Benzidine

12.659min (-0.034) 0.00ng

response 409699

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	14.54
183.00	12.20	11.36
0.00	0.00	0.00