

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042716\
 Data File : BF086452.D
 Acq On : 28 Apr 2016 4:46
 Operator : UM/SJ
 Sample : H2707-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RICHMOND-AMBOY-SB04(0.5-6.0)

Quant Time: Apr 28 07:39:46 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF042716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 27 14:20:52 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.81	152	131257	20.00	ng	0.00
21) Naphthalene-d8	8.09	136	484953	20.00	ng	-0.01
38) Acenaphthene-d10	9.85	164	172985	20.00	ng	0.00
63) Phenanthrene-d10	11.32	188	287220	20.00	ng	0.00
75) Chrysene-d12	13.95	240	317007	20.00	ng	-0.01
86) Perylene-d12	15.37	264	219943	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.40	112	893455	117.41	ng	0.01
7) Phenol-d6	6.44	99	1137735	107.12	ng	0.00
23) Nitrobenzene-d5	7.37	82	686327	76.28	ng	-0.01
41) 2,4,6-Tribromophenol	10.64	330	184080	100.91	ng	0.00
44) 2-Fluorobiphenyl	9.17	172	1080944	118.28	ng	0.00
78) Terphenyl-d14	12.91	244	782530	54.38	ng	0.00
Target Compounds						Qvalue
49) Dimethylphthalate	9.56	163	171478	13.17	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042716\
Data File : BF086452.D
Acq On : 28 Apr 2016 4:46
Operator : UM/SJ
Sample : H2707-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RICHMOND-AMBOY-SB04(0.5-6.0)

Quant Time: Apr 28 07:39:46 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 27 14:20:52 2016
Response via : Initial Calibration

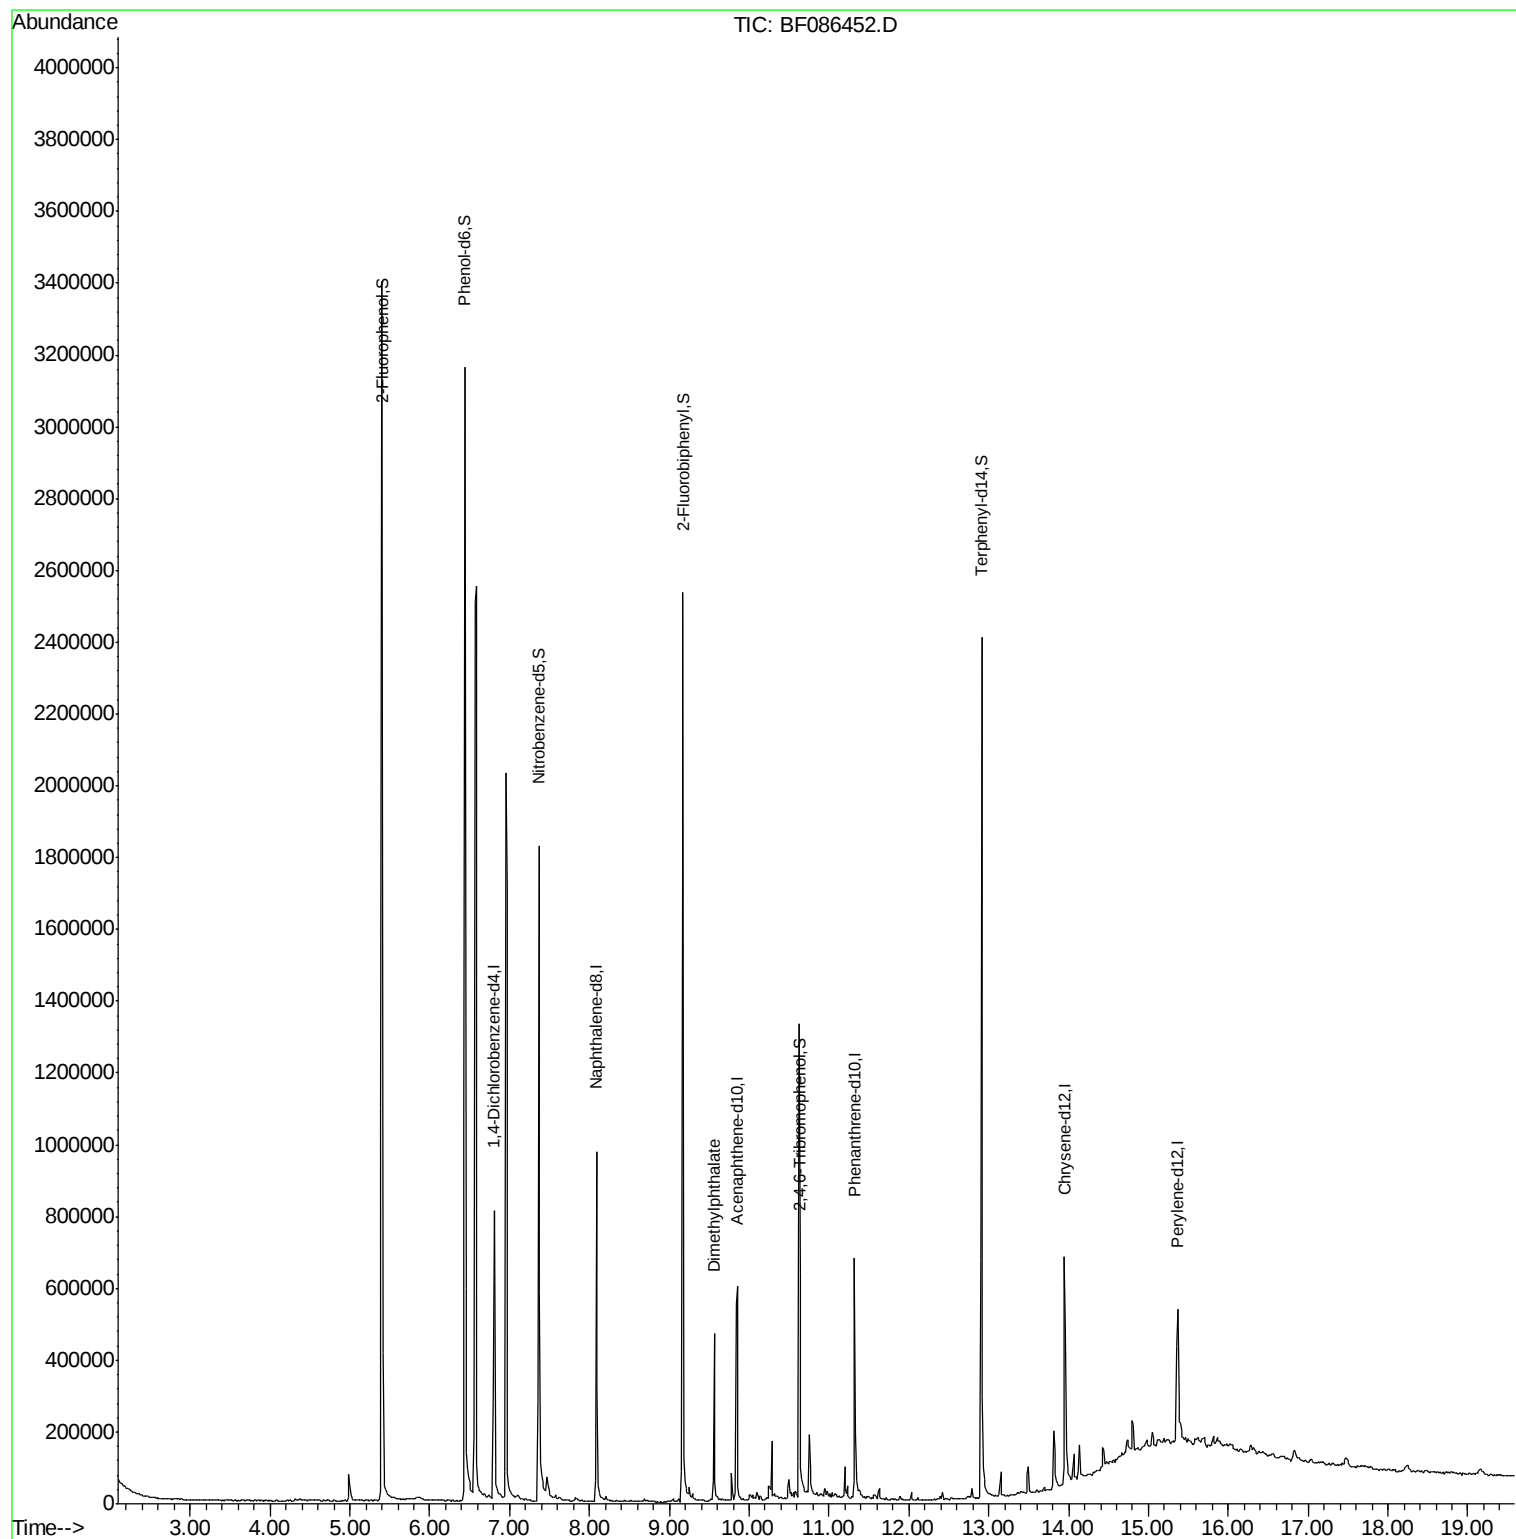

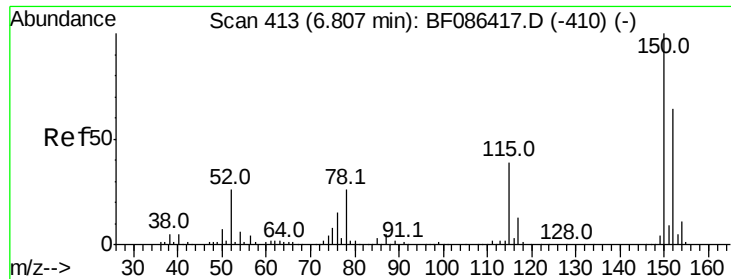

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.81 min Scan# 413

Delta R.T. 0.00 min

Lab File: BF086452.D

Acq: 28 Apr 2016 4:46

Instrument :

BNA_F

ClientSampleId :

RICHMOND-AMBOY-SB04(0.5-6.0)


Tot Ion:152 Resp: 131257

Ion Ratio Lower Upper

152 100

150 152.8 125.8 188.6




115 58.0 51.5 77.3

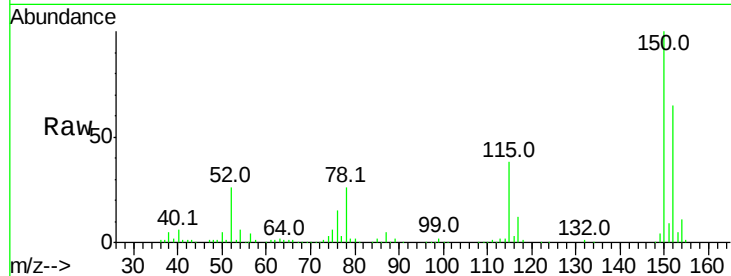

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

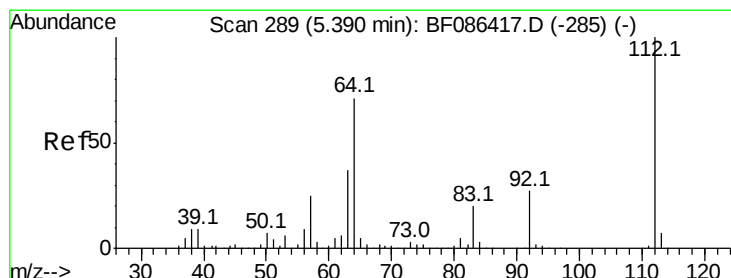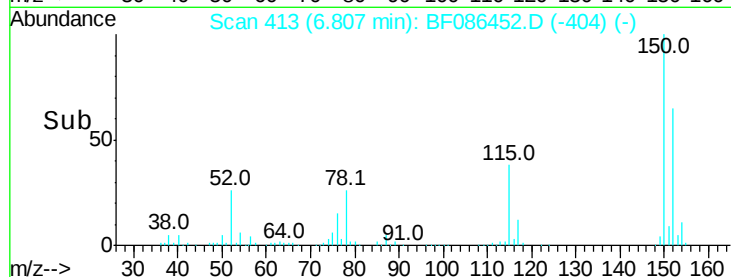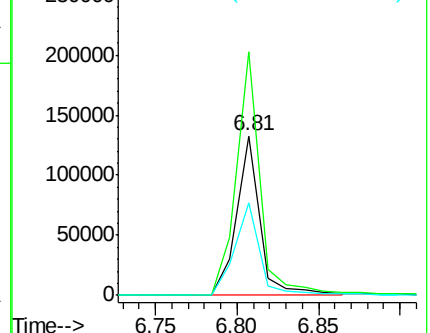

#5

2-Fluorophenol

Concen: 117.41 ng

RT: 5.40 min Scan# 290

Delta R.T. 0.01 min

Lab File: BF086452.D

Acq: 28 Apr 2016 4:46


Tgt Ion:112 Resp: 893455

Ion Ratio Lower Upper

112 100

64 72.4 52.1 78.1



63 38.4 25.7 38.5

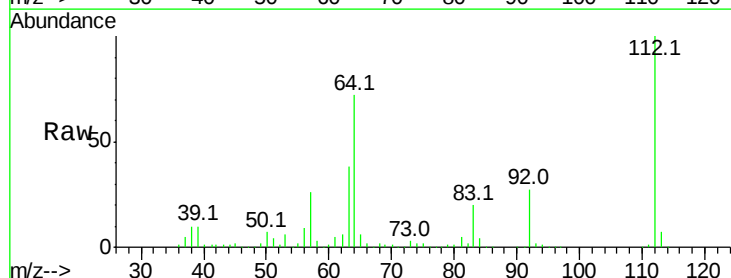


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

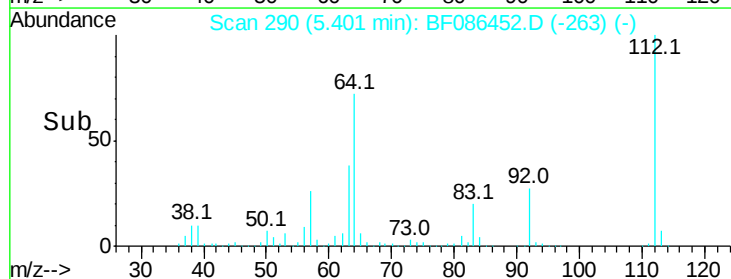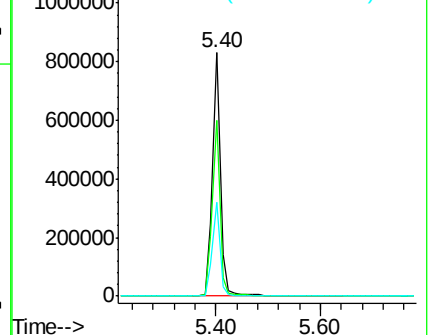

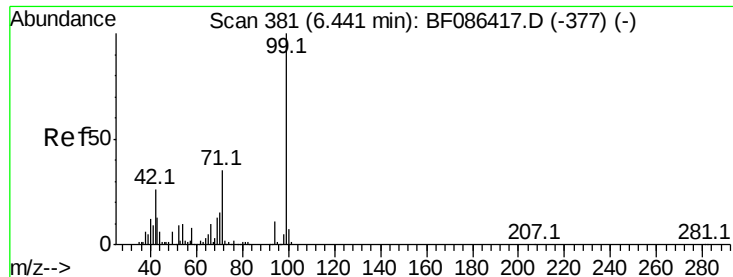

#7

Phenol-d6

Concen: 107.12 ng

RT: 6.44 min Scan# 381

Delta R.T. 0.00 min

Lab File: BF086452.D

Acq: 28 Apr 2016 4:46

Instrument :





BNA_F

ClientSampleId :

RICHMOND-AMBOY-SB04(0.5-6.0)

Tot Ion: 99 Resp: 1137735

Ion	Ratio	Lower	Upper
99	100		
42	28.0	13.6	20.4#
71	36.6	24.6	36.8

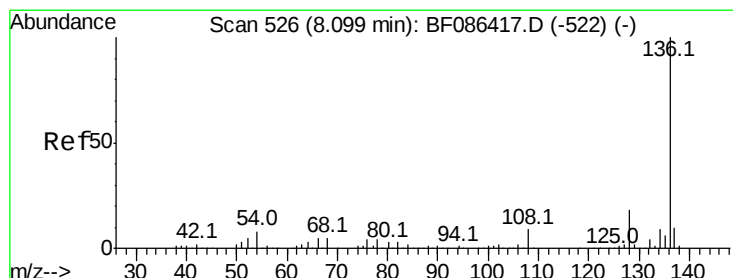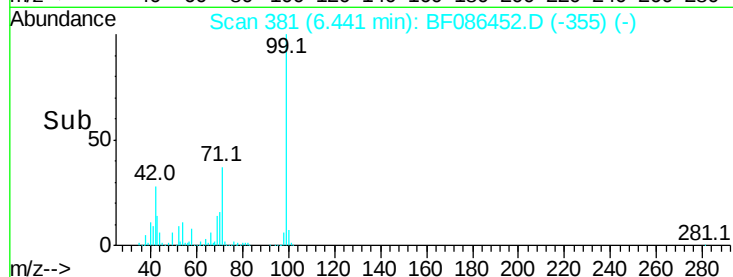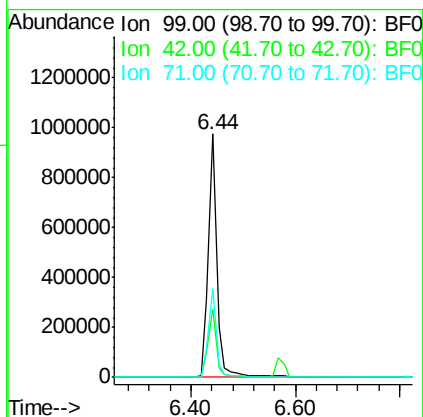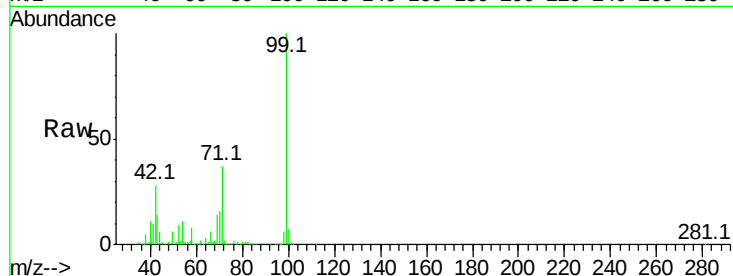

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.09 min Scan# 525




Delta R.T. -0.01 min


Lab File: BF086452.D

Acq: 28 Apr 2016 4:46

Tgt Ion: 136 Resp: 484953

Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.8	13.2
54	13.7	5.0	7.4#
68	8.1	4.4	6.6#


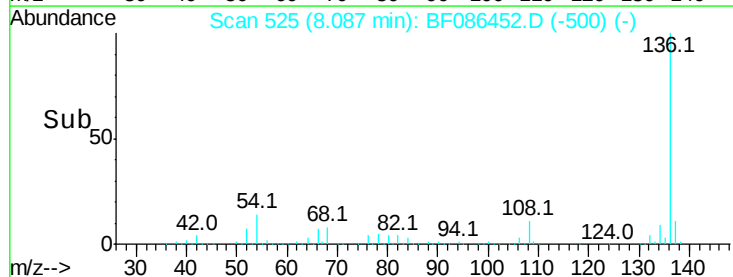
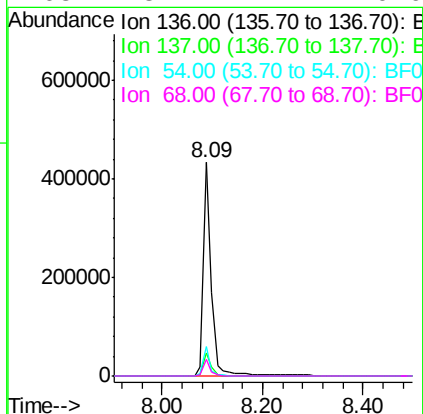
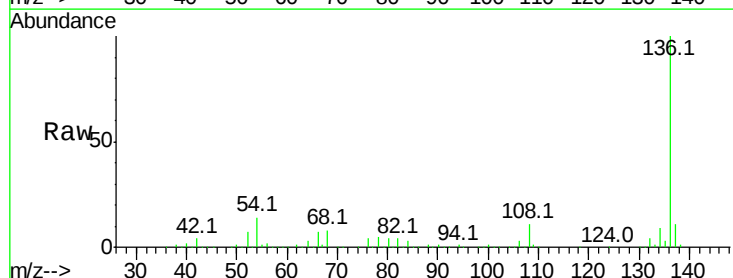


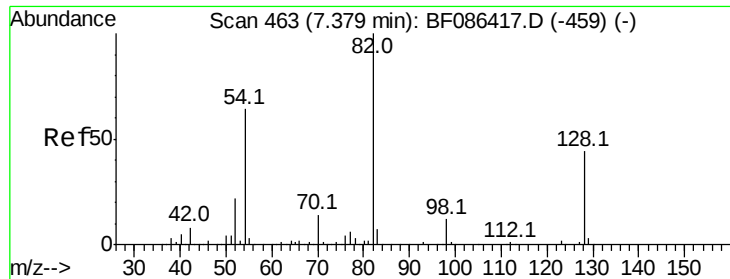

#23
 Nitrobenzene-d5
 Concen: 76.28 ng
 RT: 7.37 min Scan# 462
 Delta R.T. -0.01 min
 Lab File: BF086452.D
 Acq: 28 Apr 2016 4:46




Instrument :
 BNA_F
 ClientSampleId :
 RICHMOND-AMBOY-SB04(0.5-6.0)


Tot Ion	Ratio	Lower	Upper
82	100		
128	38.7	40.6	61.0#
54	68.8	38.1	57.1#

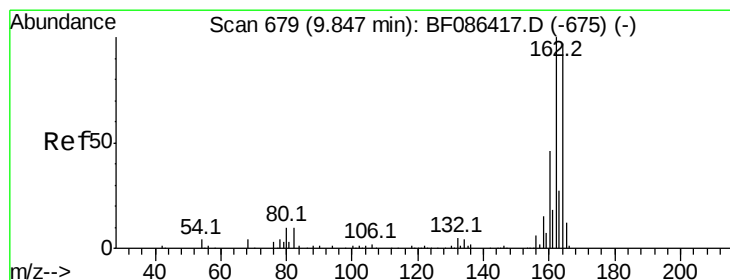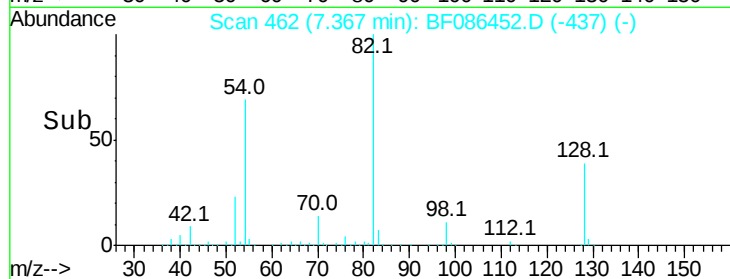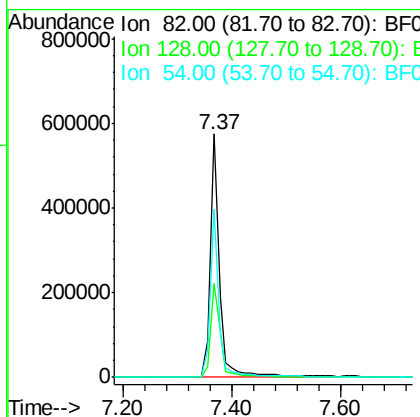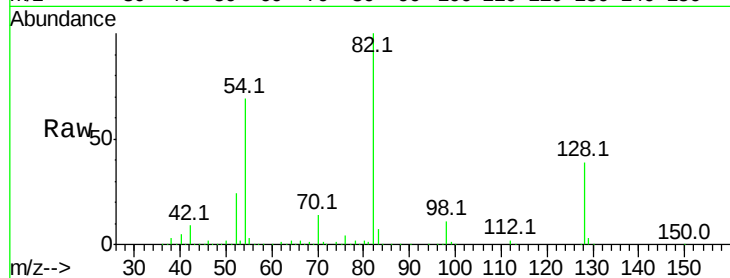

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.85 min Scan# 679
 Delta R.T. 0.00 min
 Lab File: BF086452.D
 Acq: 28 Apr 2016 4:46

Tgt Ion	Ratio	Lower	Upper
164	100		
162	103.2	82.8	124.2
160	48.3	36.9	55.3


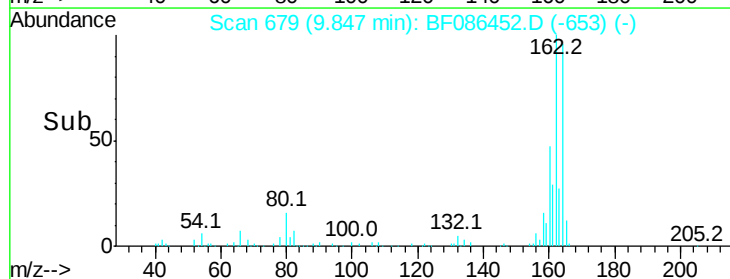
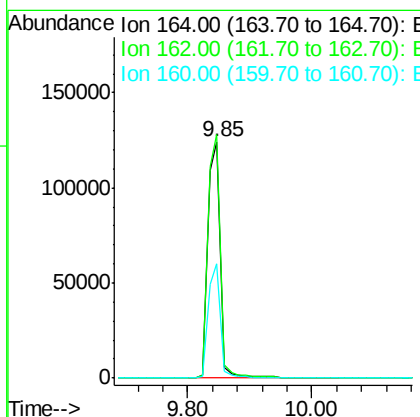
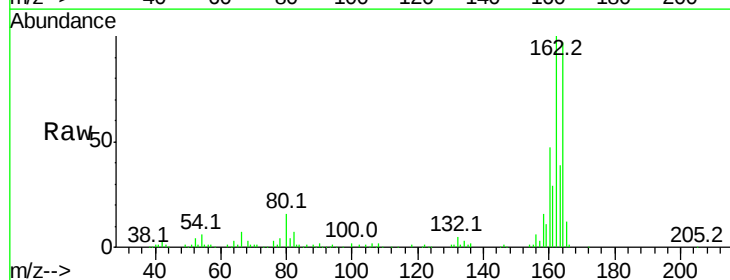


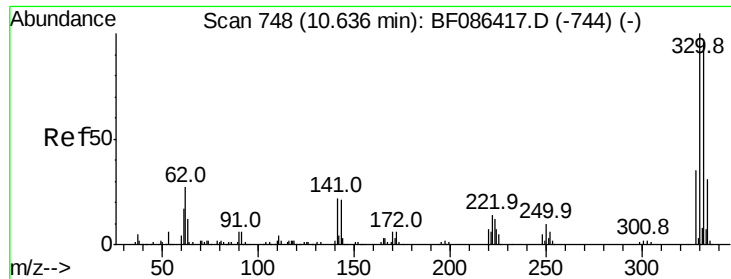

#41
 2,4,6-Tribromophenol
 Concen: 100.91 ng
 RT: 10.64 min Scan# 748
 Delta R.T. 0.00 min
 Lab File: BF086452.D
 Acq: 28 Apr 2016 4:46




Instrument :
 BNA_F
 ClientSampleId :
 RICHMOND-AMBOY-SB04(0.5-6.0)


Tot Ion:330 Resp: 184080
 Ion Ratio Lower Upper
 330 100
 332 98.1 79.0 118.4
 141 35.0 31.2 46.8

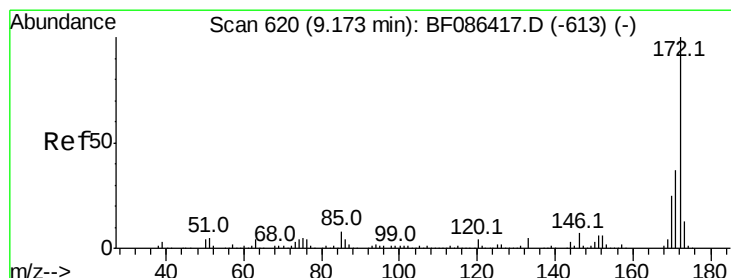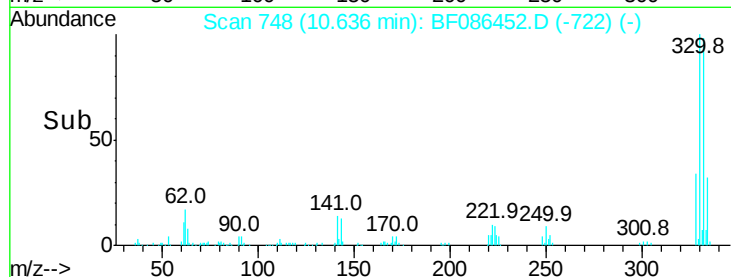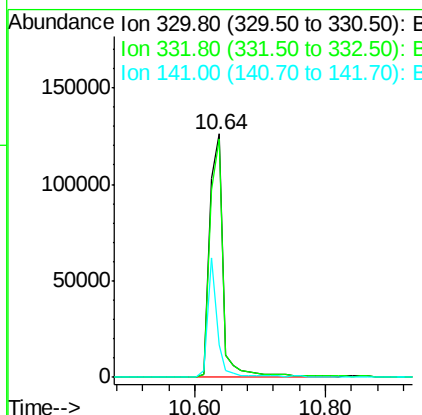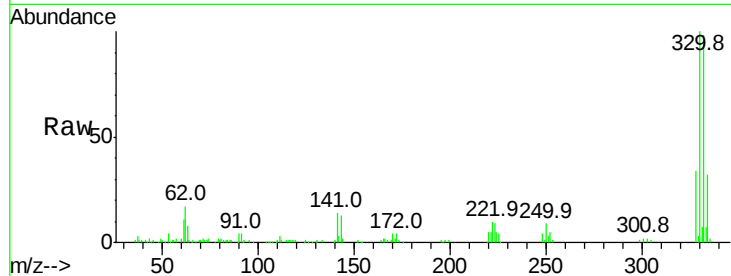

#44
 2-Fluorobiphenyl
 Concen: 118.28 ng
 RT: 9.17 min Scan# 620
 Delta R.T. 0.00 min
 Lab File: BF086452.D
 Acq: 28 Apr 2016 4:46

Tgt Ion:172 Resp: 1080944
 Ion Ratio Lower Upper
 172 100
 171 35.3 29.0 43.6
 170 24.4 19.8 29.8

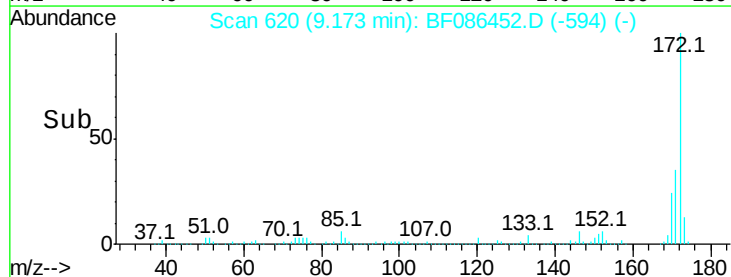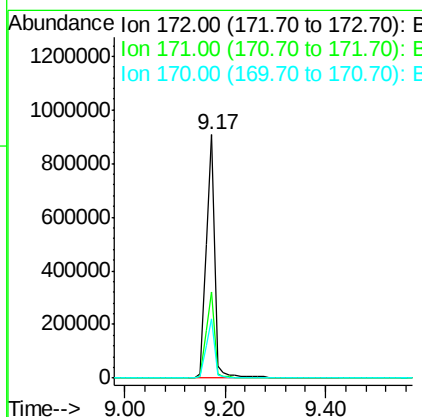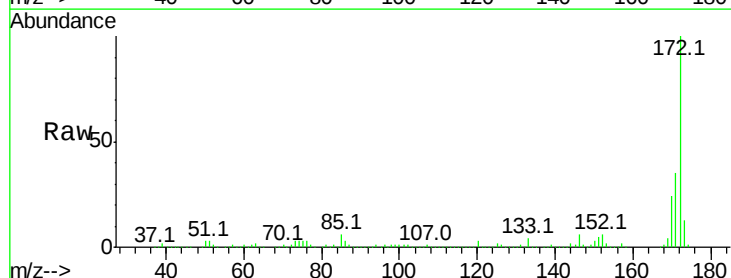

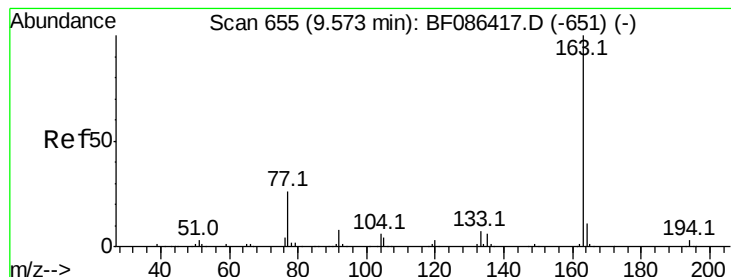

#49

Dimethylphthalate

Concen: 13.17 ng

RT: 9.56 min Scan# 654

Delta R.T. -0.01 min

Lab File: BF086452.D

Acq: 28 Apr 2016 4:46

Instrument :

BNA_F

ClientSampleId :

RICHMOND-AMBOY-SB04(0.5-6.0)


Tot Ion:163 Resp: 171478

Ion Ratio Lower Upper

163 100

194 3.4 2.6 4.0




164 10.0 8.2 12.4

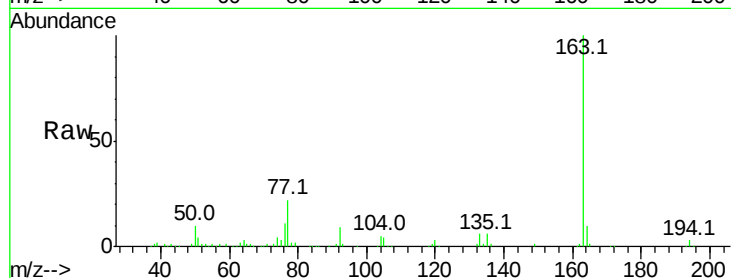

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

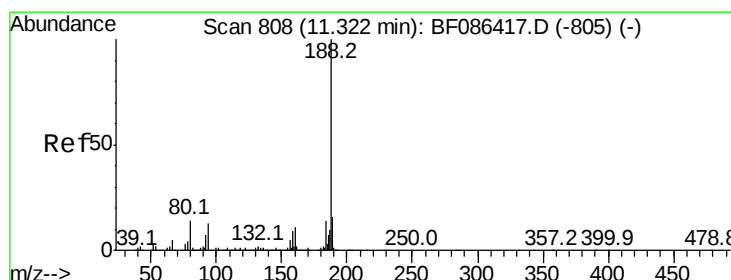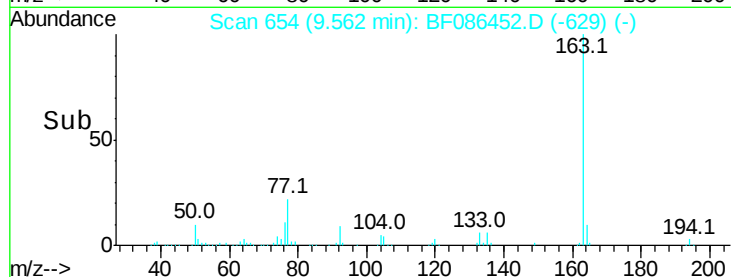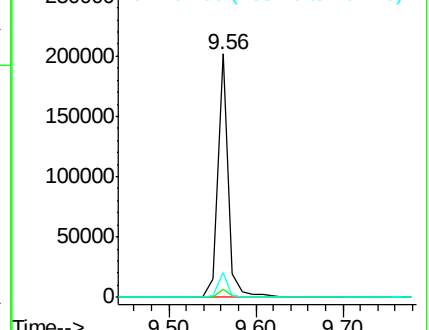

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.32 min Scan# 808

Delta R.T. 0.00 min

Lab File: BF086452.D

Acq: 28 Apr 2016 4:46


Tgt Ion:188 Resp: 287220

Ion Ratio Lower Upper

188 100

94 11.7 6.8 10.2#



80 12.7 7.1 10.7#

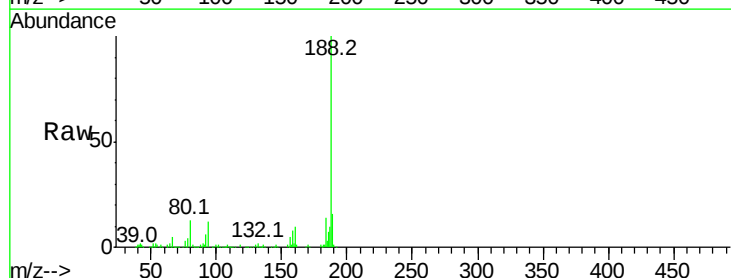


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

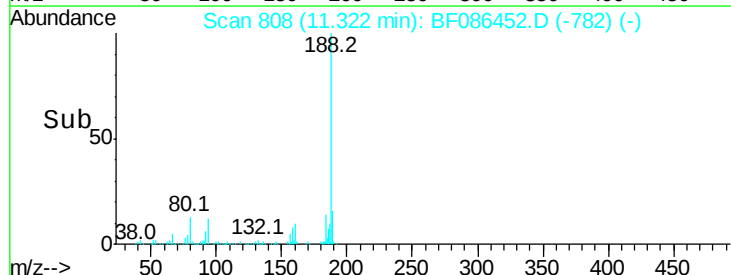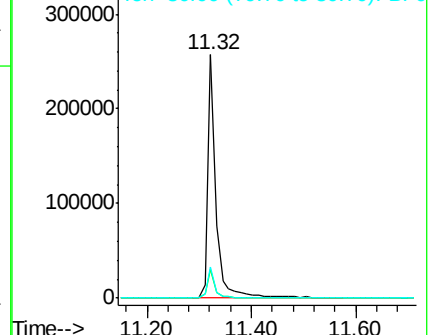

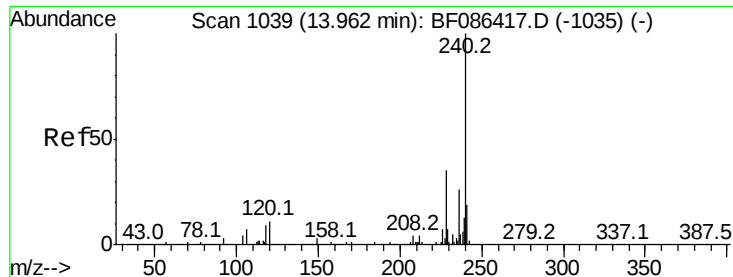

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.95 min Scan# 1038

Delta R.T. -0.01 min

Lab File: BF086452.D

Acq: 28 Apr 2016 4:46

Instrument :

BNA_F

ClientSampleId :

RICHMOND-AMBOY-SB04(0.5-6.0)


Tot Ion:240 Resp: 317007

Ion Ratio Lower Upper

240 100

120 17.0 11.2 16.8#




236 26.8 21.2 31.8

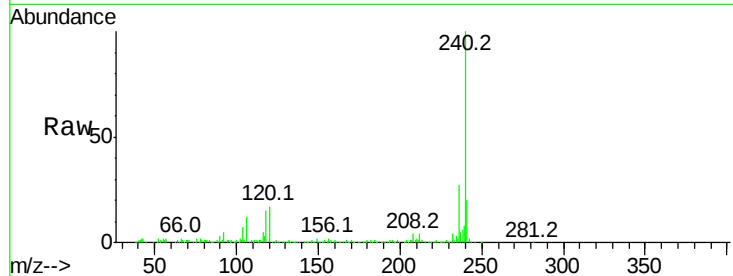

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

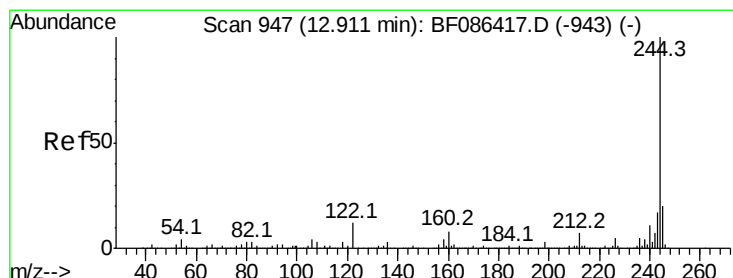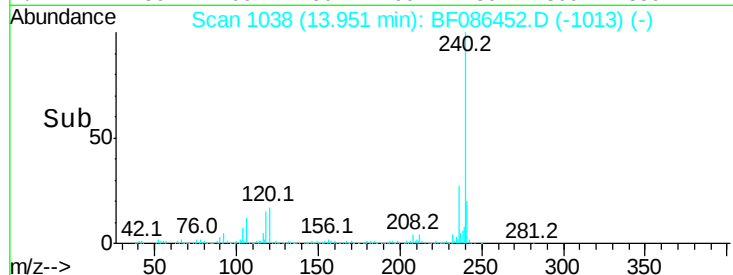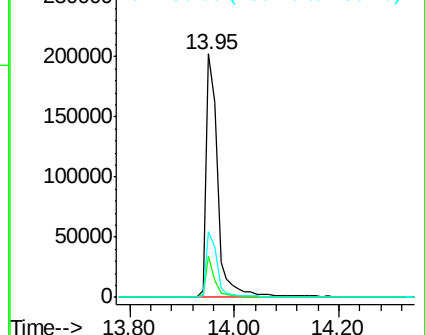

#78

Terphenyl-d14

Concen: 54.38 ng

RT: 12.91 min Scan# 947

Delta R.T. 0.00 min

Lab File: BF086452.D

Acq: 28 Apr 2016 4:46


Tgt Ion:244 Resp: 782530

Ion Ratio Lower Upper

244 100

212 7.5 6.2 9.2



122 12.5 12.0 18.0

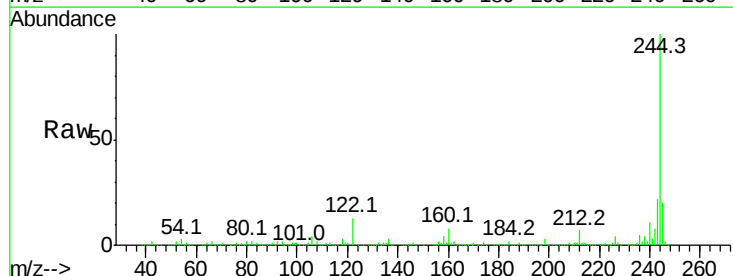


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

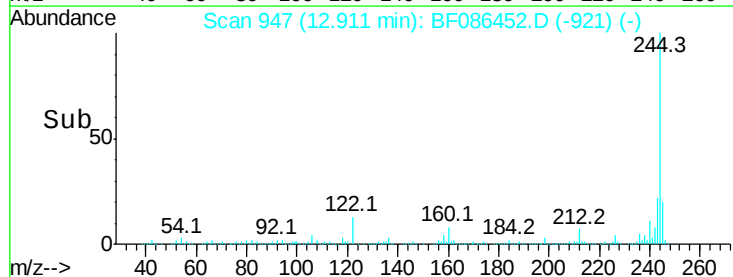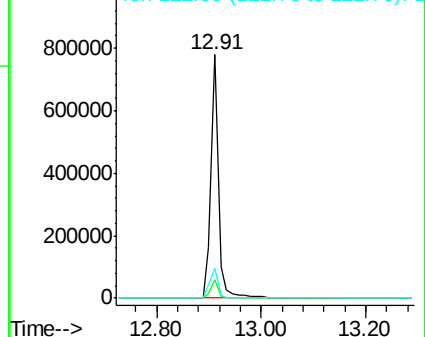


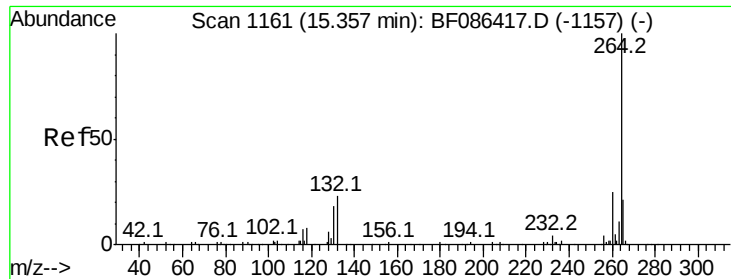

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 15.37 min Scan# 1162
 Delta R.T. 0.01 min
 Lab File: BF086452.D
 Acq: 28 Apr 2016 4:46

Instrument :
 BNA_F
 ClientSampleId :
 RICHMOND-AMBOY-SB04(0.5-6.0)

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.3	19.5	29.3
265	21.2	17.3	25.9

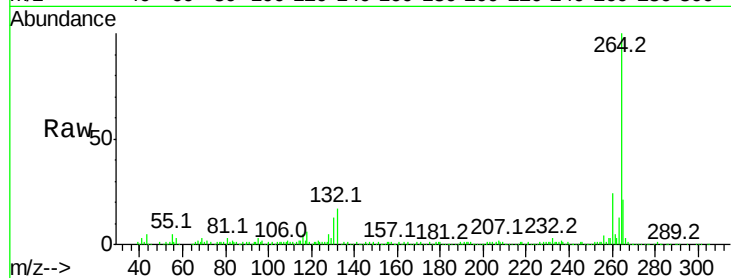

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

