

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042716\
 Data File : BF086458.D
 Acq On : 28 Apr 2016 7:37
 Operator : UM/SJ
 Sample : H2707-10
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RICHMOND-AMBOY-SB10(0.5-6.0)

Quant Time: Apr 28 11:20:31 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF042716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 27 14:20:52 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.81	152	138034	20.00	ng	0.00
21) Naphthalene-d8	8.09	136	500763	20.00	ng	-0.01
38) Acenaphthene-d10	9.85	164	179394	20.00	ng	0.00
63) Phenanthrene-d10	11.32	188	309910	20.00	ng	0.00
75) Chrysene-d12	13.95	240	327692	20.00	ng	-0.01
86) Perylene-d12	15.37	264	228784	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.40	112	1128677	141.04	ng	0.01
7) Phenol-d6	6.44	99	1534207	137.36	ng	0.00
23) Nitrobenzene-d5	7.37	82	880283	94.75	ng	-0.01
41) 2,4,6-Tribromophenol	10.64	330	243037	128.47	ng	0.00
44) 2-Fluorobiphenyl	9.17	172	1281658	142.66	ng	0.00
78) Terphenyl-d14	12.91	244	926171	62.27	ng	0.00
Target Compounds						Qvalue
49) Dimethylphthalate	9.56	163	143571	10.63	ng	99
83) Bis(2-ethylhexyl)phthalate	13.95	149	75904	5.98	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042716\
Data File : BF086458.D
Acq On : 28 Apr 2016 7:37
Operator : UM/SJ
Sample : H2707-10
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RICHMOND-AMBOY-SB10(0.5-6.0)

Quant Time: Apr 28 11:20:31 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF042716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 27 14:20:52 2016
Response via : Initial Calibration

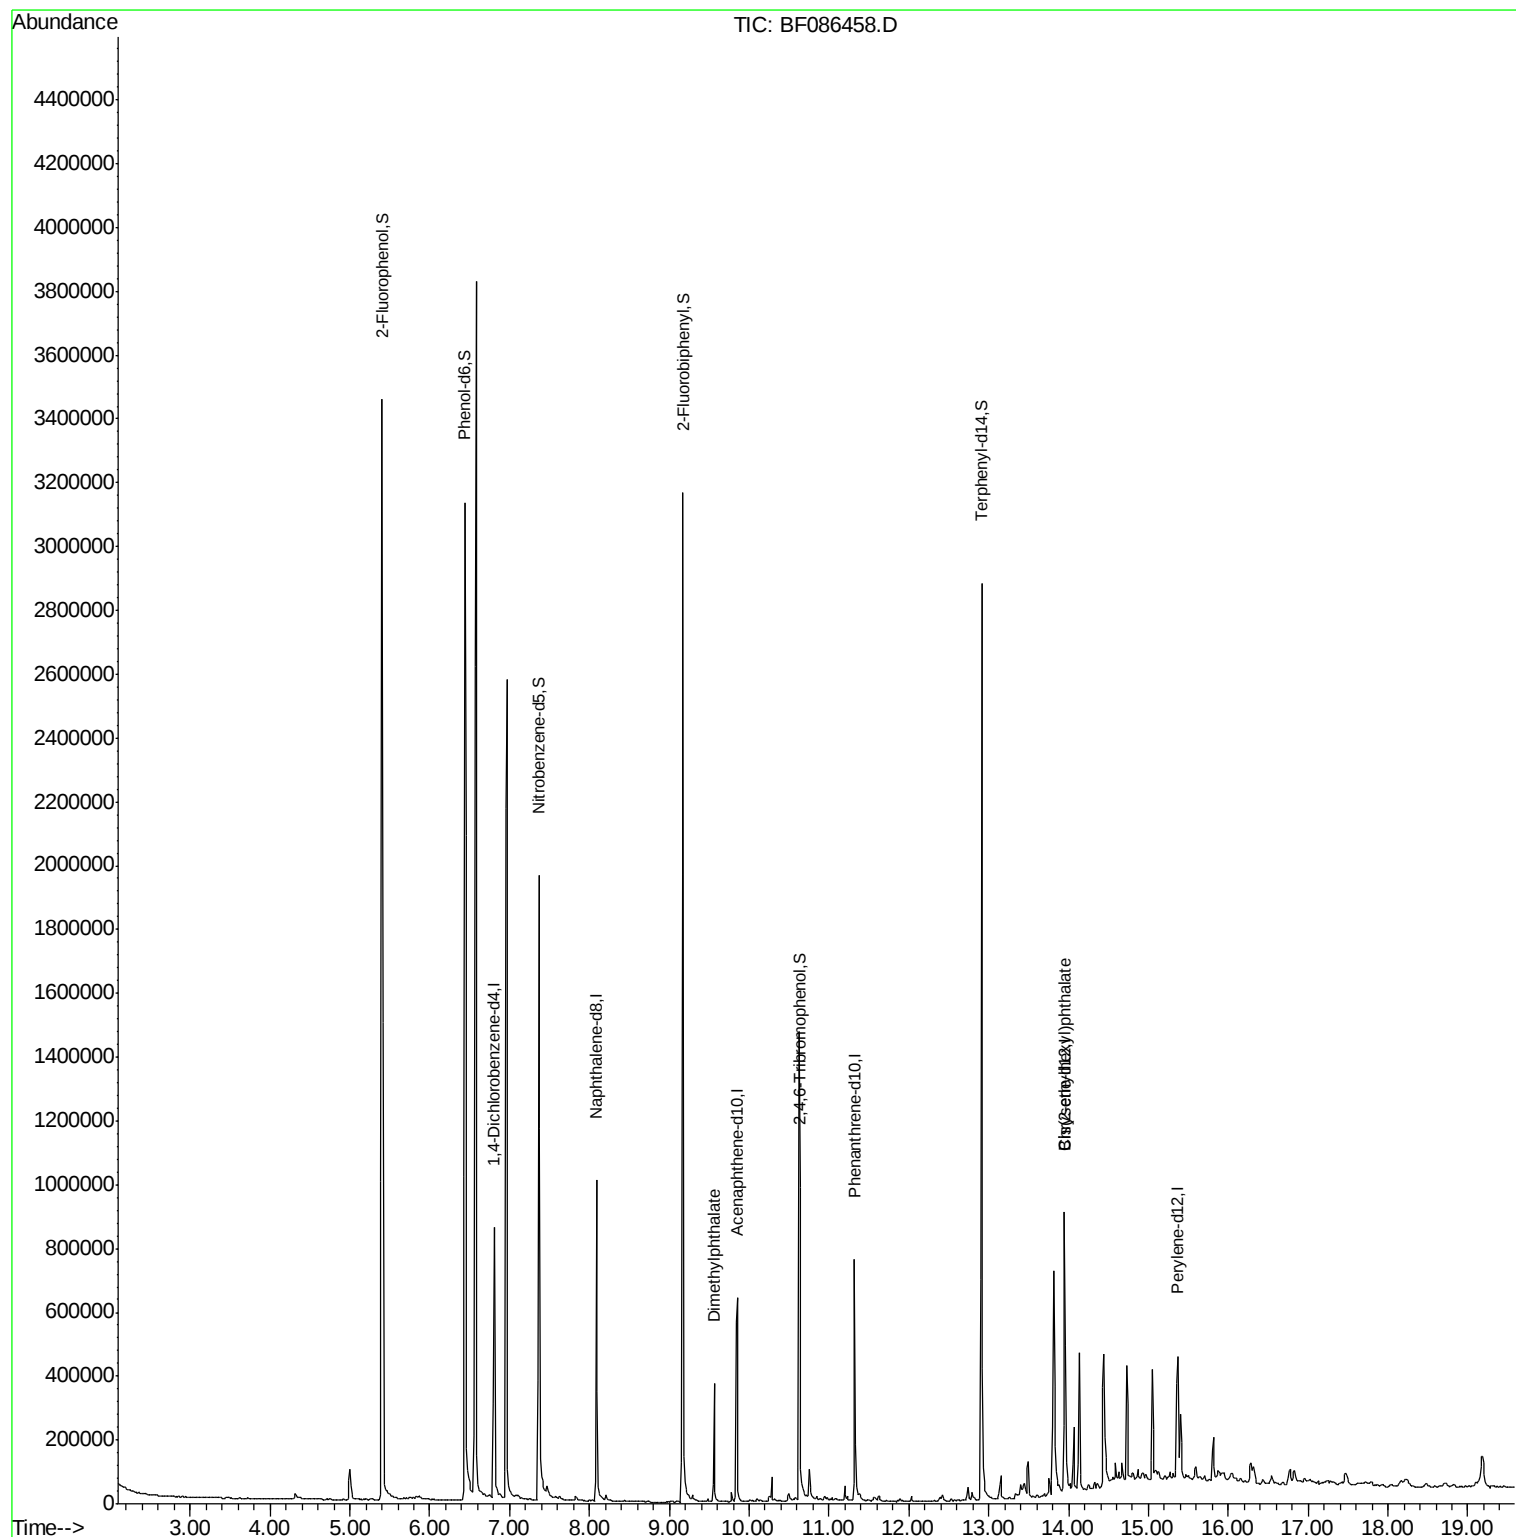



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.81 min Scan# 413

Delta R.T. 0.00 min

Lab File: BF086458.D

Acq: 28 Apr 2016 7:37

Instrument :

BNA_F

ClientSampleId :

RICHMOND-AMBOY-SB10(0.5-6.0)


Tot Ion:152 Resp: 138034

Ion Ratio Lower Upper

152 100

150 156.2 125.8 188.6




115 58.4 51.5 77.3



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

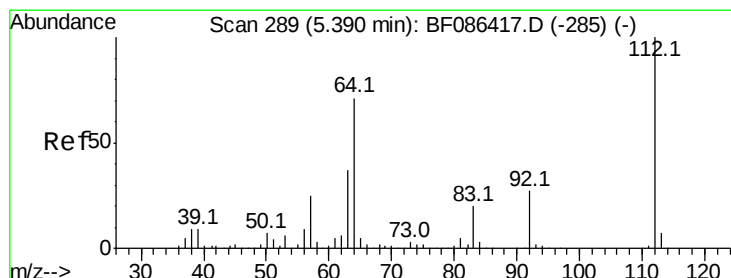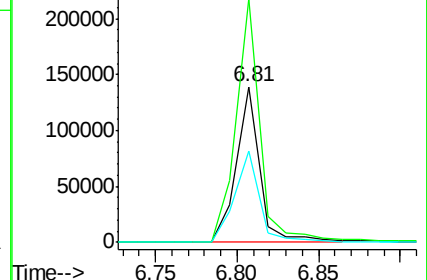

#5

2-Fluorophenol

Concen: 141.04 ng

RT: 5.40 min Scan# 290

Delta R.T. 0.01 min

Lab File: BF086458.D

Acq: 28 Apr 2016 7:37


Tgt Ion:112 Resp: 1128677

Ion Ratio Lower Upper

112 100

64 73.6 52.1 78.1



63 38.9 25.7 38.5#



Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

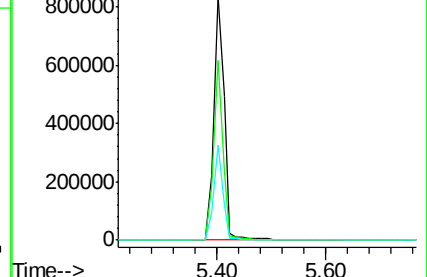



#7

Phenol-d6

Concen: 137.36 ng

RT: 6.44 min Scan# 381

Delta R.T. 0.00 min

Lab File: BF086458.D

Acq: 28 Apr 2016 7:37

Instrument :





BNA_F

ClientSampleId :

RICHMOND-AMBOY-SB10(0.5-6.0)

Tot Ion: 99 Resp: 1534207

Ion	Ratio	Lower	Upper
99	100		
42	28.1	13.6	20.4#
71	36.1	24.6	36.8

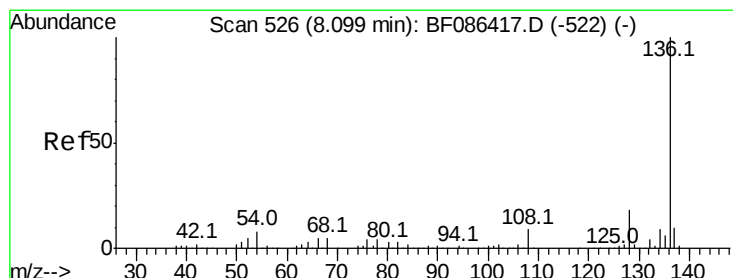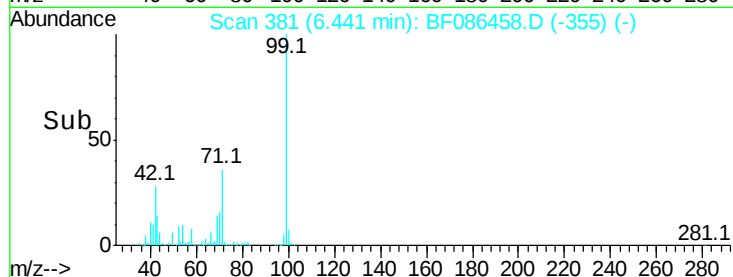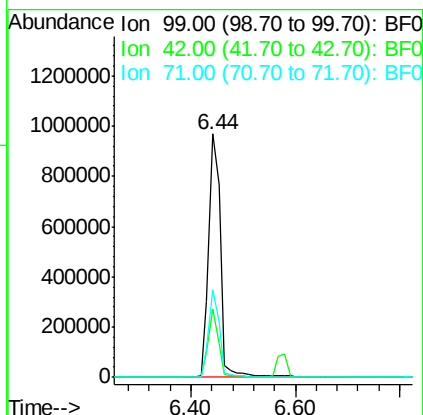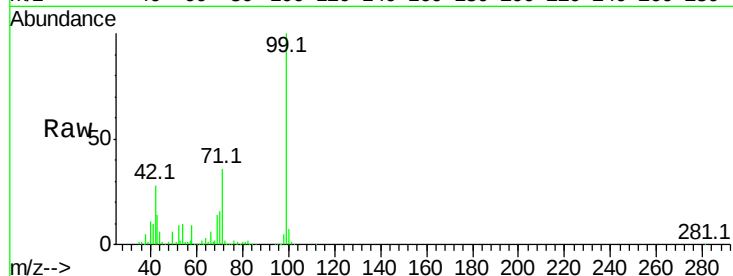

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.09 min Scan# 525




Delta R.T. -0.01 min


Lab File: BF086458.D

Acq: 28 Apr 2016 7:37

Tgt Ion: 136 Resp: 500763

Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.8	13.2
54	14.1	5.0	7.4#
68	7.9	4.4	6.6#


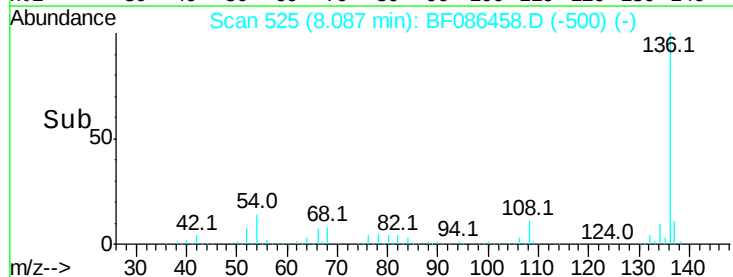
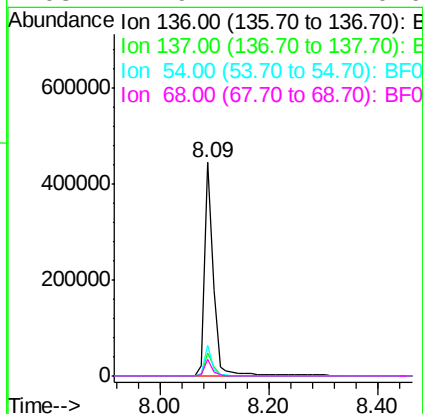
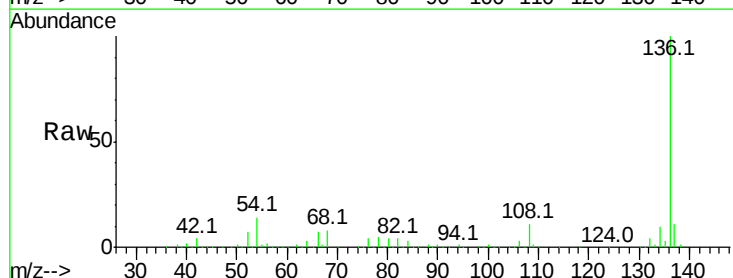


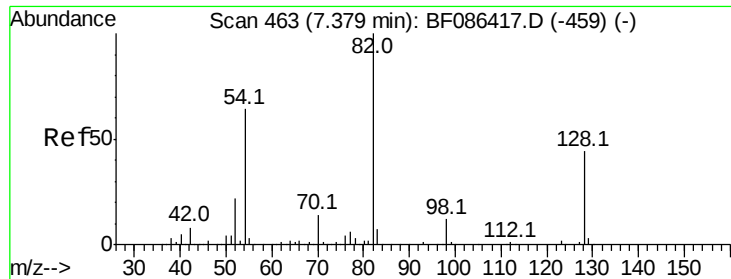

#23
Nitrobenzene-d5
Concen: 94.75 ng
RT: 7.37 min Scan# 462
Delta R.T. -0.01 min
Lab File: BF086458.D
Acq: 28 Apr 2016 7:37




Instrument :
BNA_F
ClientSampleId :
RICHMOND-AMBOY-SB10(0.5-6.0)


Tot Ion	82	Resp	880283
Ion Ratio	100	Lower	Upper
128	38.8	40.6	61.0#
54	69.6	38.1	57.1#

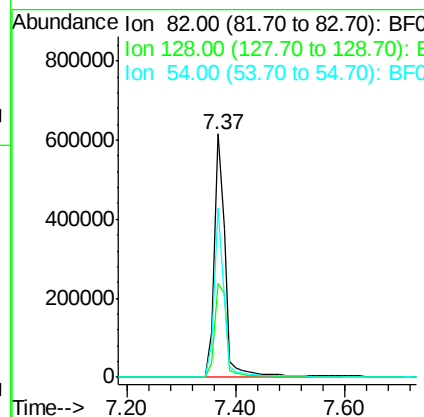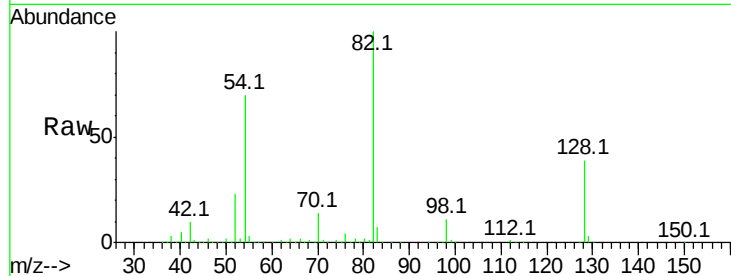

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.85 min Scan# 679
Delta R.T. 0.00 min
Lab File: BF086458.D
Acq: 28 Apr 2016 7:37

Tgt Ion	164	Resp	179394
Ion Ratio	100	Lower	Upper
162	106.7	82.8	124.2
160	48.7	36.9	55.3

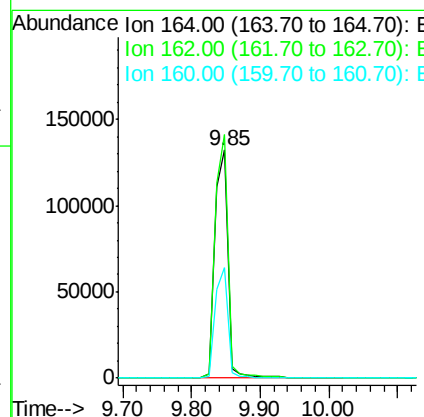







#41
 2,4,6-Tribromophenol
 Concen: 128.47 ng
 RT: 10.64 min Scan# 748
 Delta R.T. 0.00 min
 Lab File: BF086458.D
 Acq: 28 Apr 2016 7:37

Instrument :
 BNA_F
 ClientSampleId :
 RICHMOND-AMBOY-SB10(0.5-6.0)

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.3	79.0	118.4
141	32.5	31.2	46.8

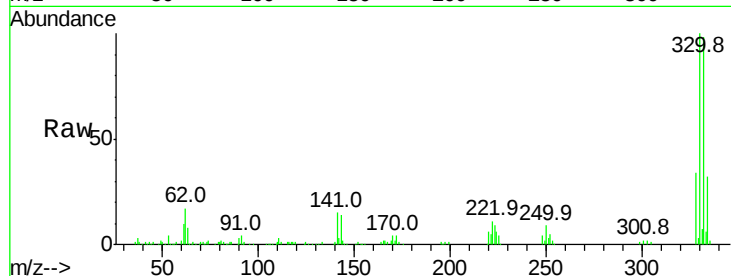


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


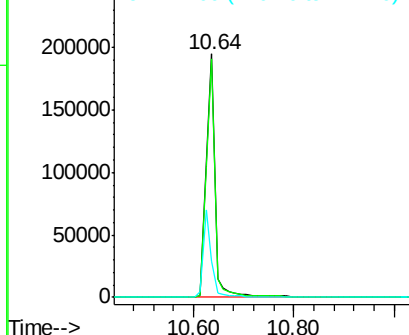



#44
 2-Fluorobiphenyl
 Concen: 142.66 ng
 RT: 9.17 min Scan# 620
 Delta R.T. 0.00 min
 Lab File: BF086458.D
 Acq: 28 Apr 2016 7:37

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.7	29.0	43.6
170	24.6	19.8	29.8



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

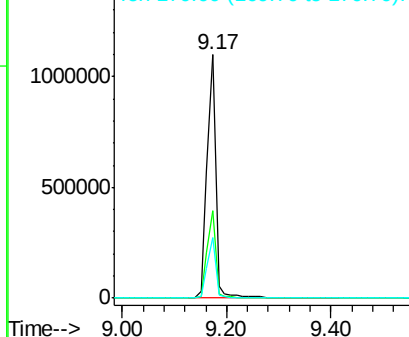

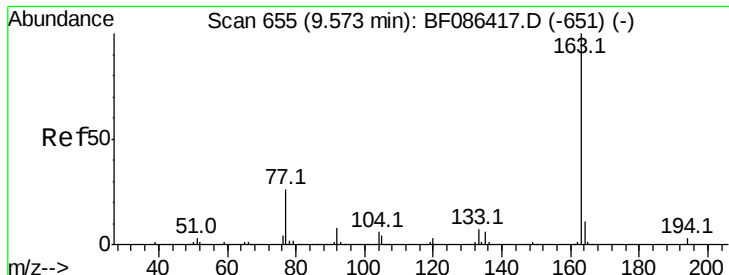

#49

Dimethylphthalate

Concen: 10.63 ng

RT: 9.56 min Scan# 654

Delta R.T. -0.01 min

Lab File: BF086458.D

Acq: 28 Apr 2016 7:37

Instrument :

BNA_F

ClientSampleId :

RICHMOND-AMBOY-SB10(0.5-6.0)


Tot Ion:163 Resp: 143571

Ion Ratio Lower Upper

163 100

194 3.2 2.6 4.0




164 9.7 8.2 12.4

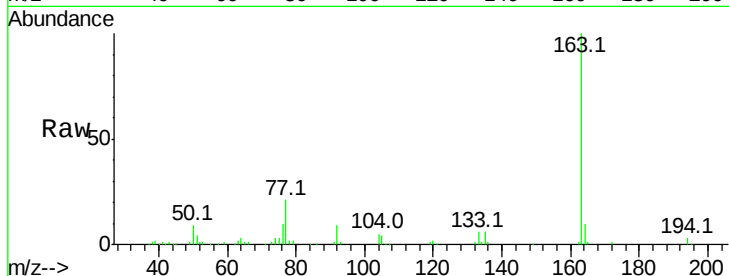

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

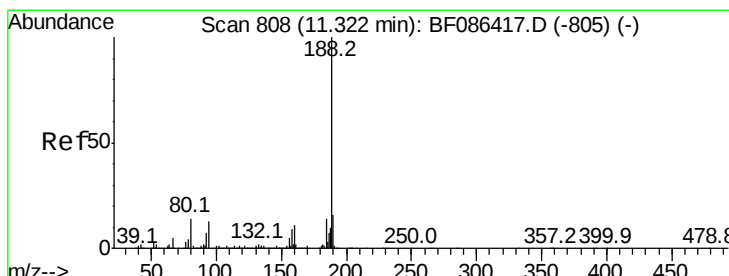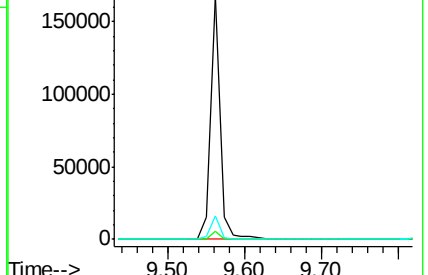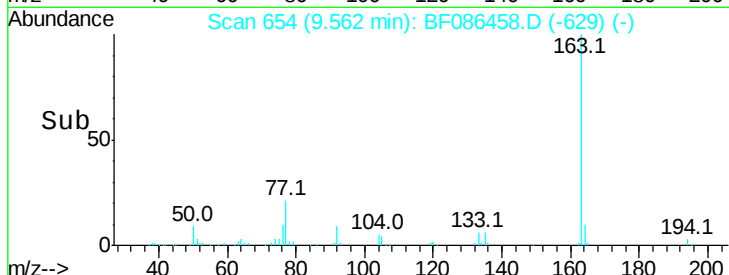

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.32 min Scan# 808

Delta R.T. 0.00 min

Lab File: BF086458.D

Acq: 28 Apr 2016 7:37


Tgt Ion:188 Resp: 309910

Ion Ratio Lower Upper

188 100

94 11.7 6.8 10.2#



80 12.9 7.1 10.7#

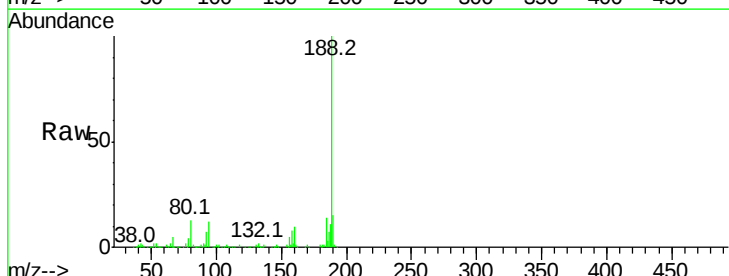


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

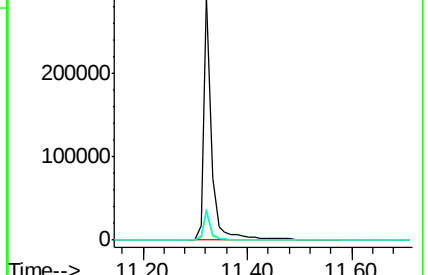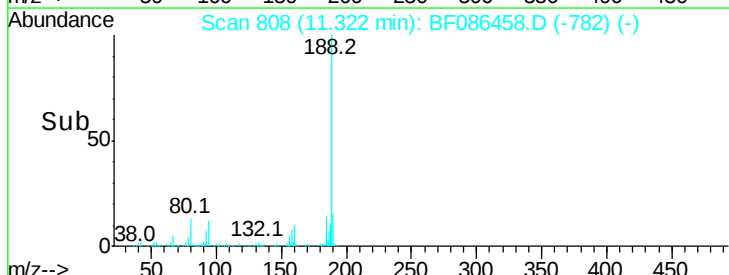

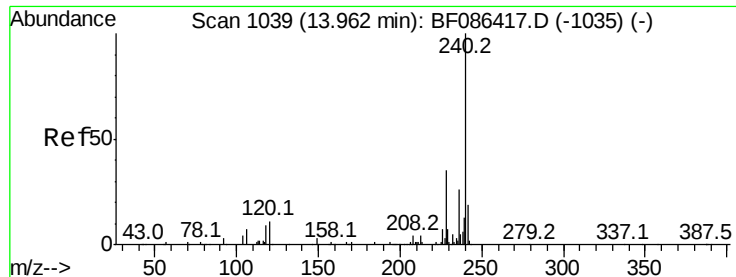

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.95 min Scan# 1038

Delta R.T. -0.01 min

Lab File: BF086458.D

Acq: 28 Apr 2016 7:37

Instrument :

BNA_F

ClientSampleId :

RICHMOND-AMBOY-SB10(0.5-6.0)


Tot Ion:240 Resp: 327692

Ion Ratio Lower Upper

240 100

120 17.3 11.2 16.8#




236 26.5 21.2 31.8

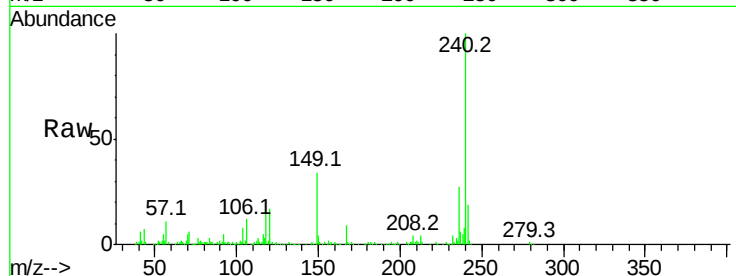

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

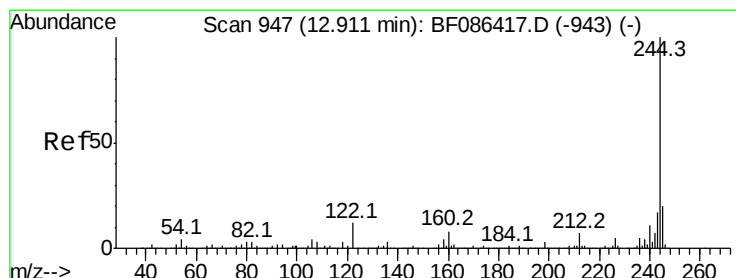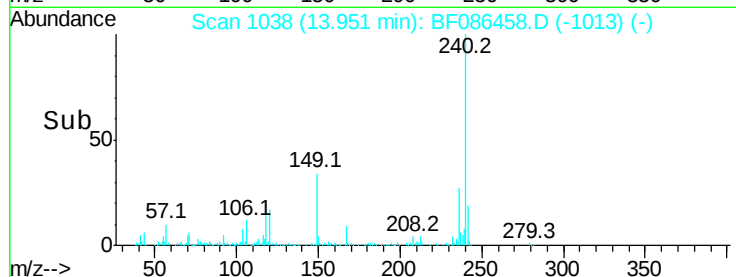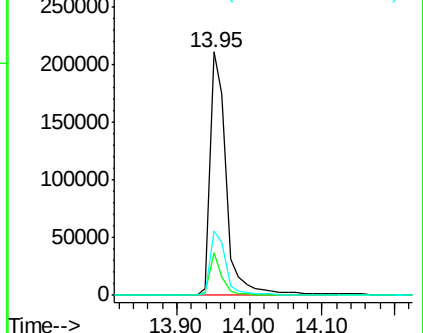

#78

Terphenyl-d14

Concen: 62.27 ng

RT: 12.91 min Scan# 947

Delta R.T. 0.00 min

Lab File: BF086458.D

Acq: 28 Apr 2016 7:37


Tgt Ion:244 Resp: 926171

Ion Ratio Lower Upper

244 100

212 7.7 6.2 9.2



122 13.6 12.0 18.0

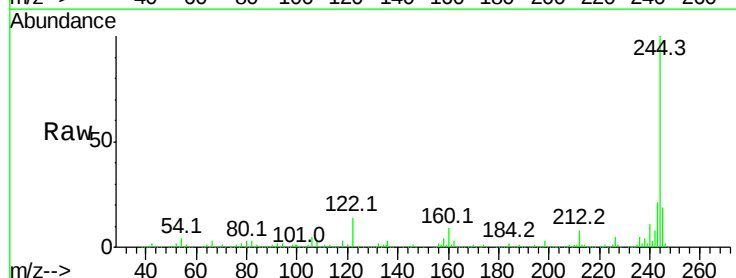


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

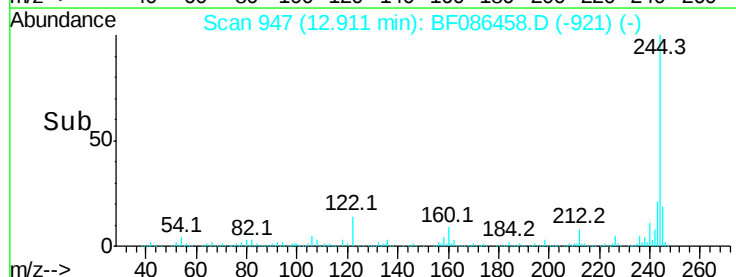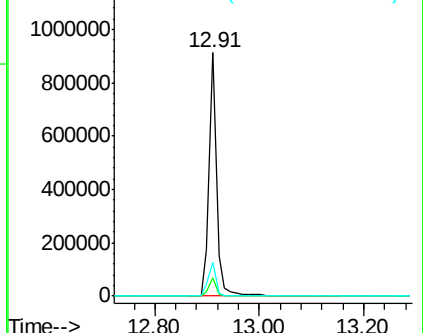



#83

Bis(2-ethylhexyl)phthalate

Concen: 5.98 ng

RT: 13.95 min Scan# 1038

Delta R.T. 0.00 min

Lab File: BF086458.D

Acq: 28 Apr 2016 7:37

Instrument :

BNA_F

ClientSampleId :

RICHMOND-AMBOY-SB10(0.5-6.0)


Tot Ion:149 Resp: 75904

Ion Ratio Lower Upper




149 100

167 26.1 21.8 32.6

279 3.6 2.6 4.0



Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E

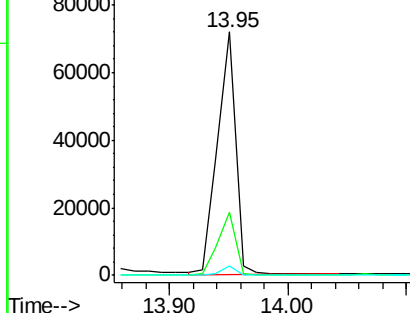

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.37 min Scan# 1162

Delta R.T. 0.01 min

Lab File: BF086458.D

Acq: 28 Apr 2016 7:37


Tgt Ion:264 Resp: 228784

Ion Ratio Lower Upper

264 100

260 24.4 19.5 29.3

265 21.8 17.3 25.9



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

