


Data Path : Z:\HPCHEM1\BNA F\Data\BF042716\
 Data File : BF086413.D
 Acq On : 27 Apr 2016 9:59
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 27 14:20:52 2016

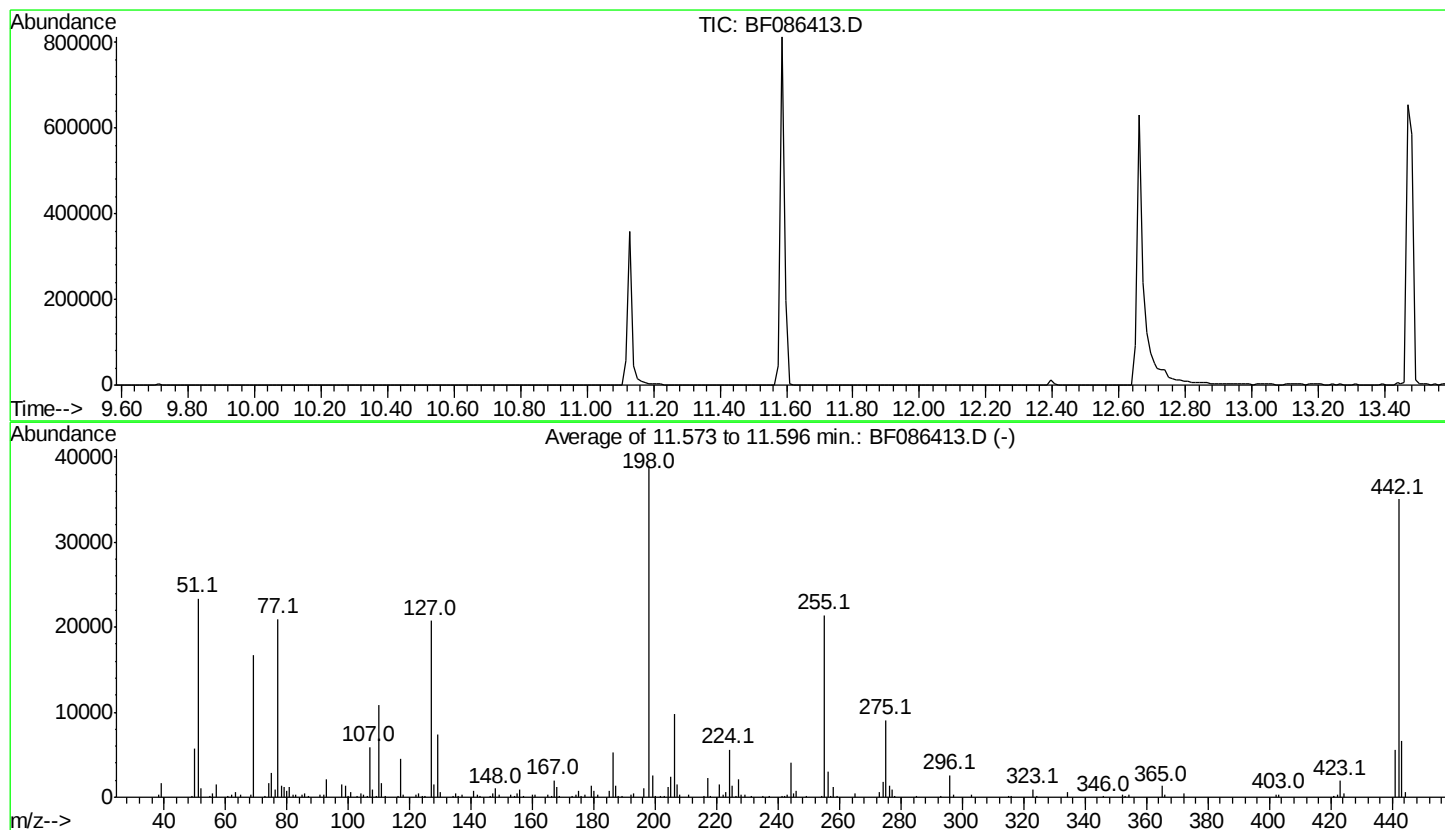

AutoFind: Scans 830, 831, 832; Background Corrected with Scan 827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.0	23392	PASS
68	69	0.00	2	1.6	260	PASS
69	198	0.00	100	42.8	16674	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.2	20729	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38986	PASS
199	198	5	9	6.4	2503	PASS
275	198	10	60	23.3	9072	PASS
365	198	1	100	3.5	1350	PASS
441	442	0.01	24	15.8	5553	PASS
442	198	50	100	89.9	35056	PASS
443	442	15	24	18.8	6598	PASS