


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042716\
 Data File : BF086450.D
 Acq On : 28 Apr 2016 3:49
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 27 14:20:52 2016

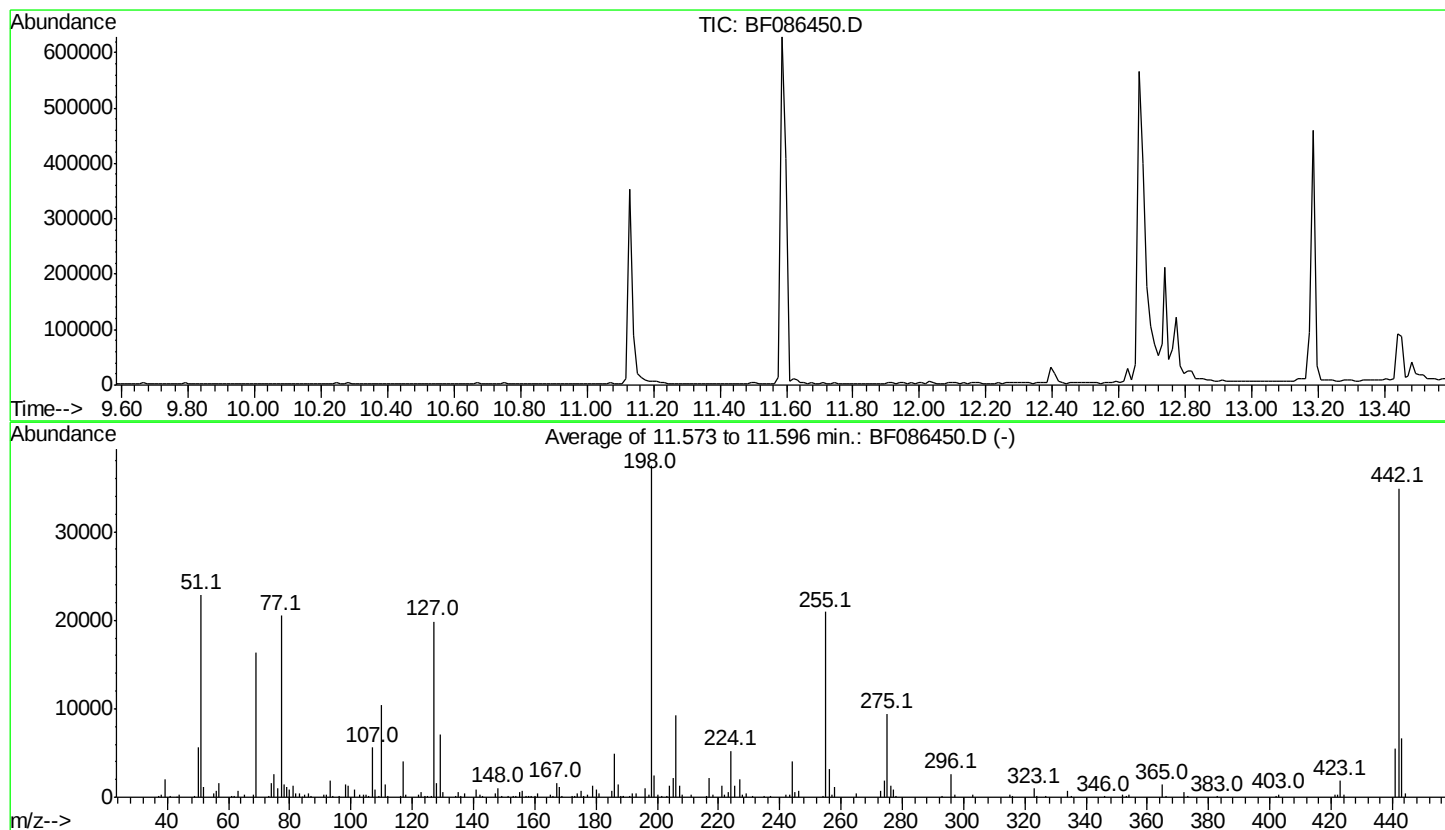

AutoFind: Scans 830, 831, 832; Background Corrected with Scan 827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.0	22866	PASS
68	69	0.00	2	1.7	271	PASS
69	198	0.00	100	43.6	16322	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.1	19890	PASS
197	198	0.00	2	0.9	346	PASS
198	198	100	100	100.0	37474	PASS
199	198	5	9	6.6	2455	PASS
275	198	10	60	25.1	9413	PASS
365	198	1	100	3.7	1391	PASS
441	442	0.01	24	15.7	5461	PASS
442	198	50	100	93.1	34889	PASS
443	442	15	24	19.2	6689	PASS