
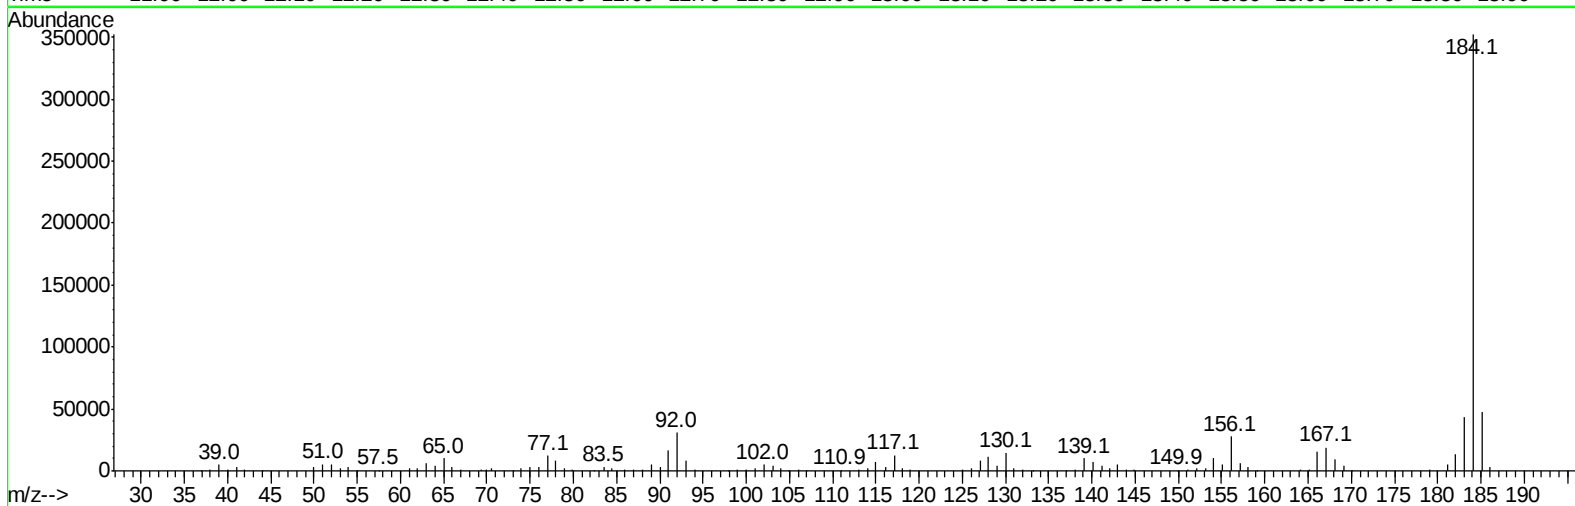


Data Path : Z:\HPCHEM1\BNA F\DATA\BF042717\
Data File : BF094664.D
Acq On : 27 Apr 2017 13:35
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 07:19:53 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

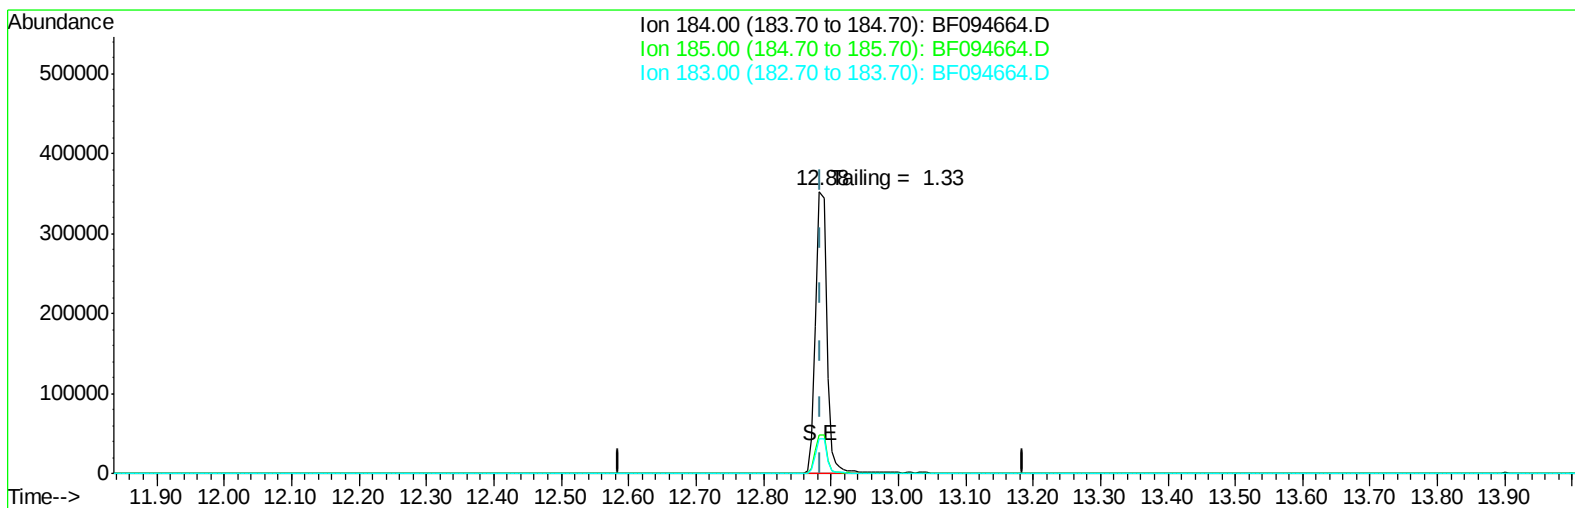

TIC: BF094664.D

(76) Benzidine



12.883min (-0.003) 69152.16ng

response 397594

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.51#
183.00	12.20	12.35
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042717\
Data File : BF094664.D
Acq On : 27 Apr 2017 13:35
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 07:19:53 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

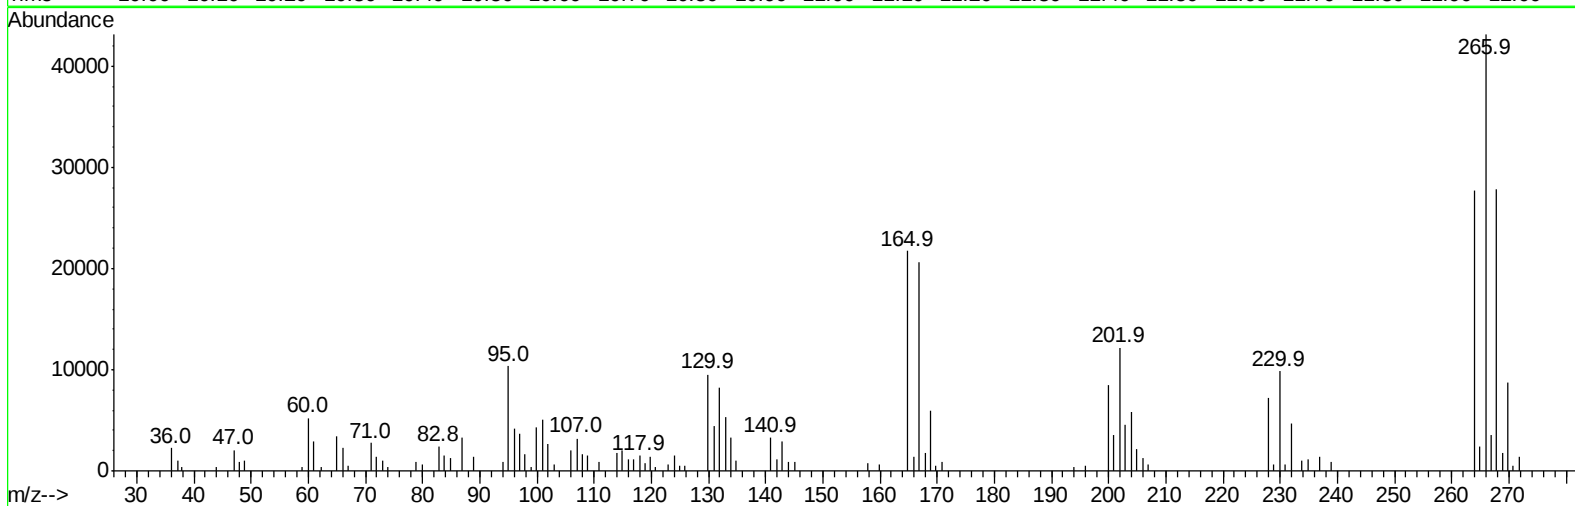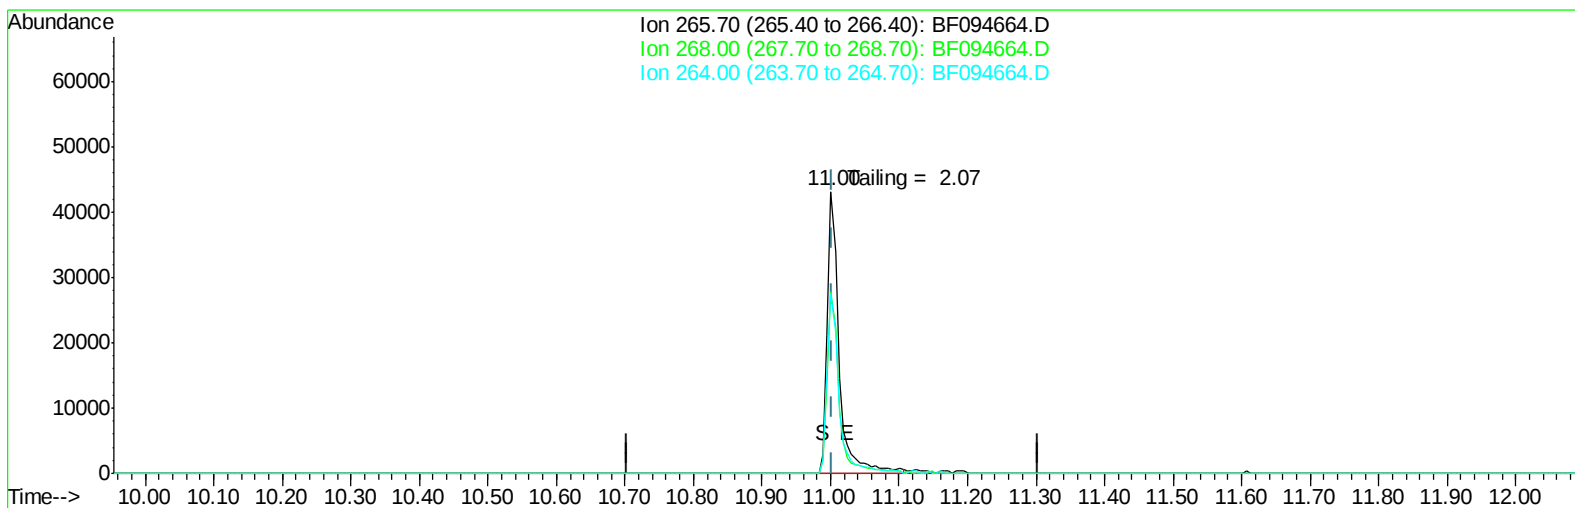

TIC: BF094664.D

(69) Pentachlorophenol (C)

11.001min (-0.003) 0.00ng

response 49910

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.58
264.00	64.60	64.11
0.00	0.00	0.00