


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042717\
 Data File : BF094664.D
 Acq On : 27 Apr 2017 13:35
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF041717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 17 14:59:23 2017

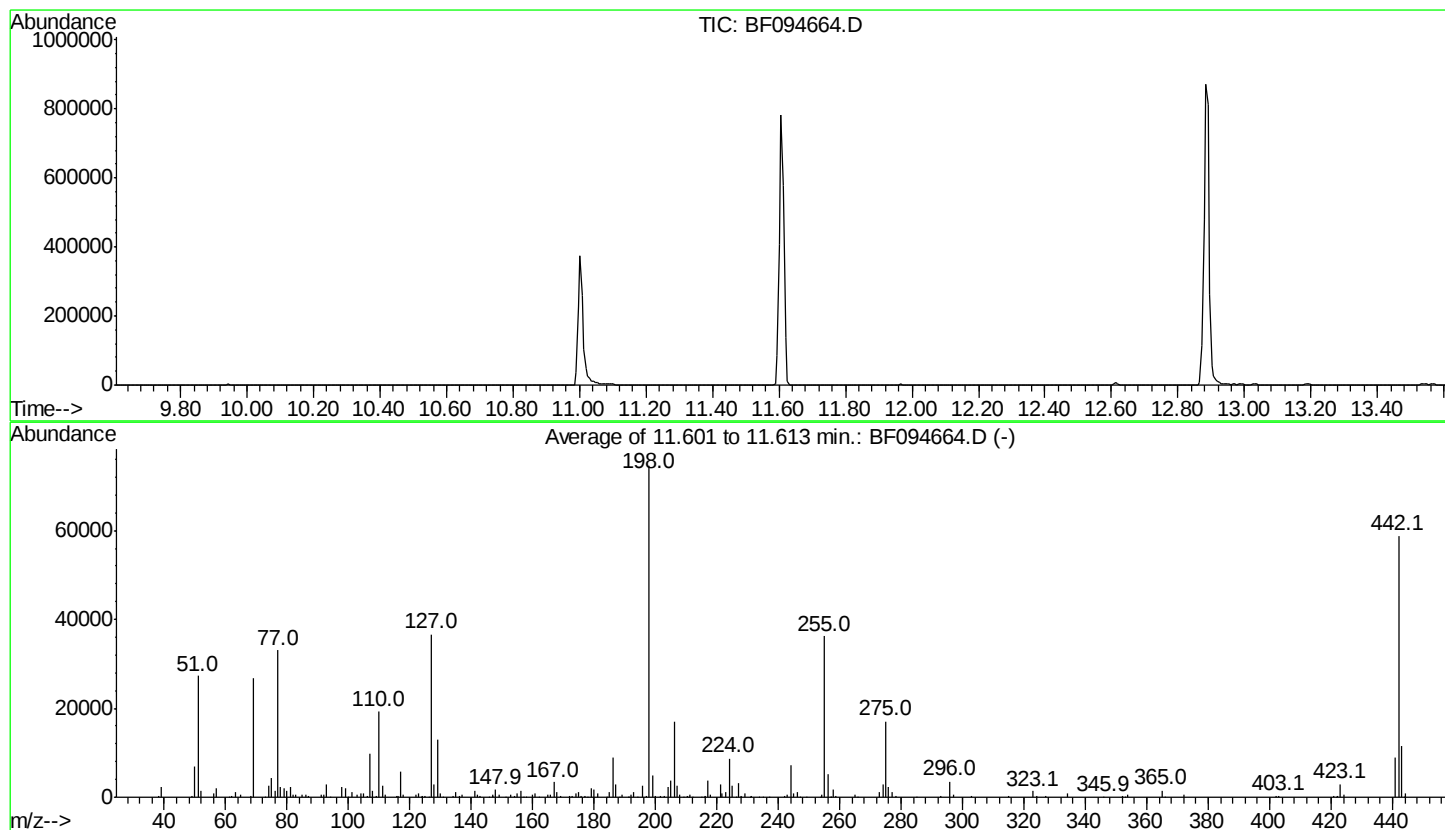

AutoFind: Scans 1643, 1644, 1645; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	27237	PASS
68	69	0.00	2	1.5	405	PASS
69	198	0.00	100	36.0	26864	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.2	36698	PASS
197	198	0.00	2	0.3	237	PASS
198	198	100	100	100.0	74586	PASS
199	198	5	9	6.5	4830	PASS
275	198	10	60	22.9	17098	PASS
365	198	1	100	2.0	1505	PASS
441	442	0.01	24	15.3	8985	PASS
442	198	50	100	78.9	58861	PASS
443	442	15	24	19.7	11618	PASS