
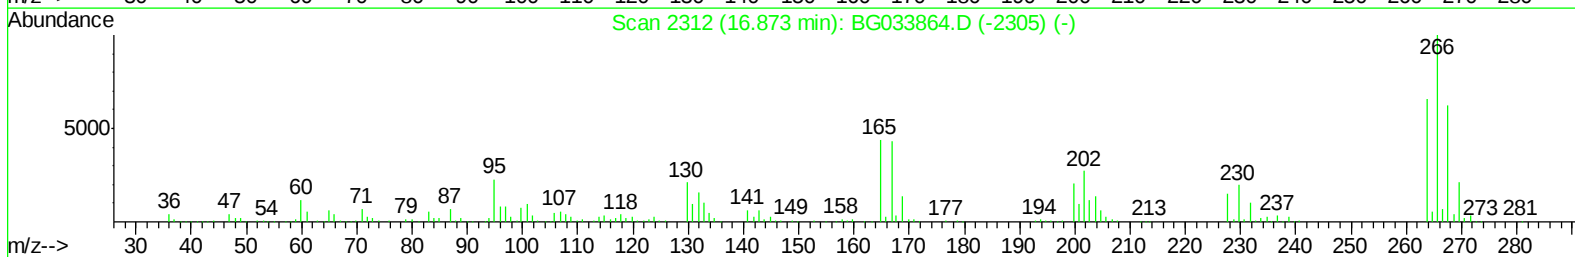
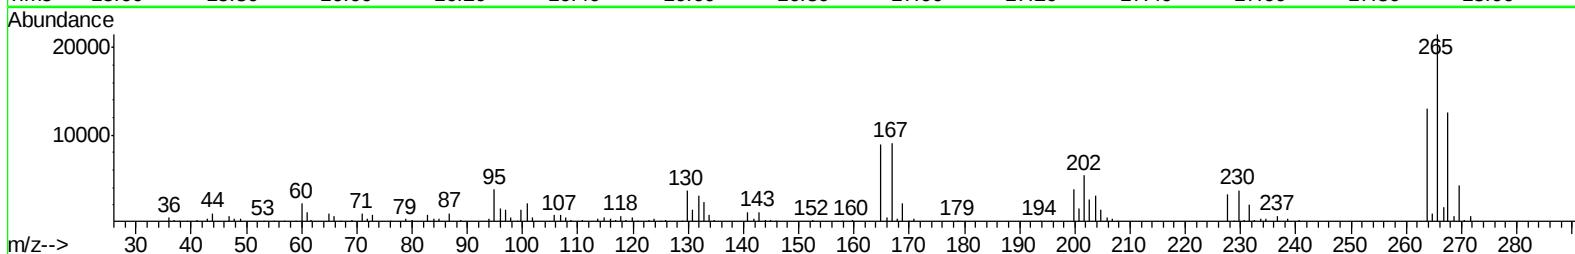


Data Path : Z:\HPCHEM1\BNA G\DATA\BG042718\
Data File : BG034037.D
Acq On : 27 Apr 2018 13:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 05:57:08 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 19 13:56:22 2018
Response via : Initial Calibration

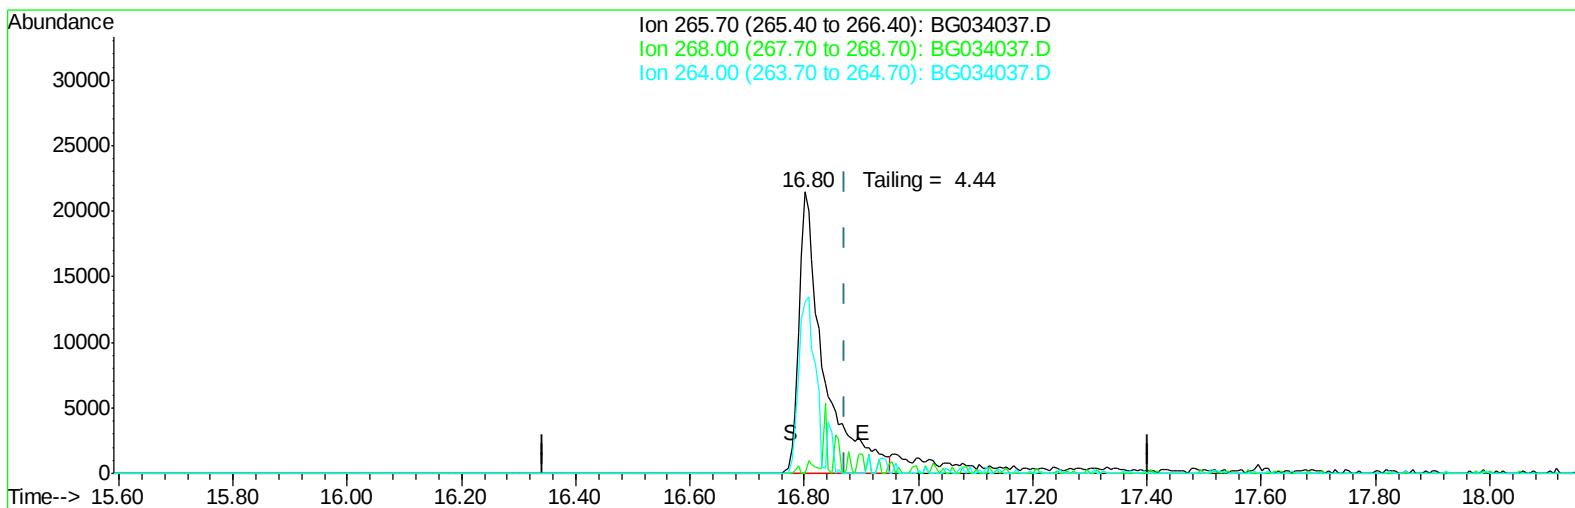

TIC: BG034037.D

(69) Pentachlorophenol (C)

16.801min (-0.072) 18724.24ng

response 64471

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	3.36#
264.00	62.00	65.31
0.00	0.00	0.00