
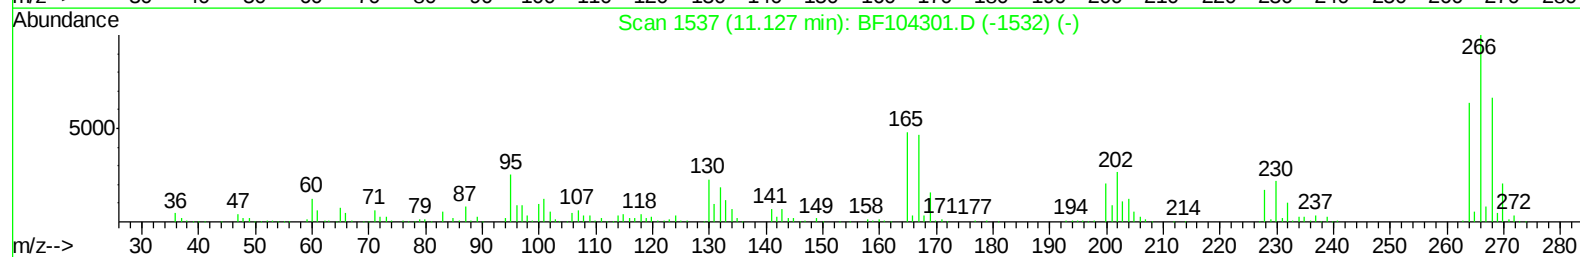
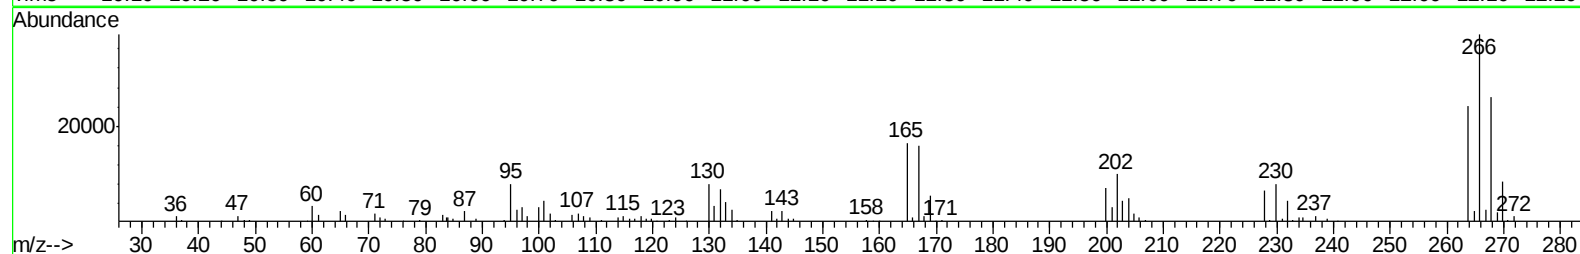


Data Path : Z:\HPCHEM1\BNA F\Data\BF042718\
Data File : BF104879.D
Acq On : 27 Apr 2018 12:55
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 03:46:56 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 17:16:11 2018
Response via : Initial Calibration

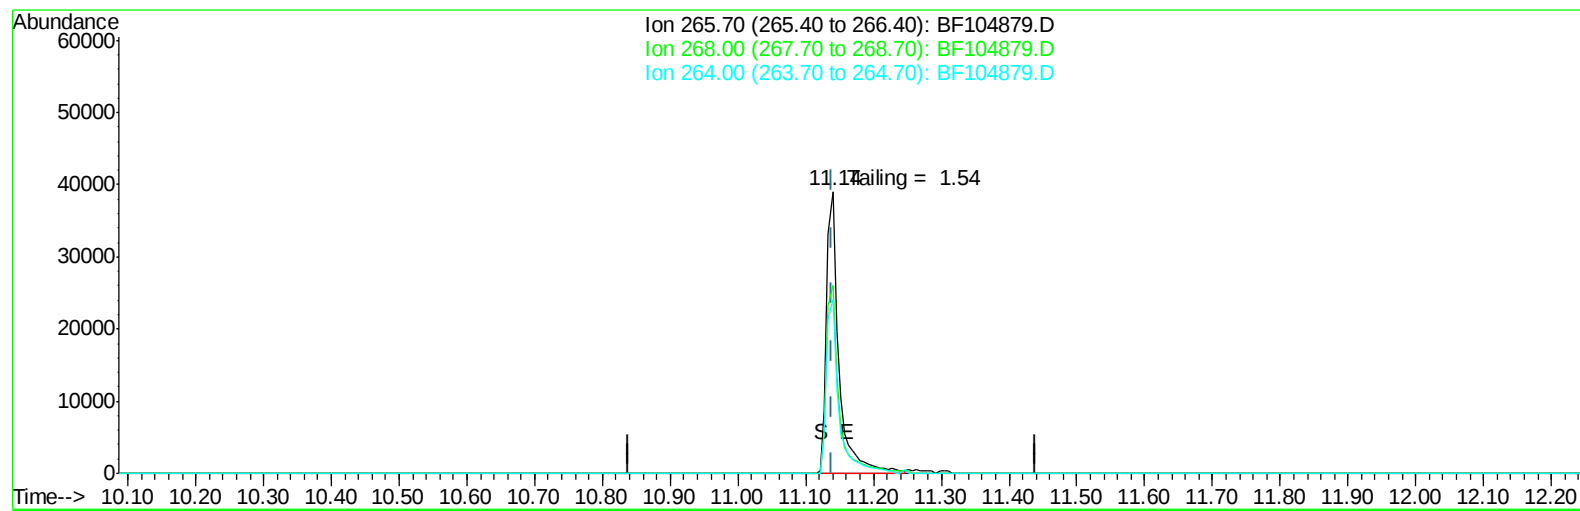

TIC: BF104879.D

(69) Pentachlorophenol (C)




11.139min (+0.000) 27527.79ng

response 48307

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.97
264.00	61.90	61.76
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF042718\
 Data File : BF104879.D
 Acq On : 27 Apr 2018 12:55
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 03:46:56 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 27 17:16:11 2018
 Response via : Initial Calibration

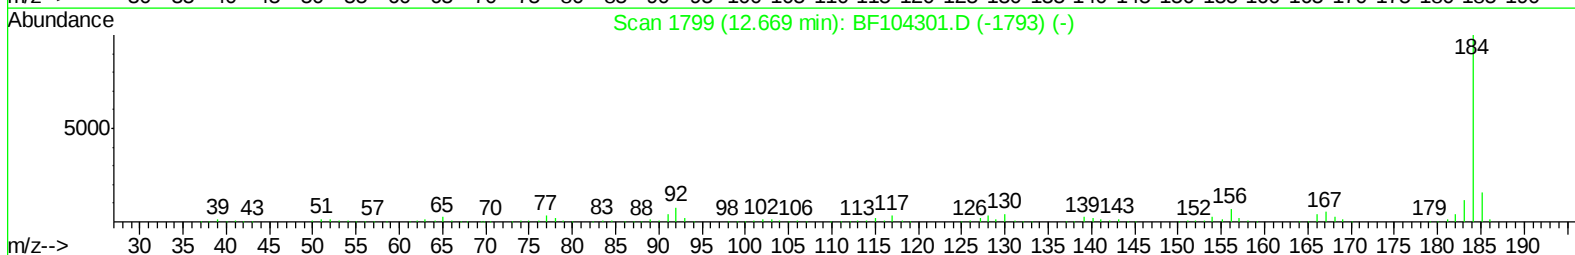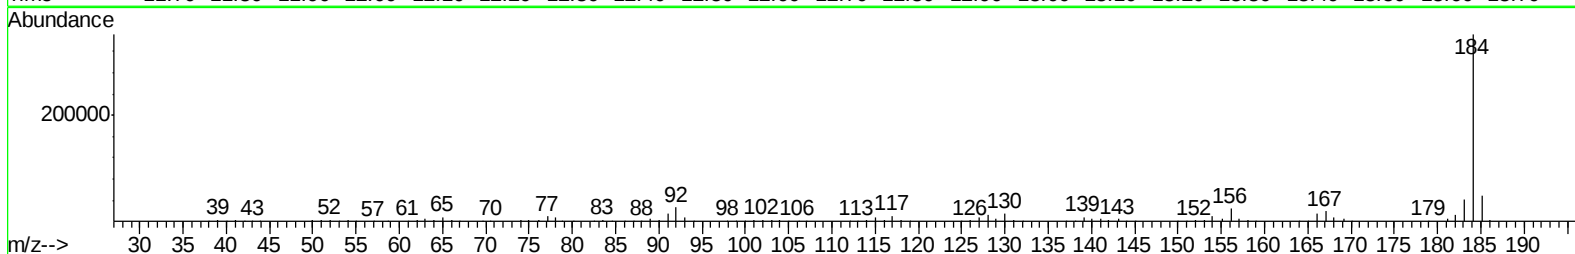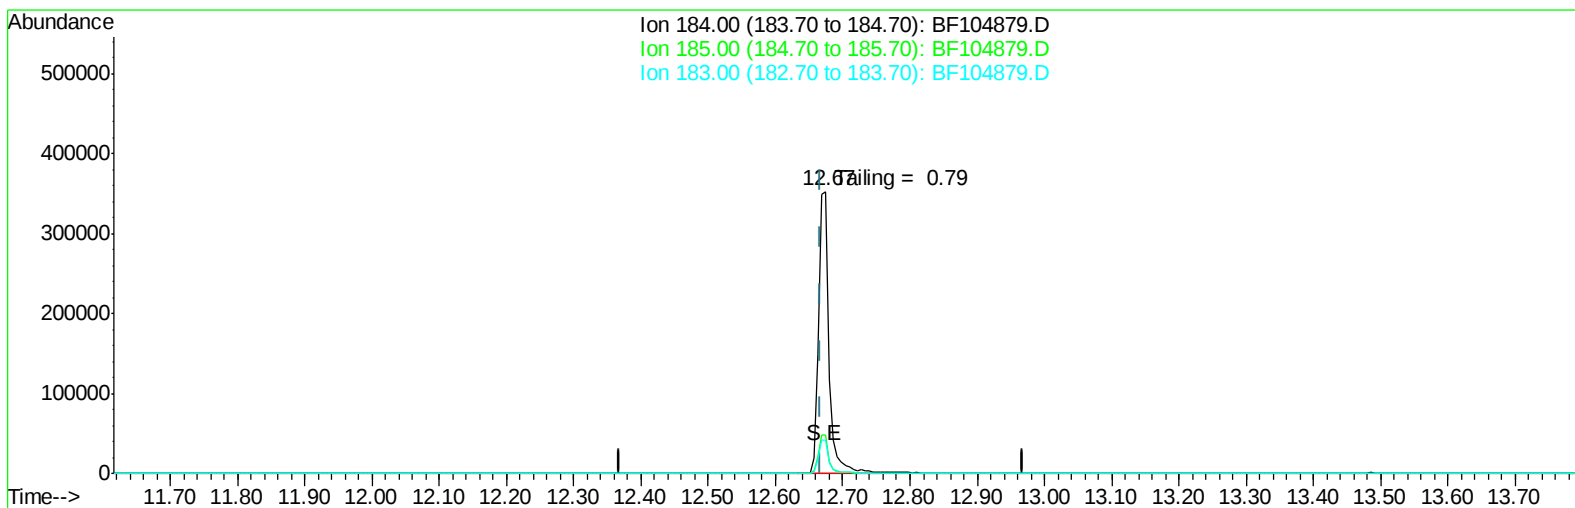

TIC: BF104879.D

(76) Benzidine

12.675min (+0.006) 0.00ng

response 393771

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.52
183.00	11.60	11.64
0.00	0.00	0.00