
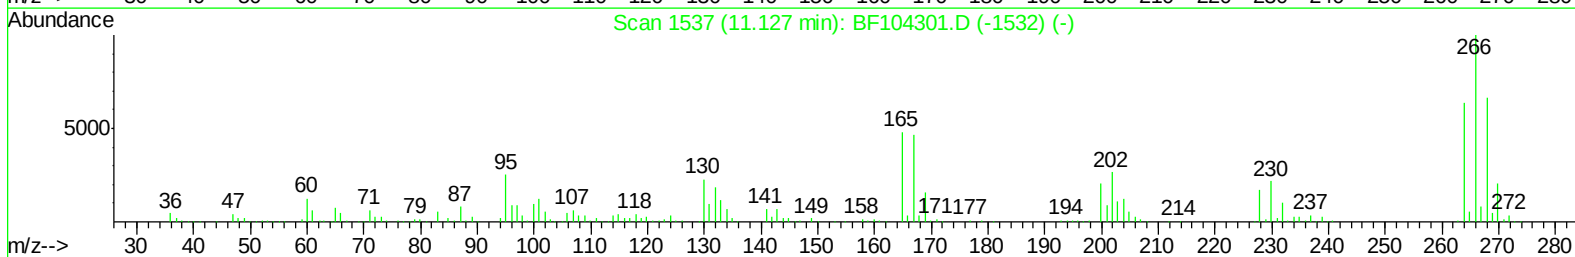
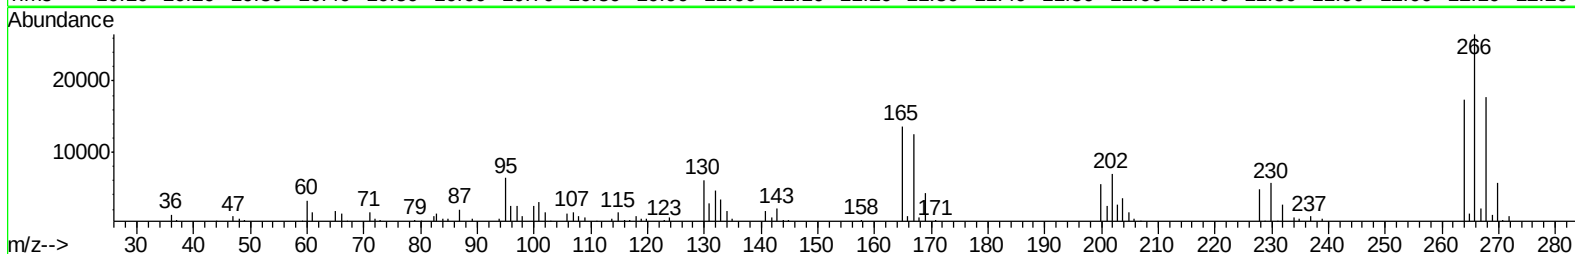


Data Path : Z:\HPCHEM1\BNA F\Data\BF042718\
Data File : BF104903.D
Acq On : 28 Apr 2018 2:00
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 04:12:59 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 17:16:11 2018
Response via : Initial Calibration

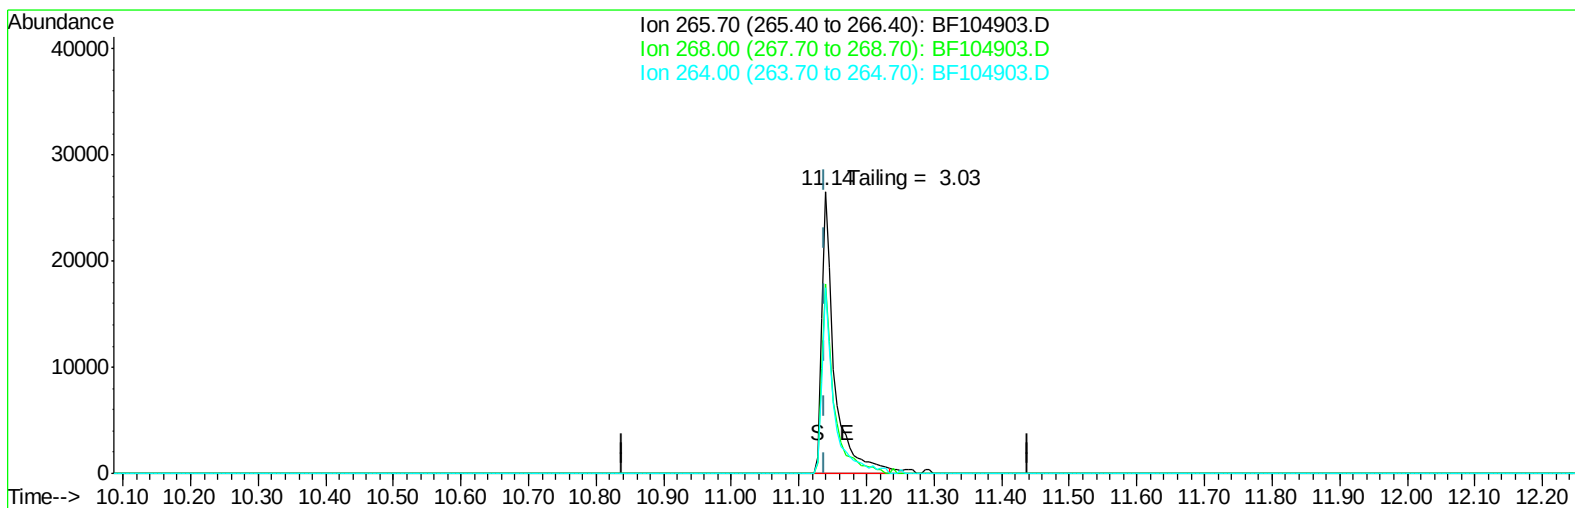

TIC: BF104903.D

(69) Pentachlorophenol (C)




11.139min (+0.000) 36710.98ng

response 35337

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.13
264.00	61.90	65.77
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF042718\
Data File : BF104903.D
Acq On : 28 Apr 2018 2:00
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 04:12:59 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 27 17:16:11 2018
Response via : Initial Calibration

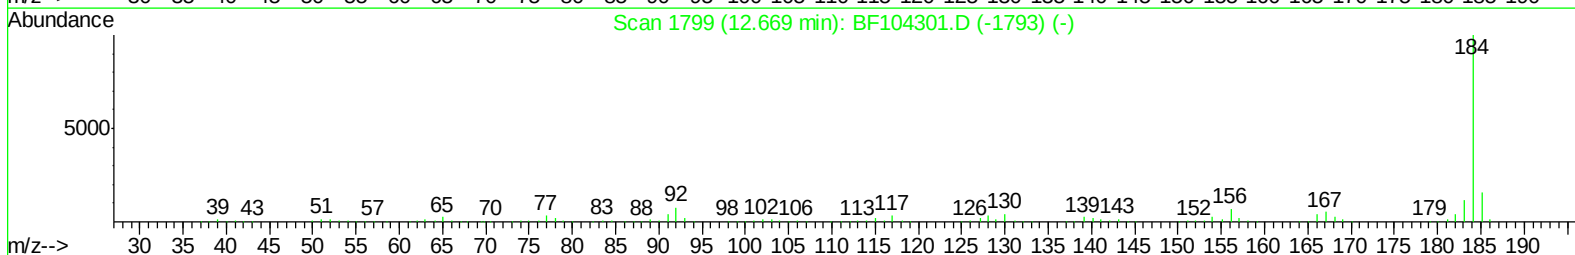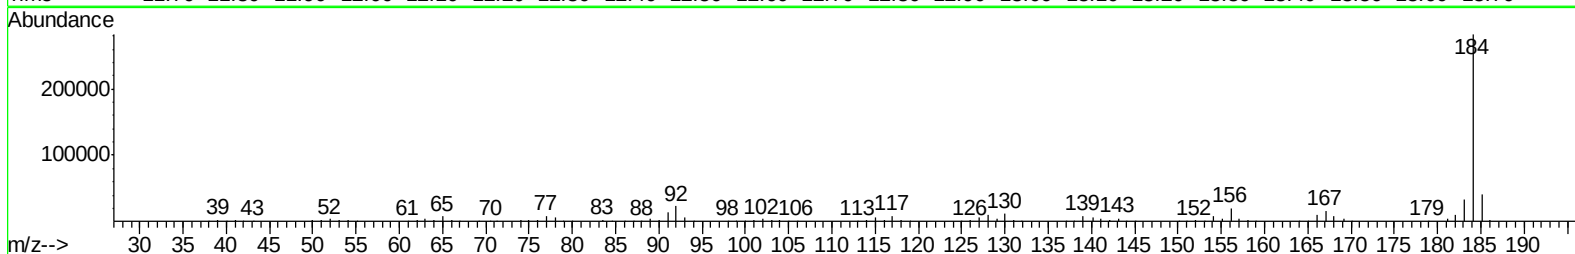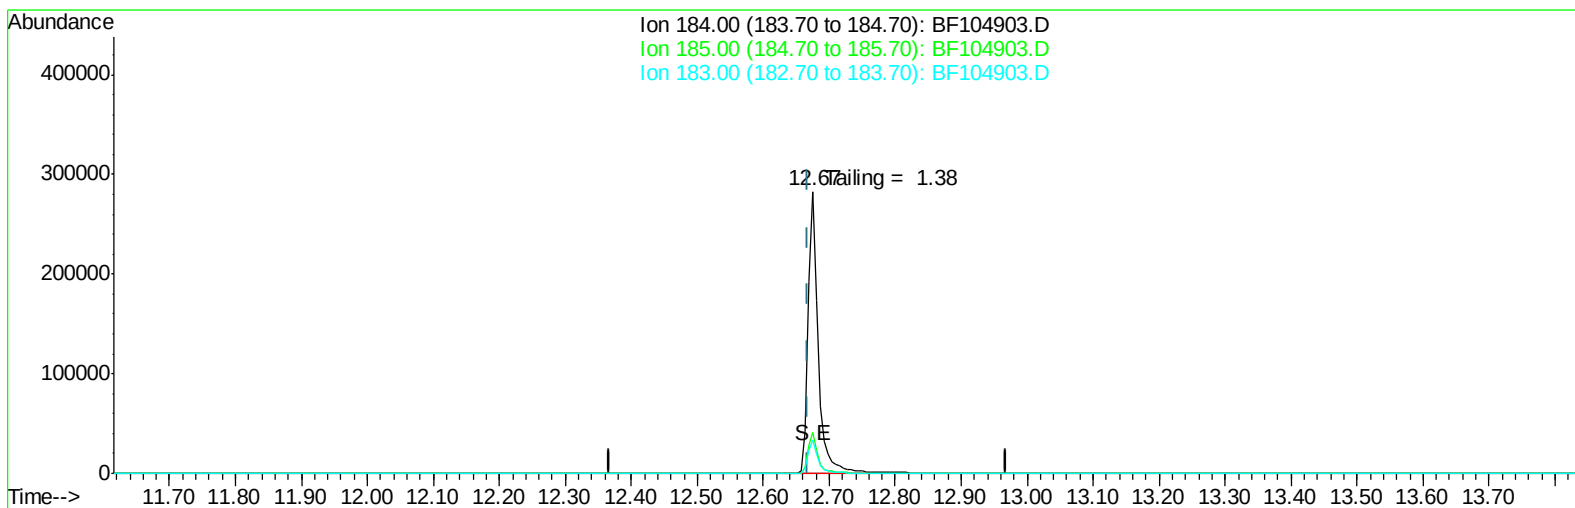

TIC: BF104903.D

(76) Benzidine

12.674min (+0.006) 0.00ng

response 308204

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.41
183.00	11.60	11.73
0.00	0.00	0.00