


Data Path : Z:\HPCHEM1\BNA F\Data\BF042718\
 Data File : BF104879.D
 Acq On : 27 Apr 2018 12:55
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 30 15:20:08 2018

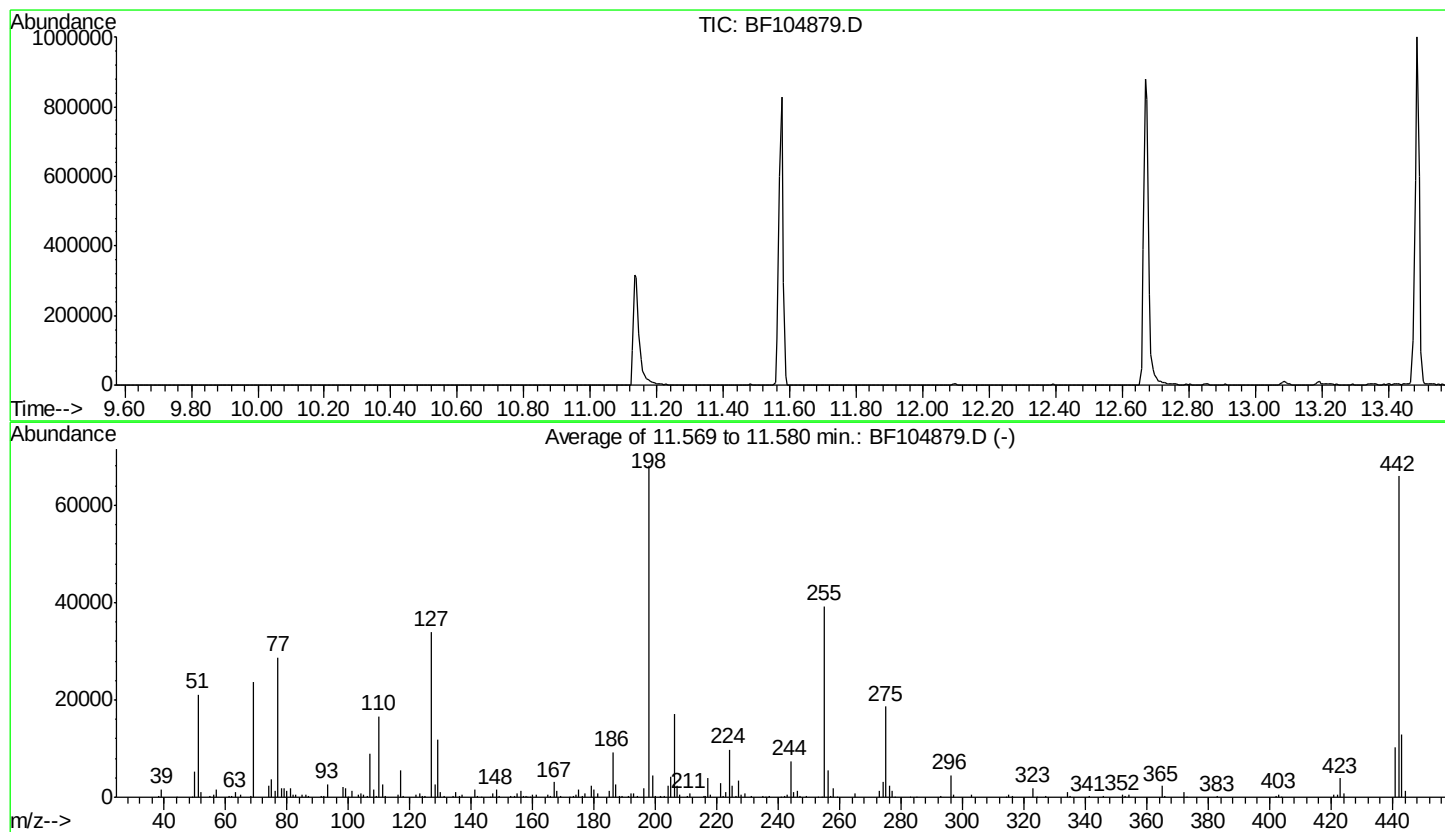

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.0	21132	PASS
68	69	0.00	2	1.7	394	PASS
69	198	0.00	100	34.8	23721	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.8	33953	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	68130	PASS
199	198	5	9	6.5	4443	PASS
275	198	10	60	27.3	18608	PASS
365	198	1	100	3.4	2350	PASS
441	443	0.01	100	79.3	10272	PASS
442	198	50	100	96.7	65896	PASS
443	442	15	24	19.7	12956	PASS