


Data Path : Z:\HPCHEM1\BNA F\Data\BF042718\
 Data File : BF104903.D
 Acq On : 28 Apr 2018 2:00
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 30 15:20:08 2018

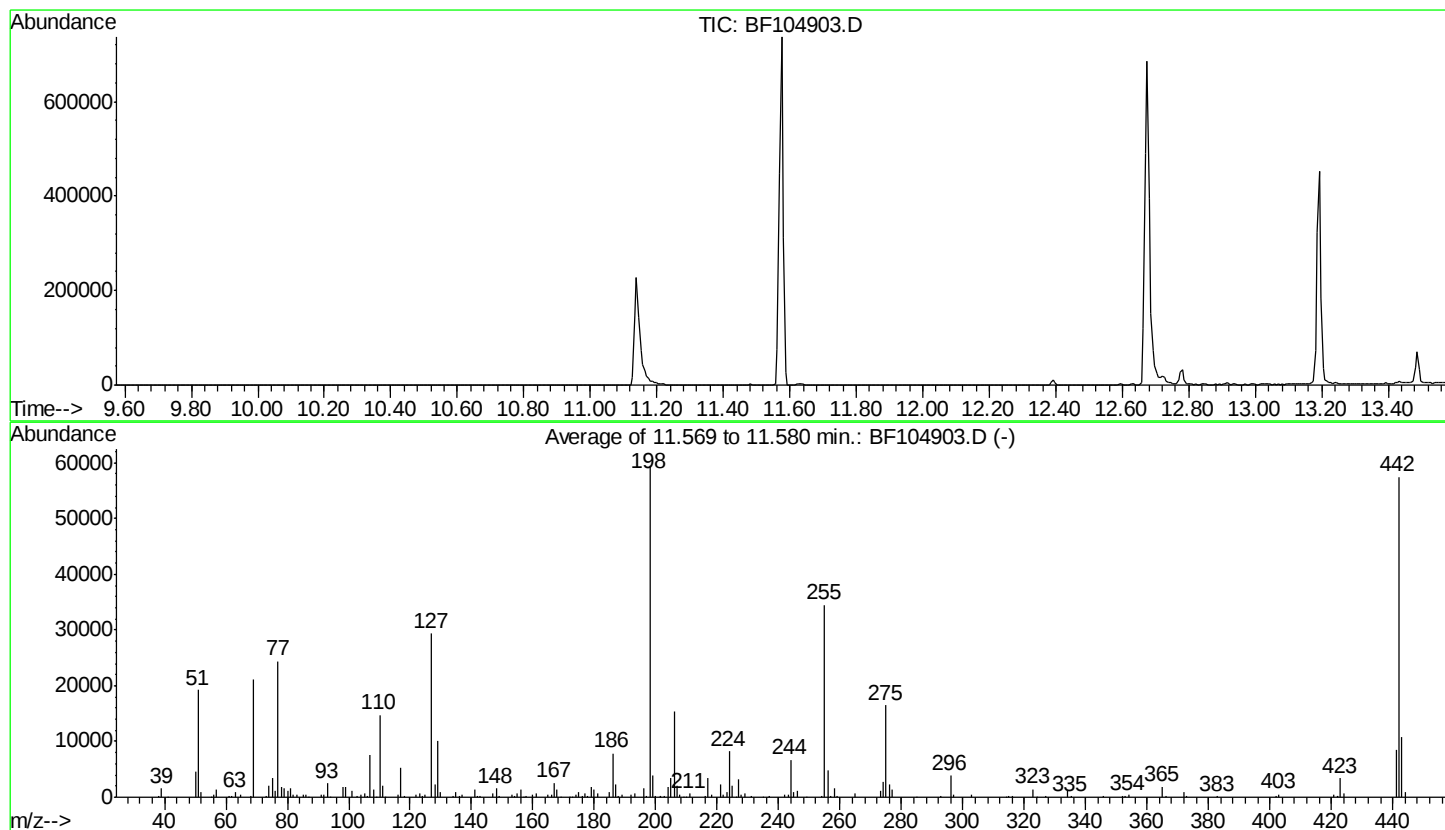

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	19219	PASS
68	69	0.00	2	1.6	333	PASS
69	198	0.00	100	35.5	21115	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.4	29370	PASS
197	198	0.00	2	0.3	193	PASS
198	198	100	100	100.0	59480	PASS
199	198	5	9	6.7	3972	PASS
275	198	10	60	27.7	16487	PASS
365	198	1	100	3.3	1956	PASS
441	443	0.01	100	80.0	8559	PASS
442	198	50	100	96.6	57464	PASS
443	442	15	24	18.6	10701	PASS