
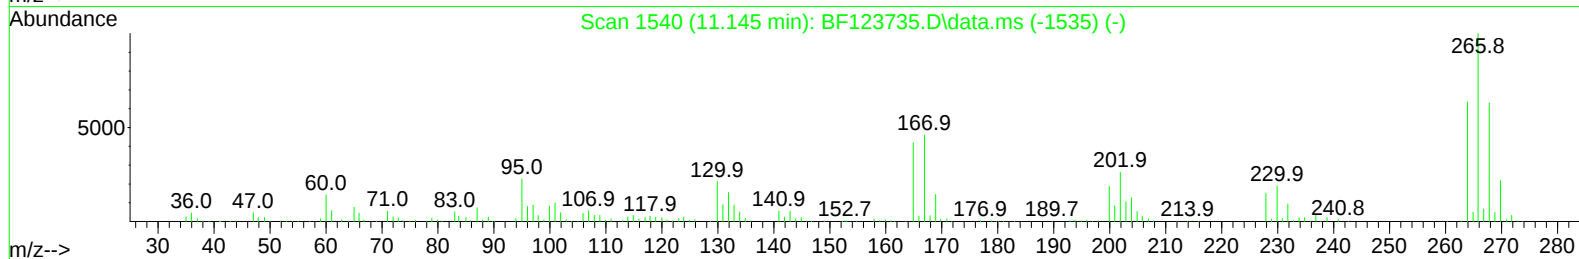
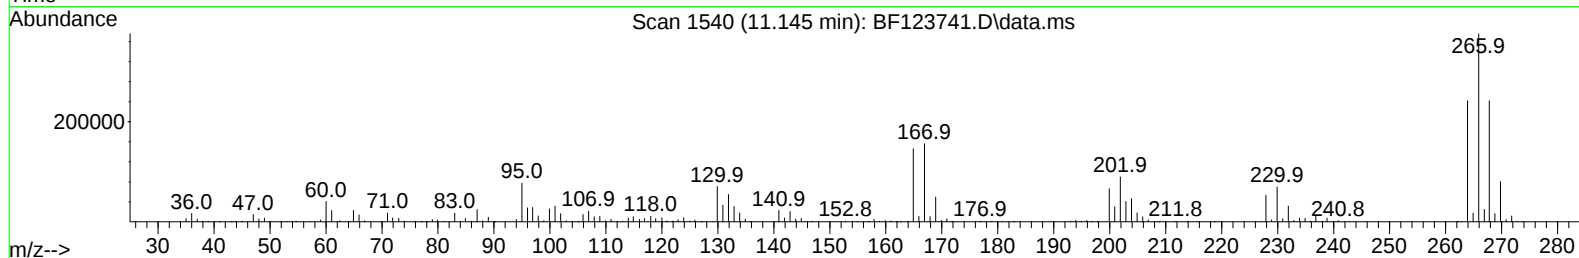


Quant Time: Apr 27 12:34:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 12:27:51 2021
Response via : Initial Calibration

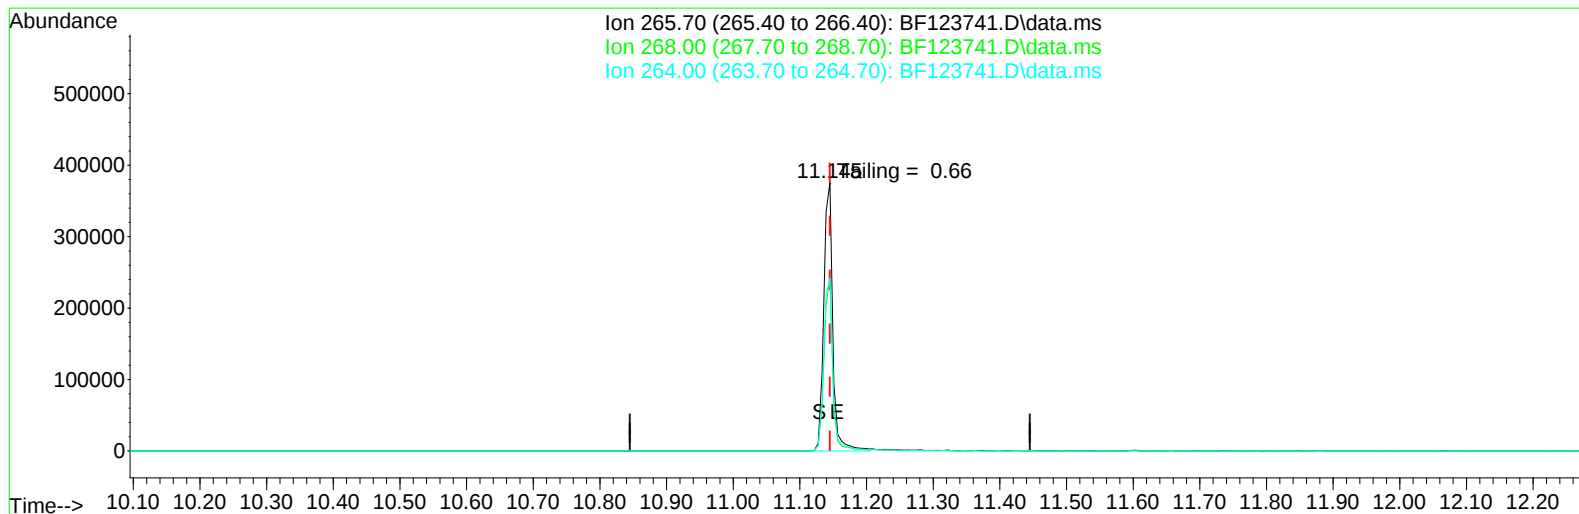

TIC: BF123741.D\data.ms

(70) **Pentachlorophenol (C)**




11.145min (-0.000) 94686.84 ng

response **359669**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.41
264.00	65.70	64.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042721\
Data File : BF123741.D
Acq On : 27 Apr 2021 11:56
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 12:34:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 12:27:51 2021
Response via : Initial Calibration

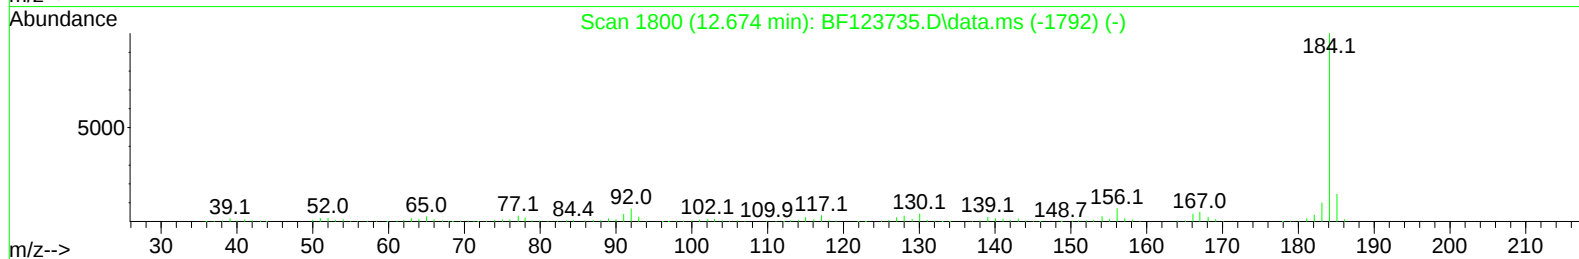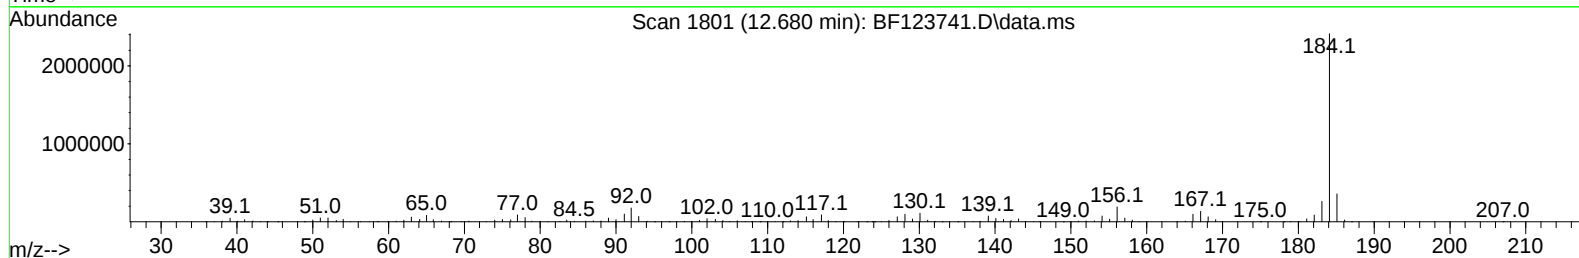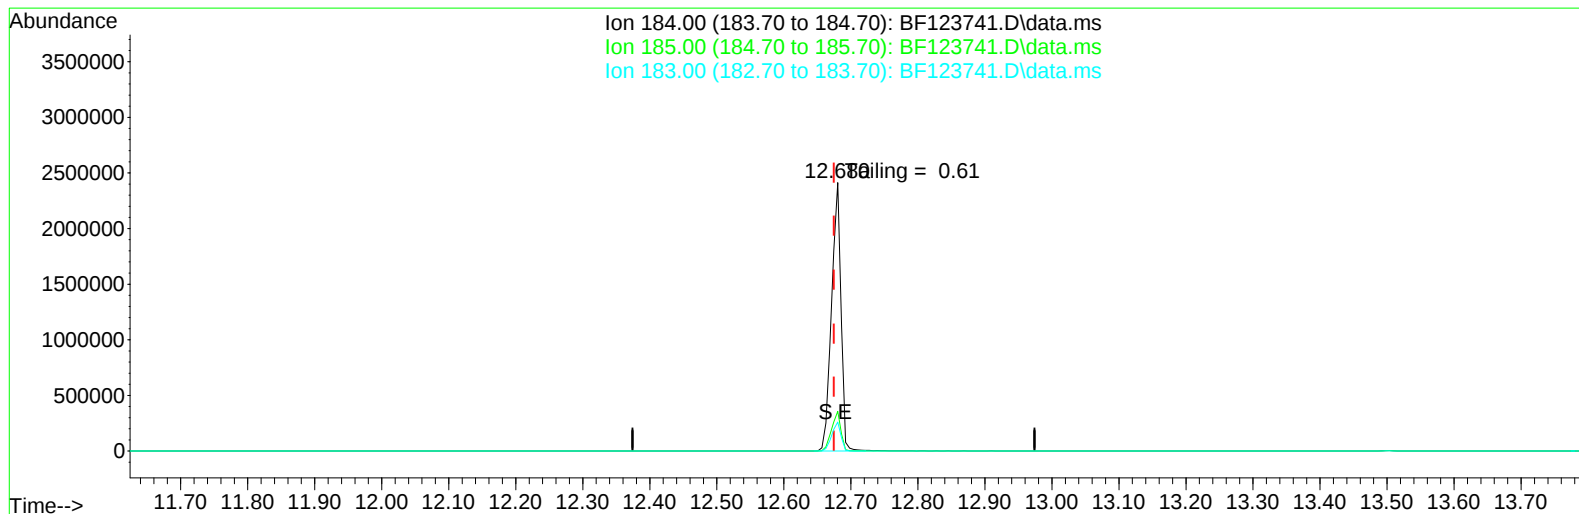

TIC: BF123741.D\data.ms

(77) Benzidine

12.680min (+ 0.006) 41412.81 ng

response 2370037

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.81
183.00	9.80	10.80
0.00	0.00	0.00