
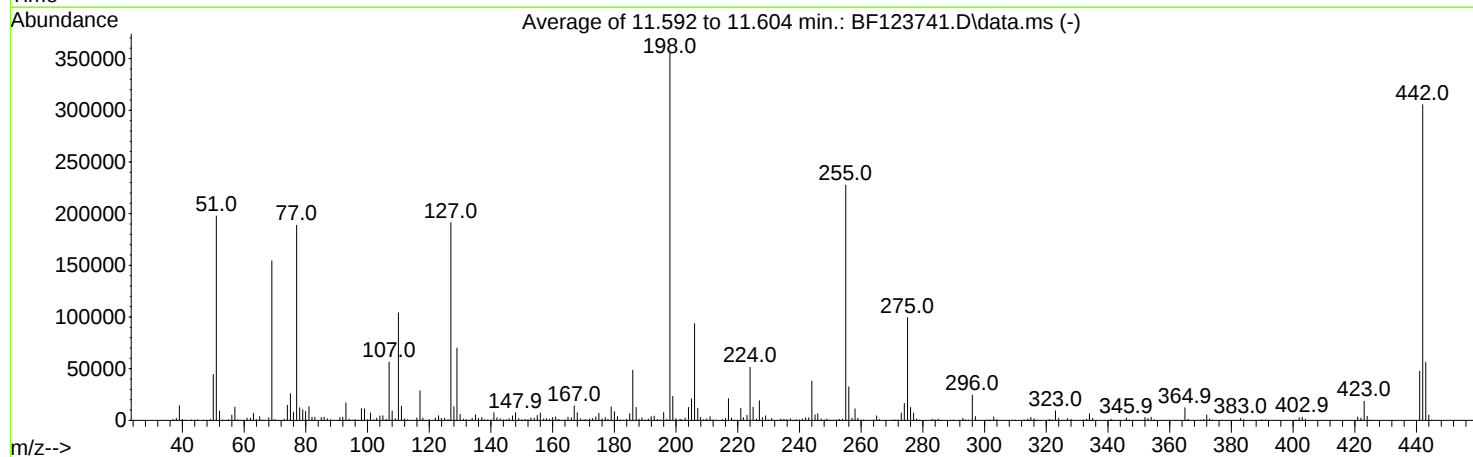


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042721\
 Data File : BF123741.D
 Acq On : 27 Apr 2021 11:56
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 27 16:30:39 2021

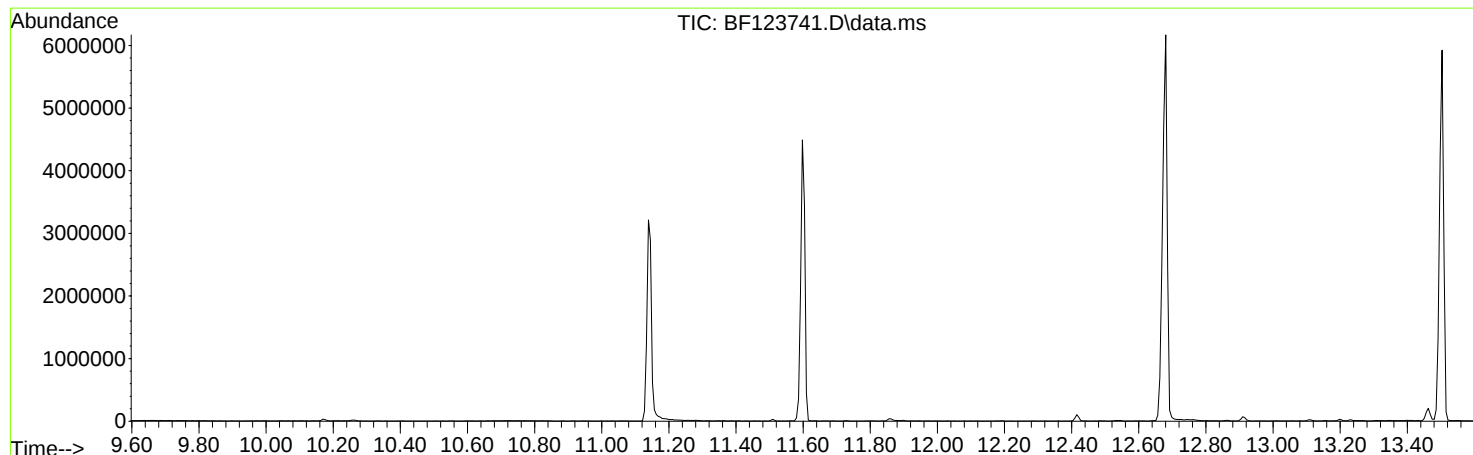

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.5	197653	PASS
68	69	0.00	2	1.7	2558	PASS
69	198	0.00	100	43.3	154269	PASS
70	69	0.00	2	0.6	920	PASS
127	198	10	80	53.7	191275	PASS
197	198	0.00	2	0.3	1025	PASS
198	198	100	100	100.0	355883	PASS
199	198	5	9	6.5	23153	PASS
275	198	10	60	27.9	99323	PASS
365	198	1	100	3.4	12188	PASS
441	198	0.01	100	13.3	47499	PASS
442	442	50	100	100.0	305461	PASS
443	442	15	24	18.4	56259	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/27/2021	BNA_F	<u>BF123741.D</u>
Compound Name	Response	Retention Time
DDT	944656	13.5
DDD	4163	13.19
DDE	1355	12.86
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5518	950174	0.58

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042721\
Data File : BF123741.D
Acq On : 27 Apr 2021 11:56
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 27 12:34:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 12:27:51 2021
Response via : Initial Calibration

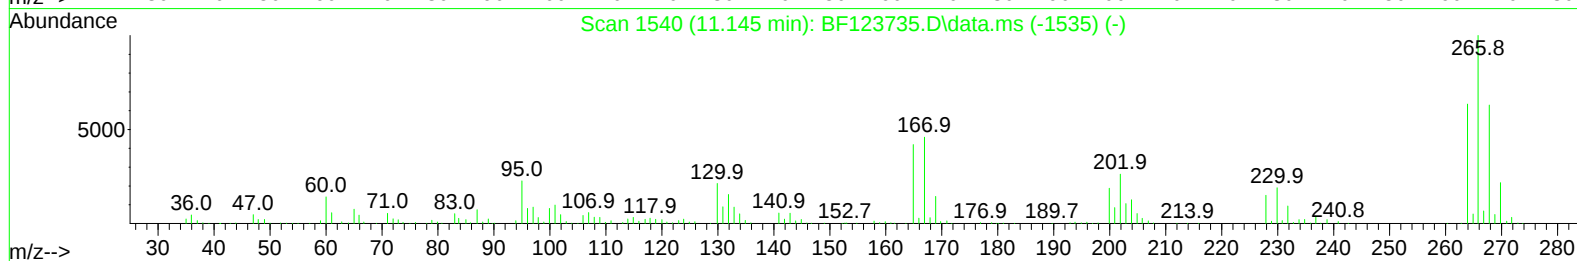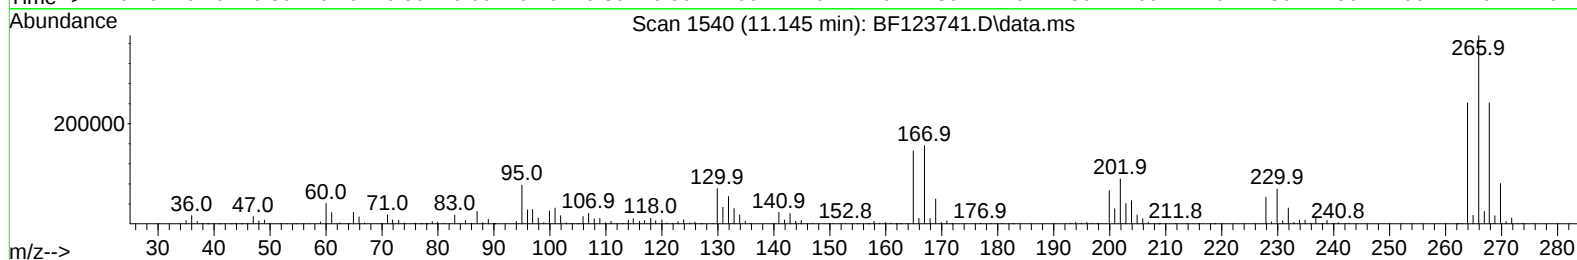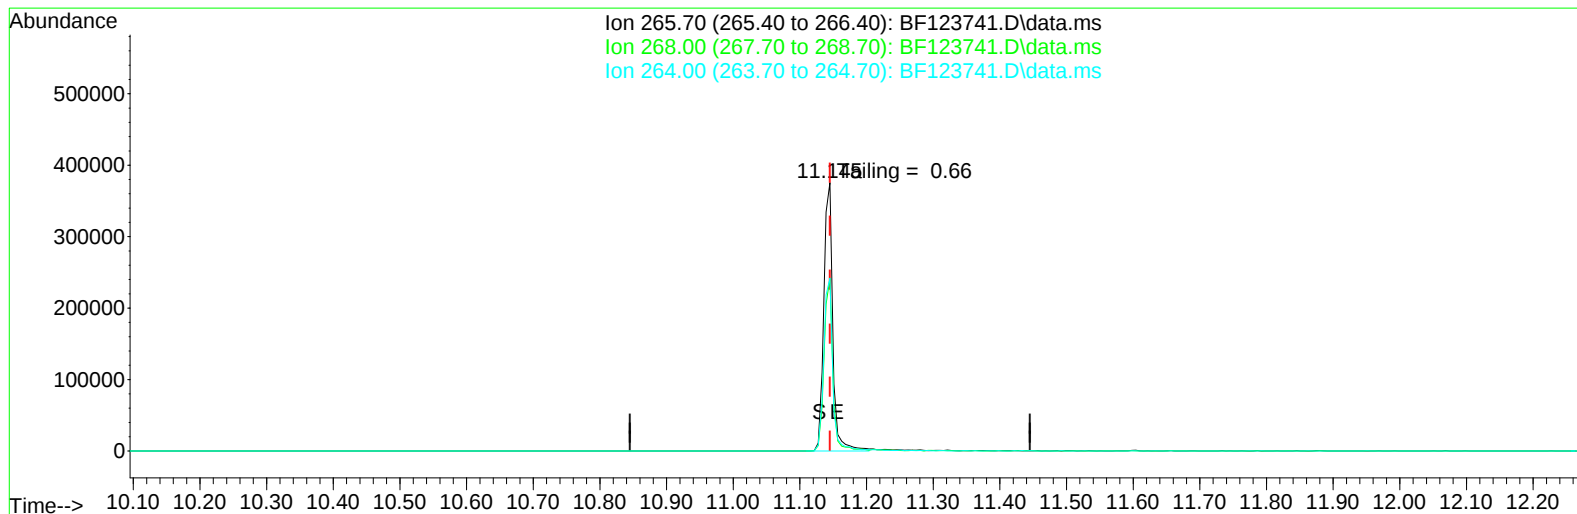

TIC: BF123741.D\data.ms

(70) Pentachlorophenol (C)

11.145min (-0.000) 94686.84 ng




response 359669

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.41
264.00	65.70	64.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042721\
Data File : BF123741.D
Acq On : 27 Apr 2021 11:56
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 27 12:34:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 27 12:27:51 2021
Response via : Initial Calibration

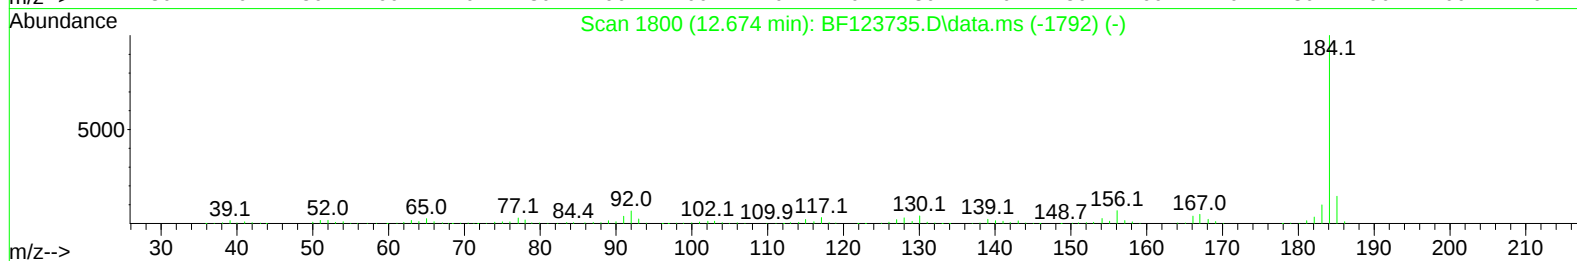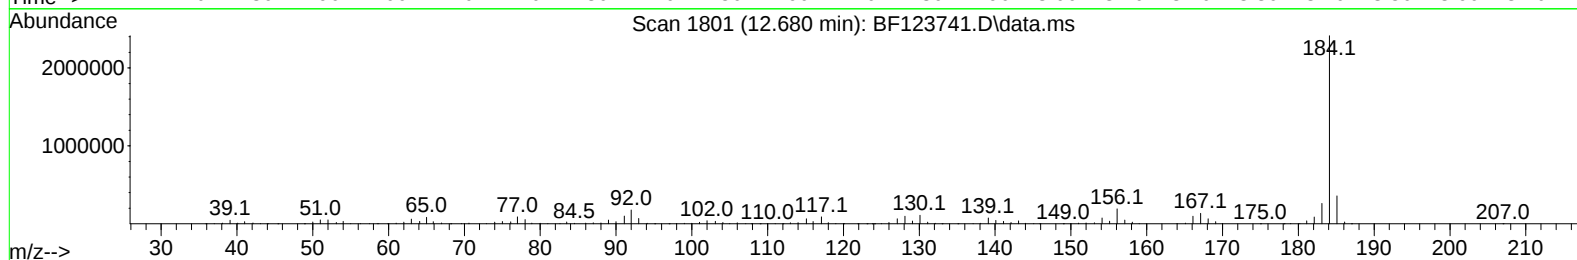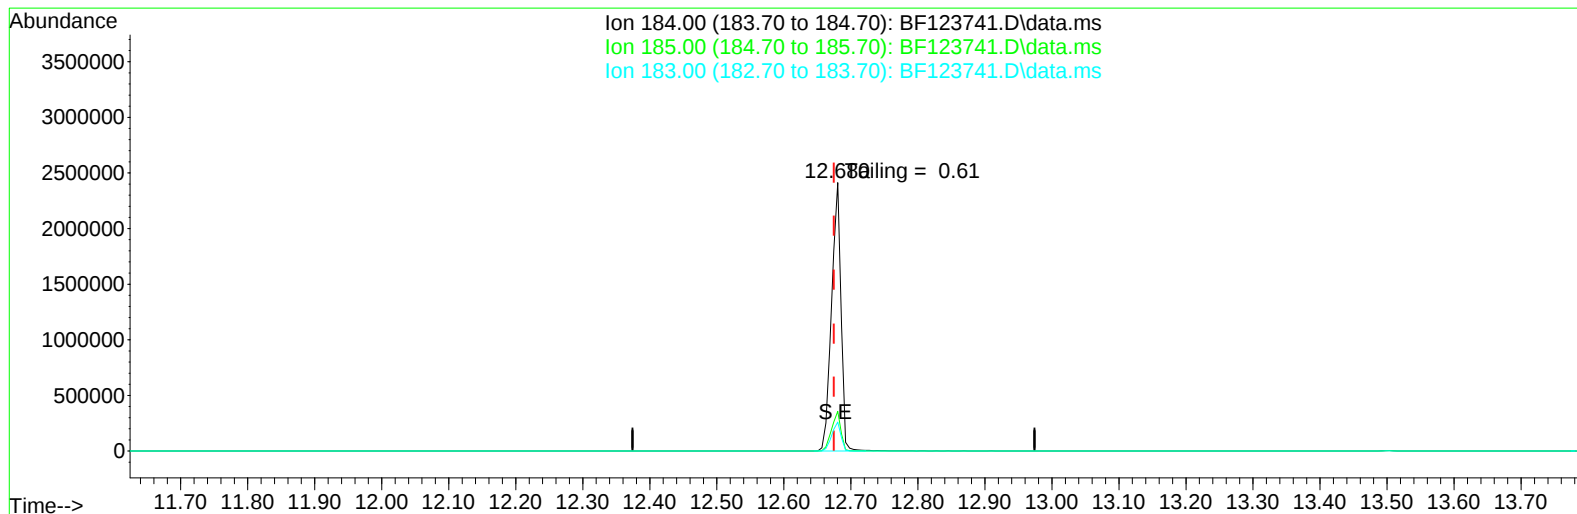

TIC: BF123741.D\data.ms

(77) Benzidine

12.680min (+ 0.006) 41412.81 ng

response 2370037

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.81
183.00	9.80	10.80
0.00	0.00	0.00