
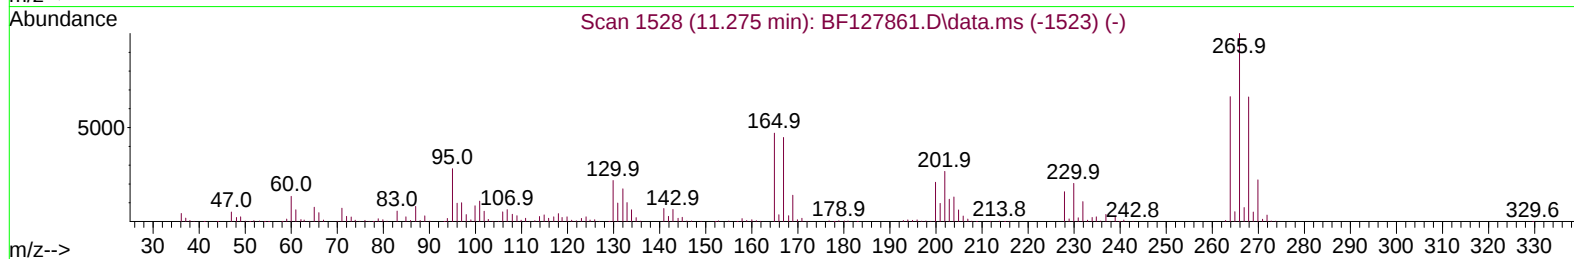
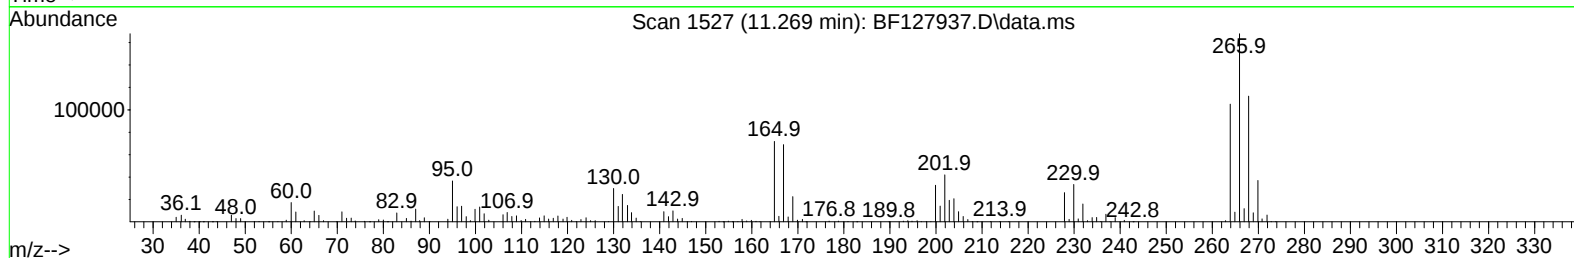


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042722\
Data File : BF127937.D
Acq On : 27 Apr 2022 11:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 17:52:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 00:43:03 2022
Response via : Initial Calibration

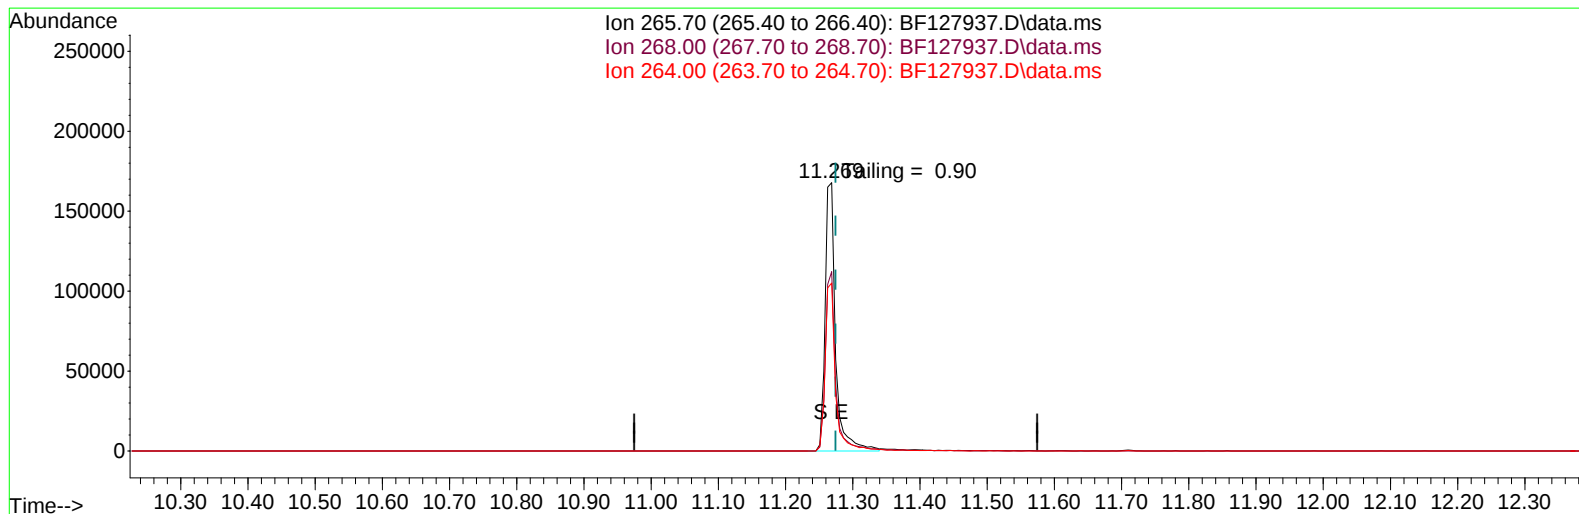

TIC: BF127937.D\data.ms

(70) Pentachlorophenol (C)




11.269min (-0.006) 399318.13 ng

response 183833

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	66.83
264.00	66.40	62.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042722\
 Data File : BF127937.D
 Acq On : 27 Apr 2022 11:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 17:52:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Apr 24 00:43:03 2022
 Response via : Initial Calibration

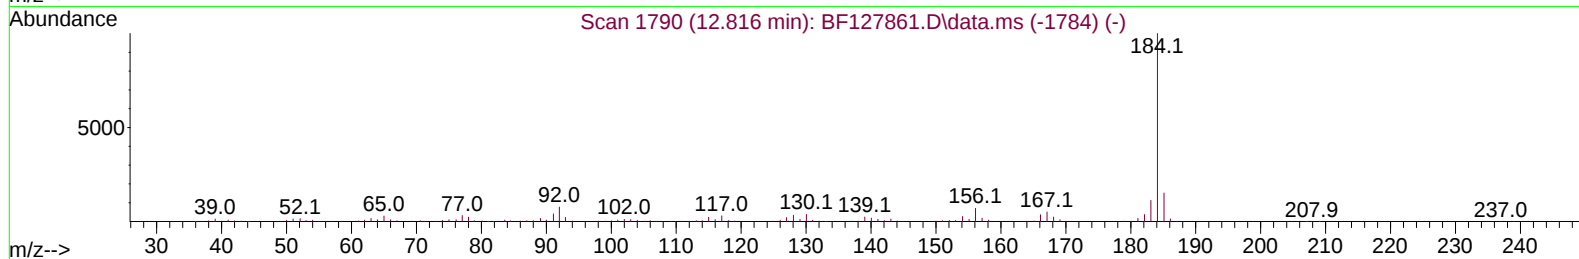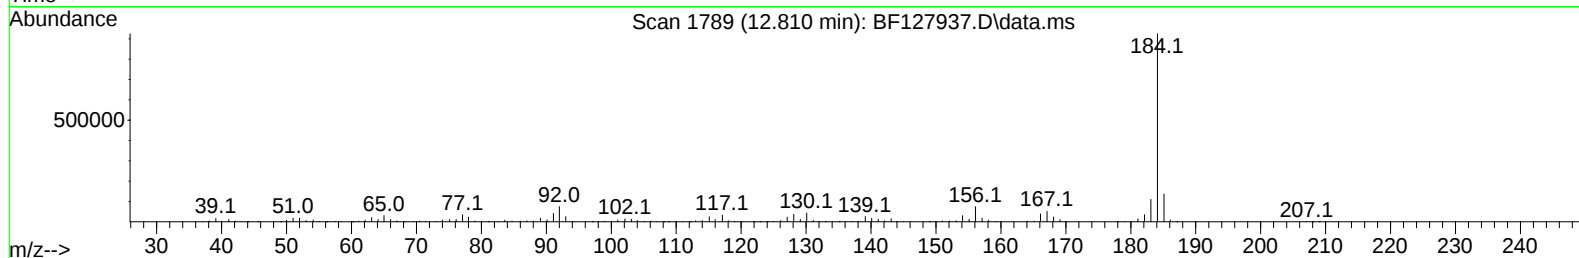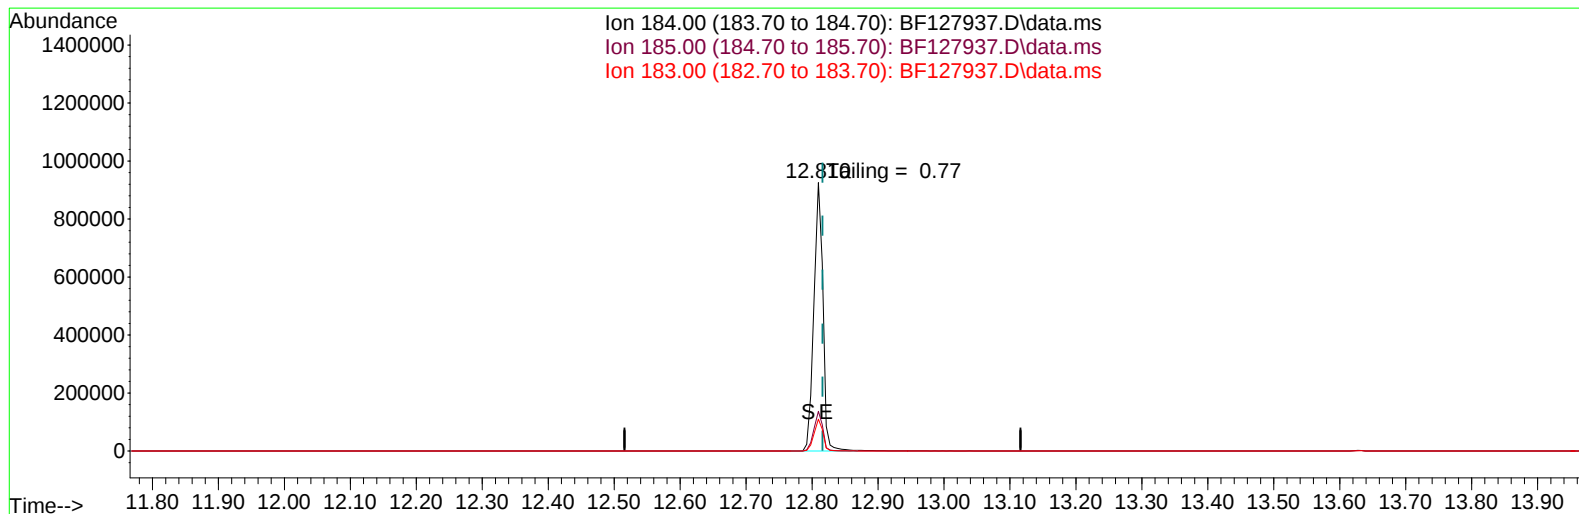

TIC: BF127937.D\data.ms

(77) Benzidine

12.810min (-0.006) 856985.51 ng

response 891847

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.79
183.00	11.20	11.90
0.00	0.00	0.00