
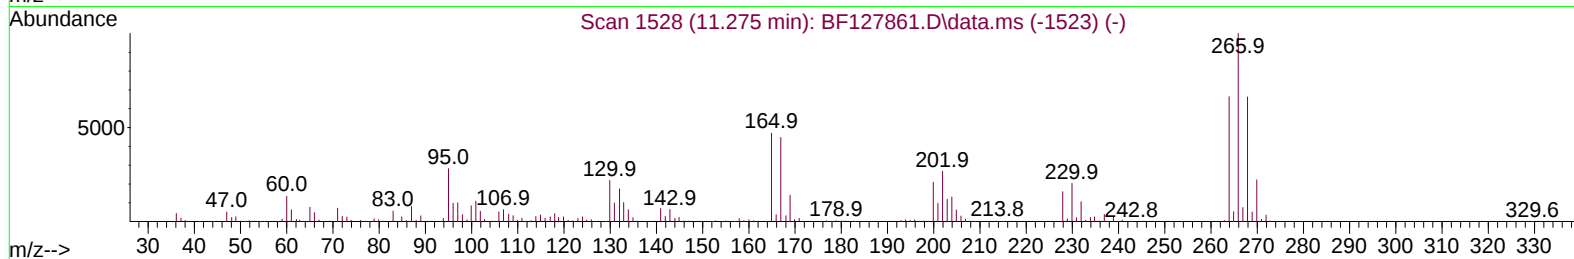
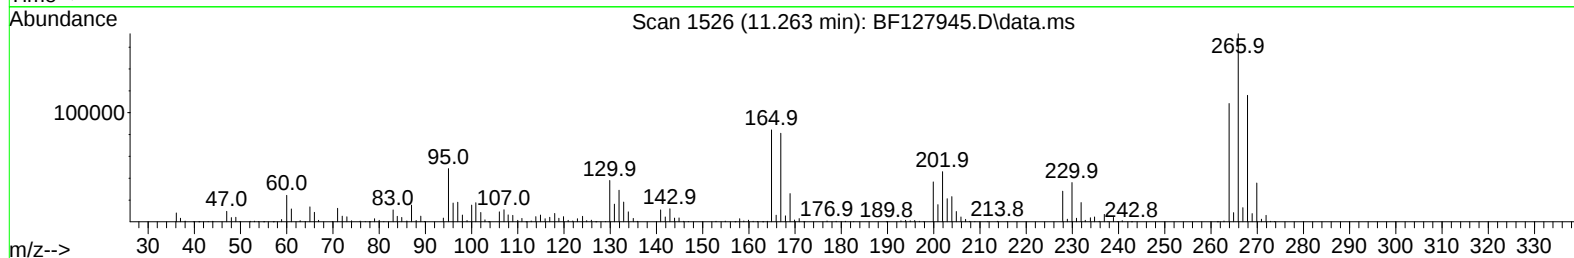


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042722\
Data File : BF127945.D
Acq On : 27 Apr 2022 15:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 17:45:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 00:43:03 2022
Response via : Initial Calibration

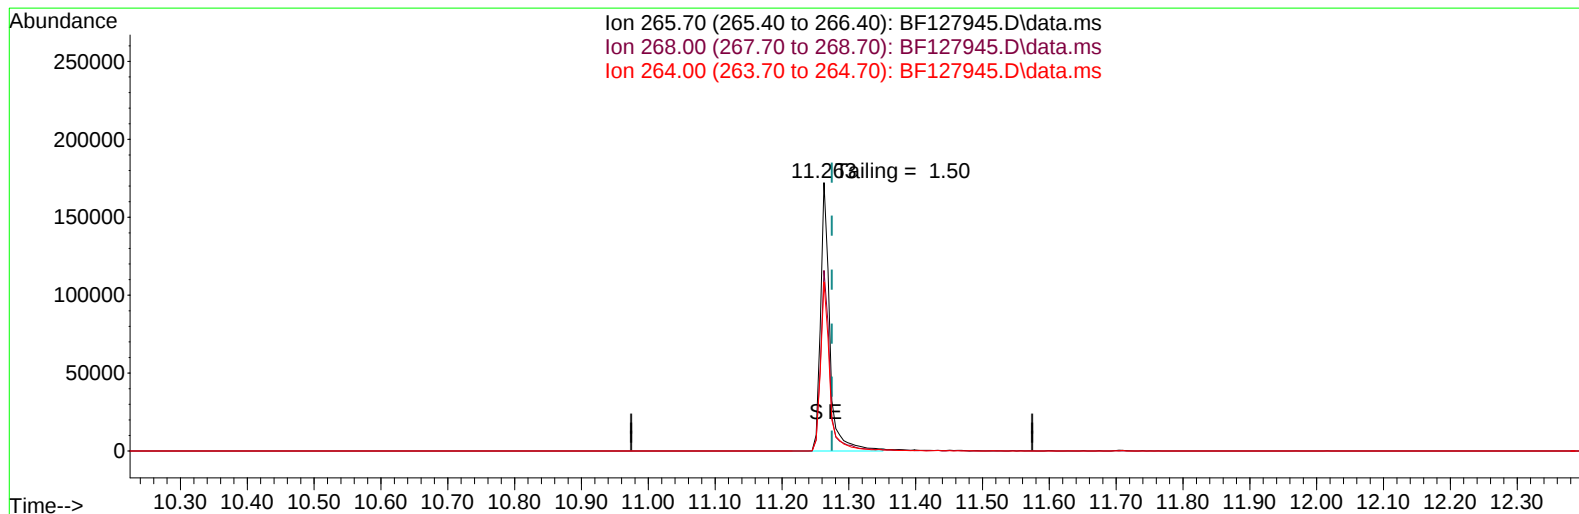

TIC: BF127945.D\data.ms

(70) Pentachlorophenol (C)




11.263min (-0.012) 158127.67 ng

response 167324

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	67.27
264.00	66.40	62.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042722\
Data File : BF127945.D
Acq On : 27 Apr 2022 15:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 17:45:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 00:43:03 2022
Response via : Initial Calibration

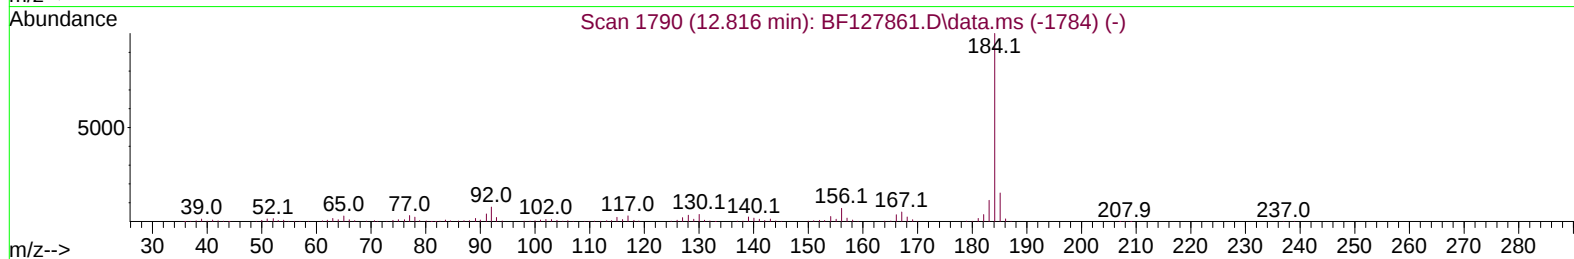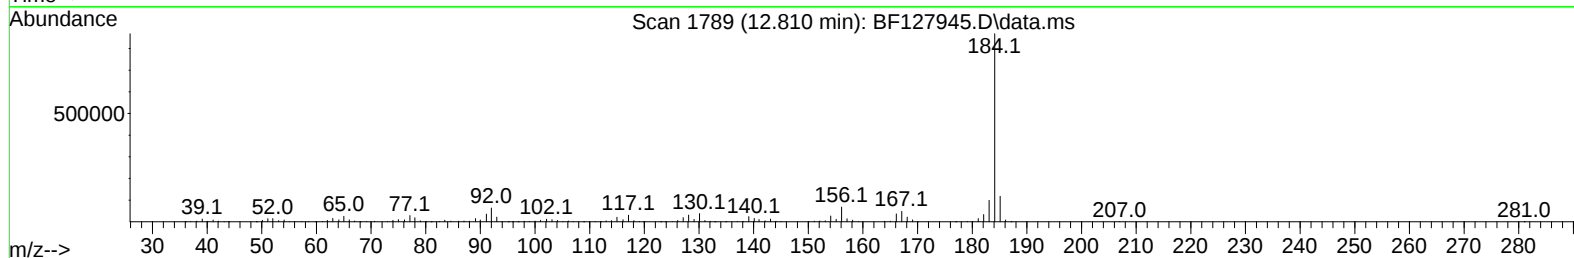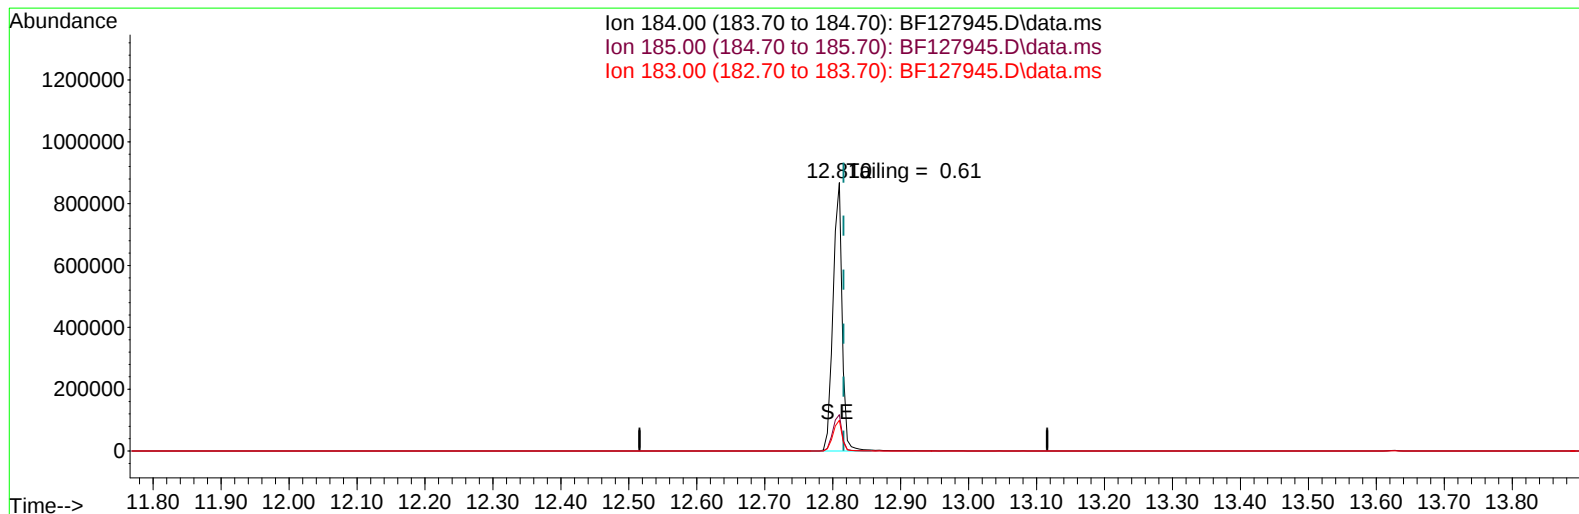

TIC: BF127945.D\data.ms

(77) Benzidine

12.810min (-0.006) 97720.20 ng

response 811714

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.54
183.00	11.20	11.46
0.00	0.00	0.00