

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF042722\  
 Data File : BF127957.D  
 Acq On : 27 Apr 2022 20:53  
 Operator : CG\JU  
 Sample : N2482-13  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 SPN-15

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127957.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 4.045       | 295           | 299         | 304          | rVB      | 58601          | 68257         | 1.74%           | 0.266%        |
| 2         | 4.457       | 365           | 369         | 380          | rBV      | 337230         | 408573        | 10.44%          | 1.594%        |
| 3         | 5.157       | 484           | 488         | 496          | rBV      | 141609         | 170239        | 4.35%           | 0.664%        |
| 4         | 5.422       | 529           | 533         | 537          | rBV      | 1186849        | 1052159       | 26.88%          | 4.106%        |
| 5         | 5.545       | 548           | 554         | 558          | rBV      | 2551355        | 2451574       | 62.63%          | 9.566%        |
| 6         | 5.781       | 591           | 594         | 597          | rBV      | 60012          | 52523         | 1.34%           | 0.205%        |
| 7         | 6.098       | 645           | 648         | 652          | rVB      | 133233         | 121081        | 3.09%           | 0.472%        |
| 8         | 6.386       | 694           | 697         | 701          | rBV      | 253626         | 225091        | 5.75%           | 0.878%        |
| 9         | 6.451       | 705           | 708         | 711          | rBV      | 133329         | 114358        | 2.92%           | 0.446%        |
| 10        | 6.486       | 711           | 714         | 717          | rVV      | 454818         | 347616        | 8.88%           | 1.356%        |
| 11        | 6.545       | 717           | 724         | 730          | rVV2     | 1034537        | 1095345       | 27.98%          | 4.274%        |
| 12        | 6.610       | 733           | 735         | 742          | rVB      | 148327         | 138754        | 3.54%           | 0.541%        |
| 13        | 6.728       | 751           | 755         | 756          | rBV      | 215159         | 196451        | 5.02%           | 0.767%        |
| 14        | 6.751       | 756           | 759         | 772          | rVV      | 1378815        | 1205211       | 30.79%          | 4.703%        |
| 15        | 6.845       | 772           | 775         | 786          | rVV      | 270845         | 390047        | 9.96%           | 1.522%        |
| 16        | 6.928       | 786           | 789         | 795          | rVV      | 747430         | 666837        | 17.03%          | 2.602%        |
| 17        | 6.986       | 795           | 799         | 802          | rVB      | 450079         | 401105        | 10.25%          | 1.565%        |
| 18        | 7.110       | 812           | 820         | 823          | rBV      | 271882         | 232101        | 5.93%           | 0.906%        |
| 19        | 7.333       | 853           | 858         | 864          | rVB2     | 58815          | 78753         | 2.01%           | 0.307%        |
| 20        | 7.463       | 876           | 880         | 881          | rBV      | 86338          | 78098         | 2.00%           | 0.305%        |
| 21        | 7.492       | 881           | 885         | 889          | rVB      | 2163774        | 2288990       | 58.47%          | 8.932%        |
| 22        | 7.569       | 894           | 898         | 901          | rBV      | 41281          | 43666         | 1.12%           | 0.170%        |
| 23        | 7.604       | 901           | 904         | 916          | rVB5     | 40068          | 73985         | 1.89%           | 0.289%        |
| 24        | 7.722       | 921           | 924         | 926          | rVB      | 55807          | 45364         | 1.16%           | 0.177%        |
| 25        | 7.881       | 945           | 951         | 955          | rBV2     | 58845          | 56037         | 1.43%           | 0.219%        |
| 26        | 7.945       | 958           | 962         | 965          | rBV      | 101948         | 87011         | 2.22%           | 0.340%        |
| 27        | 8.151       | 987           | 997         | 999          | rBV2     | 37862          | 57523         | 1.47%           | 0.224%        |
| 28        | 8.210       | 1003          | 1007        | 1010         | rVV      | 907142         | 868869        | 22.20%          | 3.390%        |
| 29        | 8.233       | 1010          | 1011        | 1018         | rVB      | 196543         | 121136        | 3.09%           | 0.473%        |
| 30        | 8.463       | 1037          | 1050        | 1053         | rBV7     | 27492          | 96050         | 2.45%           | 0.375%        |
| 31        | 9.204       | 1171          | 1176        | 1179         | rBV      | 55180          | 88247         | 2.25%           | 0.344%        |
| 32        | 9.292       | 1184          | 1191        | 1194         | rBV      | 3777706        | 3914570       | 100.00%         | 15.275%       |
| 33        | 9.386       | 1203          | 1207        | 1222         | rVB      | 705441         | 861594        | 22.01%          | 3.362%        |
| 34        | 9.969       | 1300          | 1306        | 1310         | rBV      | 1004062        | 882888        | 22.55%          | 3.445%        |
| 35        | 10.380      | 1372          | 1376        | 1379         | rVB      | 188719         | 156016        | 3.99%           | 0.609%        |
| 36        | 10.674      | 1423          | 1426        | 1428         | rBV      | 163106         | 139025        | 3.55%           | 0.542%        |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF042722\  
Data File : BF127957.D  
Acq On : 27 Apr 2022 20:53  
Operator : CG\JU  
Sample : N2482-13  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SPN-15

Integration Parameters: rteint.p  
Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042222.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

|    |        |      |      |      |     |         |         |        |        |
|----|--------|------|------|------|-----|---------|---------|--------|--------|
| 37 | 10.763 | 1437 | 1441 | 1444 | rBV | 2020744 | 1805962 | 46.13% | 7.047% |
| 38 | 11.463 | 1556 | 1560 | 1563 | rBV | 917437  | 748438  | 19.12% | 2.920% |
| 39 | 11.839 | 1621 | 1624 | 1627 | rBV | 137055  | 102065  | 2.61%  | 0.398% |
| 40 | 13.051 | 1825 | 1830 | 1833 | rBV | 2853542 | 2531389 | 64.67% | 9.878% |
| 41 | 14.104 | 2006 | 2009 | 2018 | rVB | 530159  | 515007  | 13.16% | 2.010% |
| 42 | 15.615 | 2261 | 2266 | 2277 | rBV | 498096  | 649128  | 16.58% | 2.533% |




Sum of corrected areas: 25627133

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF042722\  
Data File : BF127957.D  
Acq On : 27 Apr 2022 20:53  
Operator : CG\JU  
Sample : N2482-13  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SPN-15

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042222.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :  
TIC Integration Parameters: rteint.p

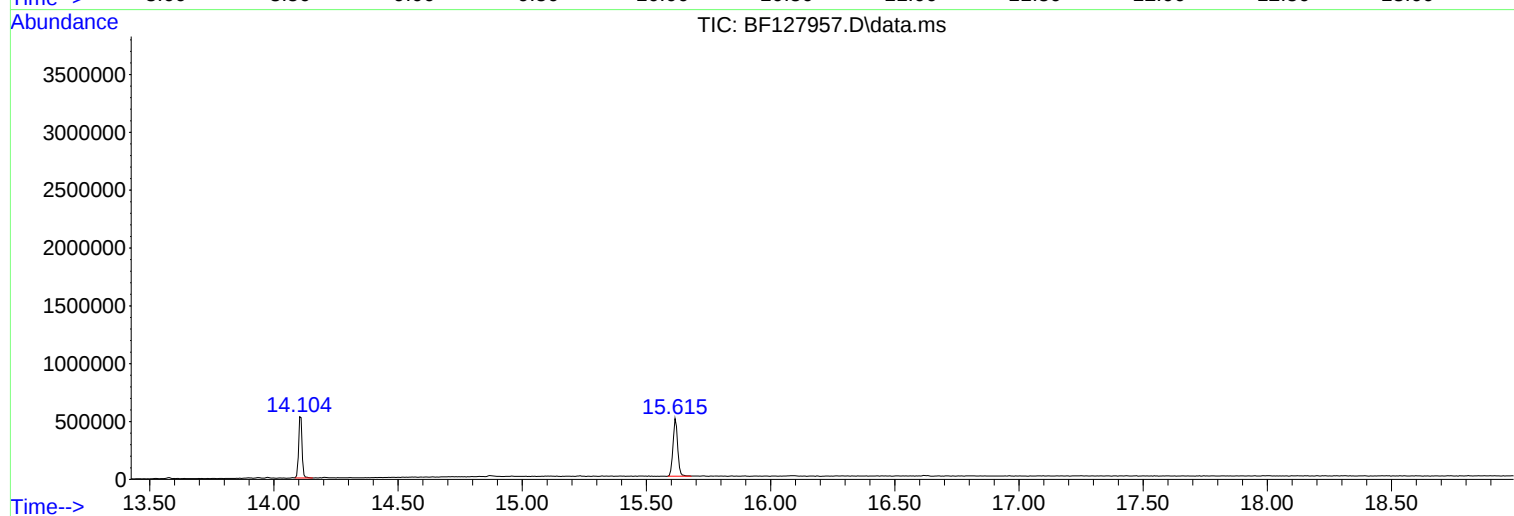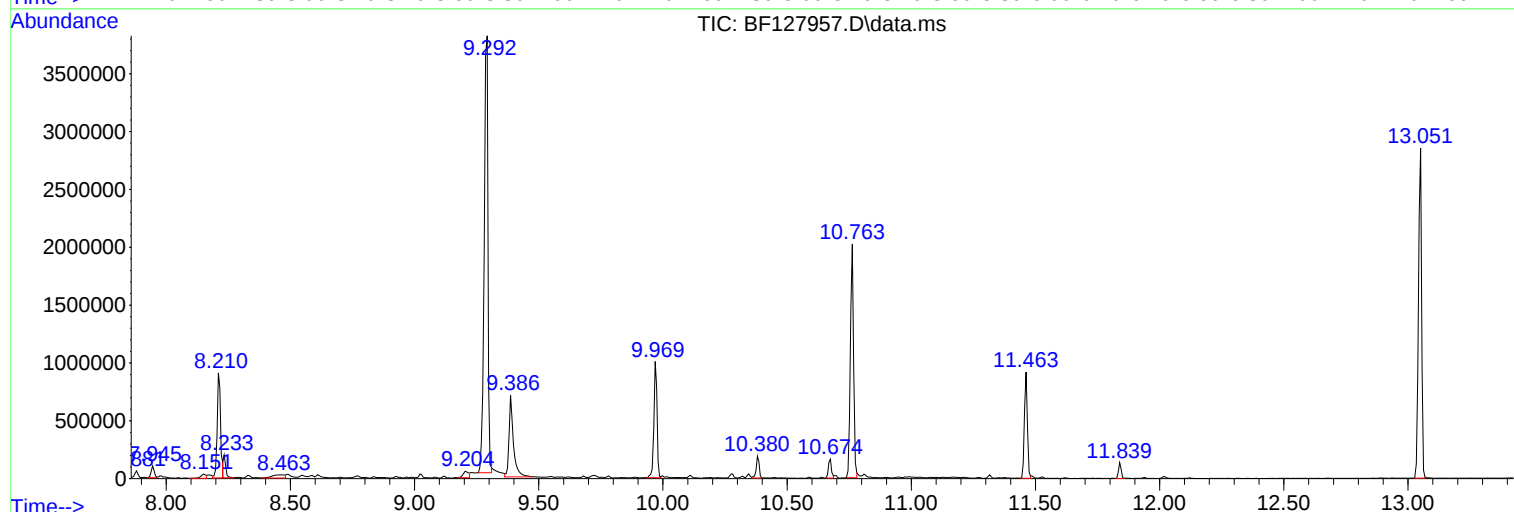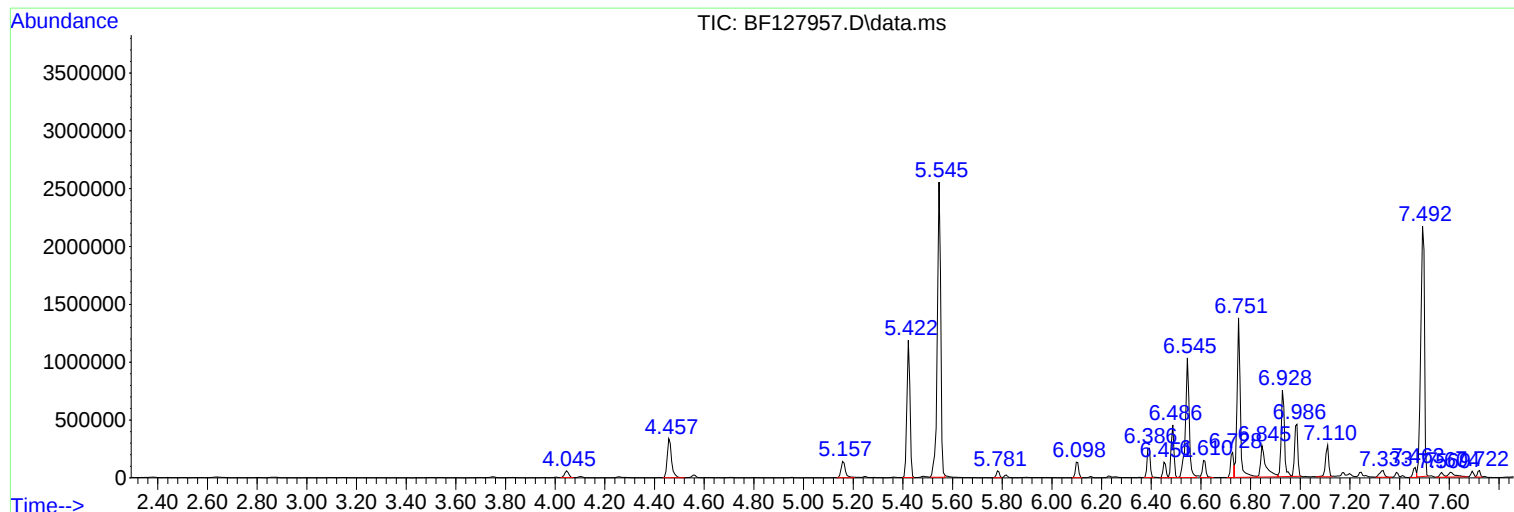

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF042722\  
Data File : BF127957.D  
Acq On : 27 Apr 2022 20:53  
Operator : CG\JU  
Sample : N2482-13  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SPN-15

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042222.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :  
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF042722\  
Data File : BF127957.D  
Acq On : 27 Apr 2022 20:53  
Operator : CG\JU  
Sample : N2482-13  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SPN-15

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042222.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :  
TIC Integration Parameters: rteint.p

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|