

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042722\
 Data File : BF127958.D
 Acq On : 27 Apr 2022 21:21
 Operator : CG\JU
 Sample : N2521-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127958.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.545	550	554	567	rVB	1735740	1554677	45.47%	9.453%
2	6.545	720	724	734	rBV	1176971	1017469	29.76%	6.186%
3	6.928	786	789	793	rBV	760377	622223	18.20%	3.783%
4	7.110	816	820	823	rVB	94080	80041	2.34%	0.487%
5	7.463	875	880	881	rBV	32313	34756	1.02%	0.211%
6	7.492	881	885	888	rVV	2147898	2121493	62.04%	12.899%
7	7.692	916	919	922	rVB	50515	37351	1.09%	0.227%
8	8.210	999	1007	1014	rBV	856648	885517	25.90%	5.384%
9	9.286	1186	1190	1194	rBV	3469775	3419462	100.00%	20.790%
10	9.969	1302	1306	1310	rBV	964809	843094	24.66%	5.126%
11	10.763	1437	1441	1455	rBV	1798520	1736186	50.77%	10.556%
12	11.463	1556	1560	1563	rBV	864061	724433	21.19%	4.405%
13	13.051	1825	1830	1833	rBV	2383081	2225489	65.08%	13.531%
14	14.104	2006	2009	2013	rBV	520596	495025	14.48%	3.010%
15	15.615	2261	2266	2274	rBV	491475	650026	19.01%	3.952%




Sum of corrected areas: 16447242

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042722\
Data File : BF127958.D
Acq On : 27 Apr 2022 21:21
Operator : CG\JU
Sample : N2521-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

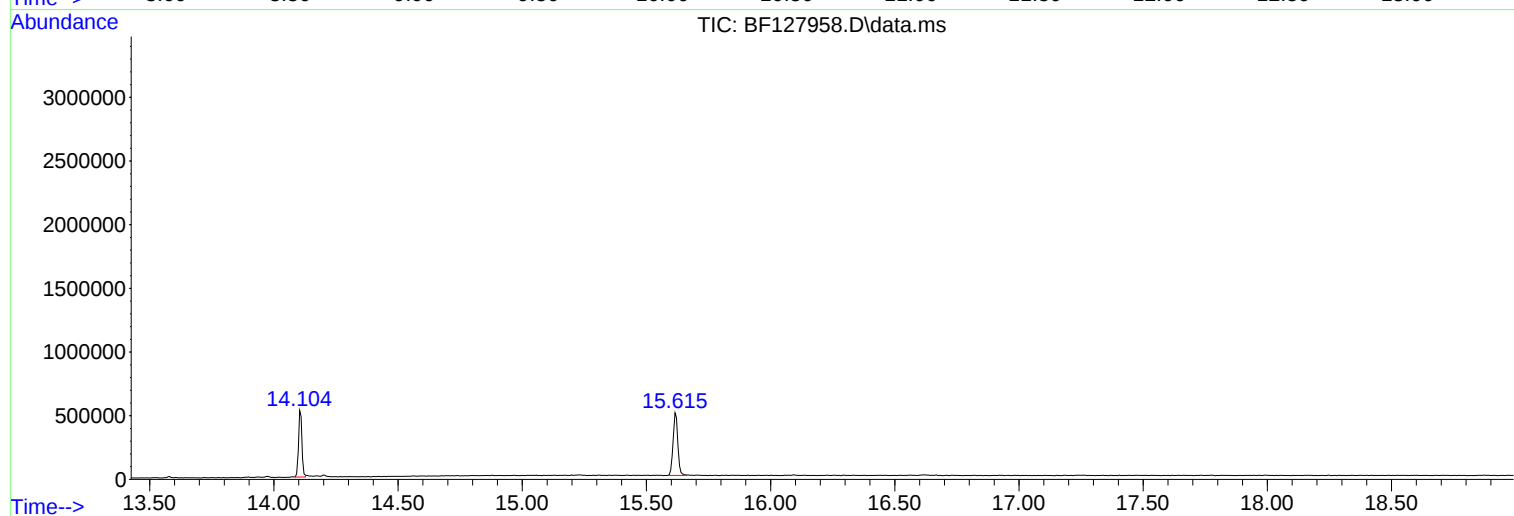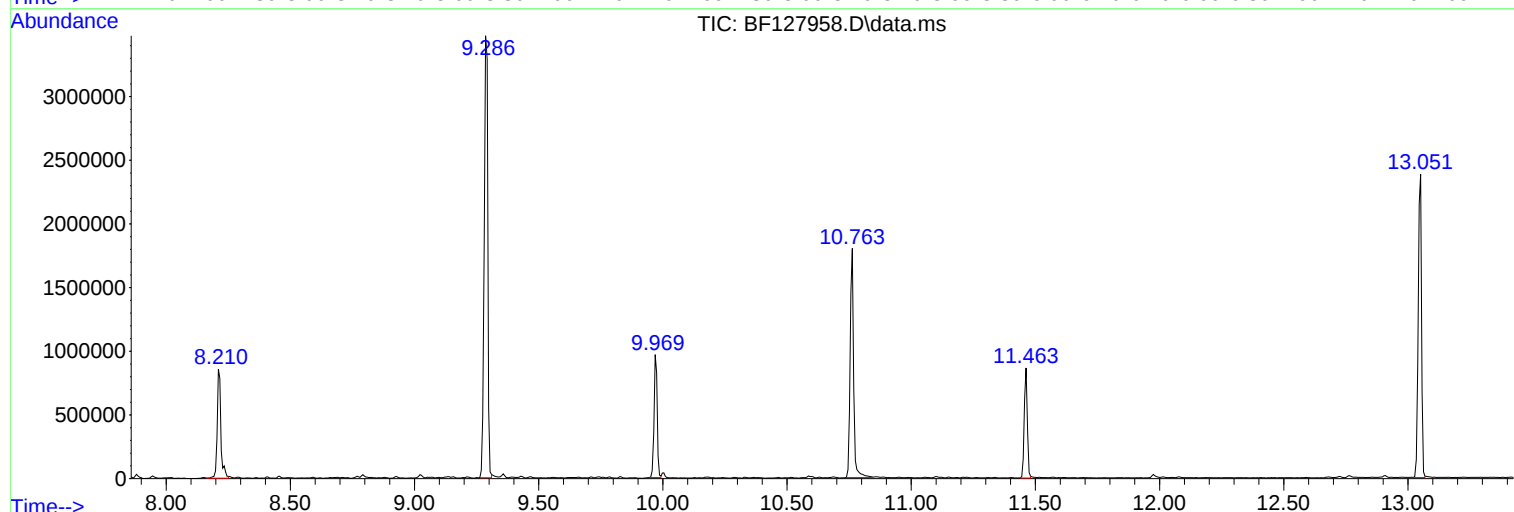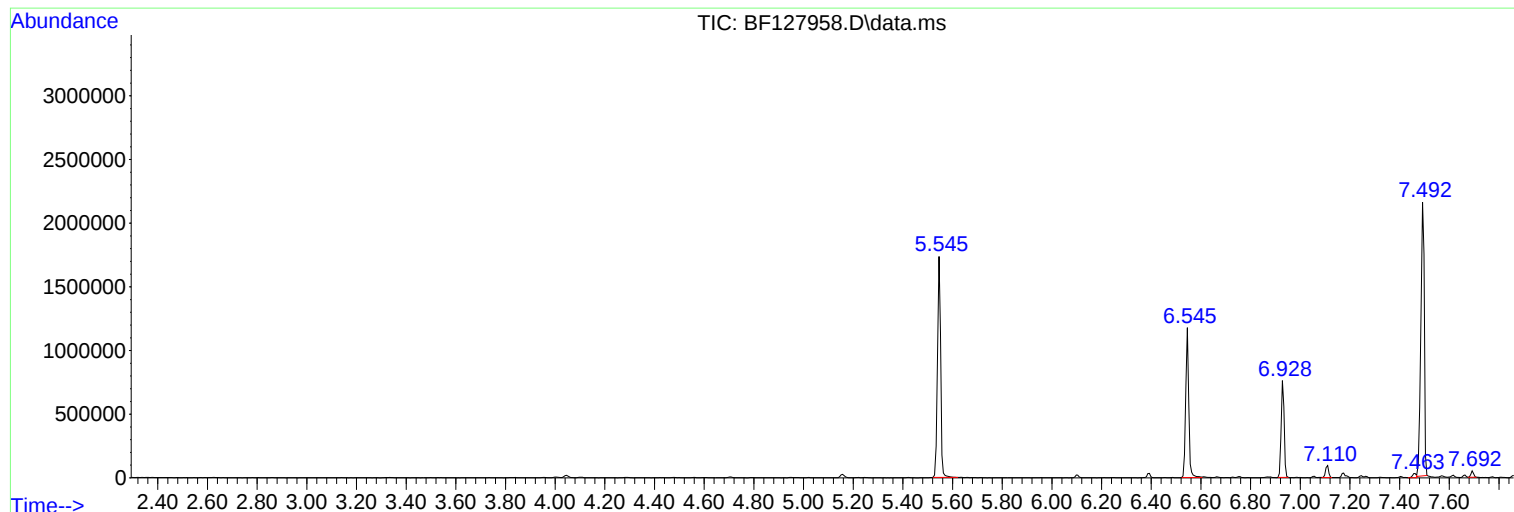

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042722\
Data File : BF127958.D
Acq On : 27 Apr 2022 21:21
Operator : CG\JU
Sample : N2521-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW3








Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Indane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.110	2.57 ng	80041	1,4-Dichlorobenzene-d4	6.928

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Indane	118	C9H10	000496-11-7	87
2			Benzene, cyclopropyl-	118	C9H10	000873-49-4	81
3			(Z)-1-Phenylpropene	118	C9H10	000766-90-5	81
4			Benzene, 2-propenyl-	118	C9H10	000300-57-2	72
5			Tetracyclo[3.3.1.0(2,8).0(4,6)]-...	118	C9H10	1000191-13-7	64

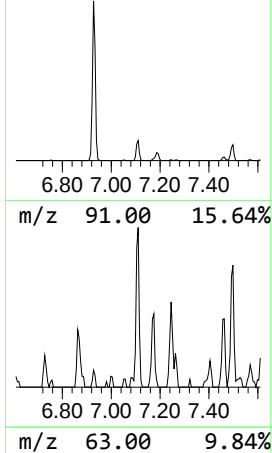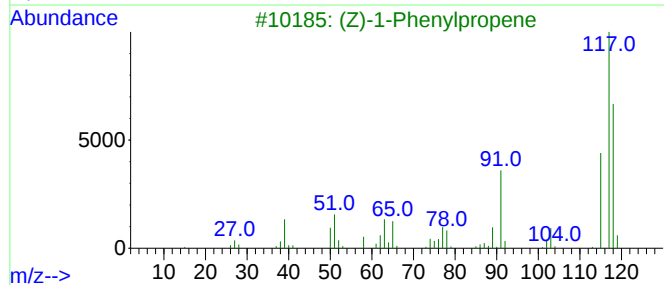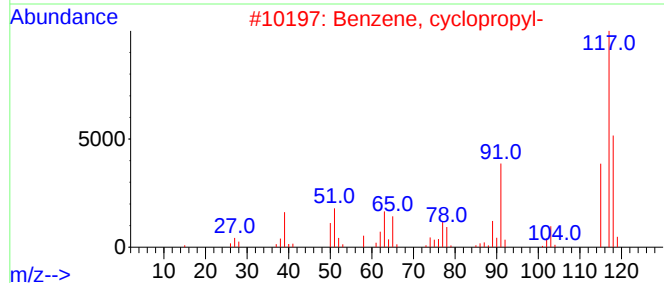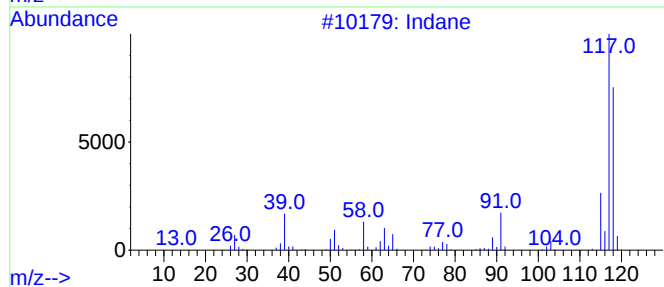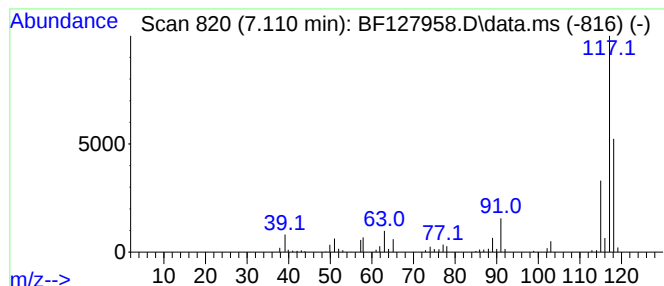

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042722\
Data File : BF127958.D
Acq On : 27 Apr 2022 21:21
Operator : CG\JU
Sample : N2521-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Indane	7.110	2.6	ng	80041	1	6.928	622223	20.0