


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042722\
 Data File : BF127937.D
 Acq On : 27 Apr 2022 11:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 28 05:13:03 2022

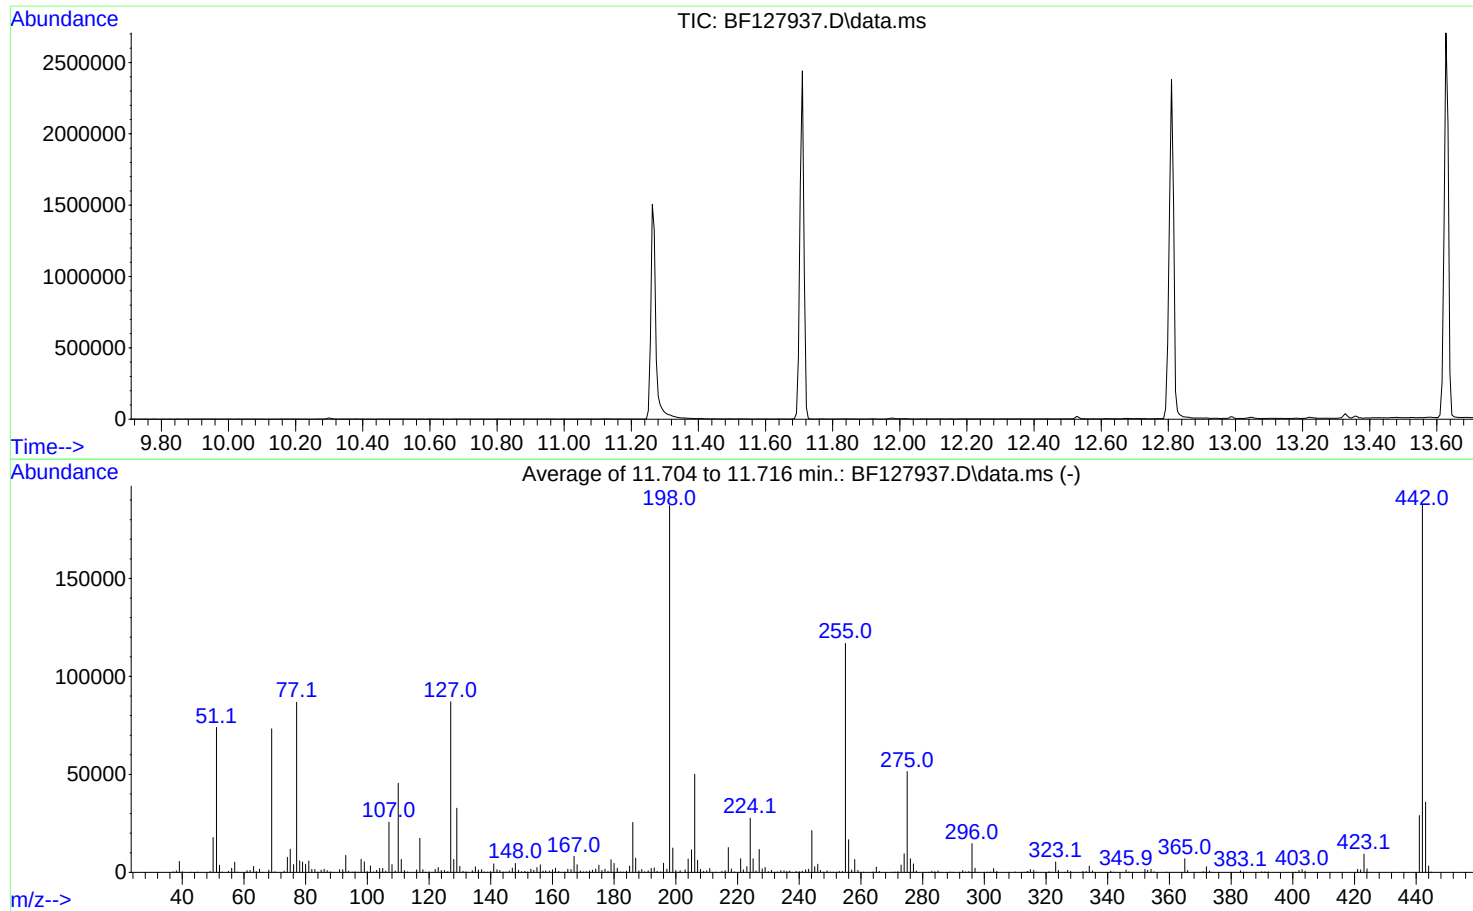




AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	73965	PASS
68	69	0.00	2	1.6	1183	PASS
69	198	0.00	100	39.1	73293	PASS
70	69	0.00	2	0.4	323	PASS
127	198	10	80	46.5	87085	PASS
197	198	0.00	2	0.9	1720	PASS
198	198	100	100	100.0	187272	PASS
199	198	5	9	6.6	12424	PASS
275	198	10	60	27.5	51411	PASS
365	198	1	100	3.7	6987	PASS
441	198	0.01	100	15.5	28973	PASS
442	442	50	100	100.0	187733	PASS
443	442	15	24	19.1	35872	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042722\
 Data File : BF127937.D
 Acq On : 27 Apr 2022 11:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 27 17:52:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Apr 24 00:43:03 2022
 Response via : Initial Calibration

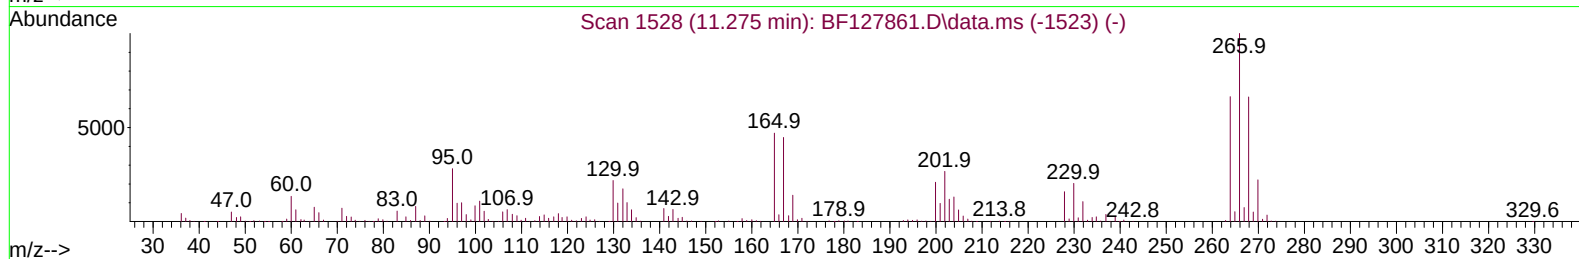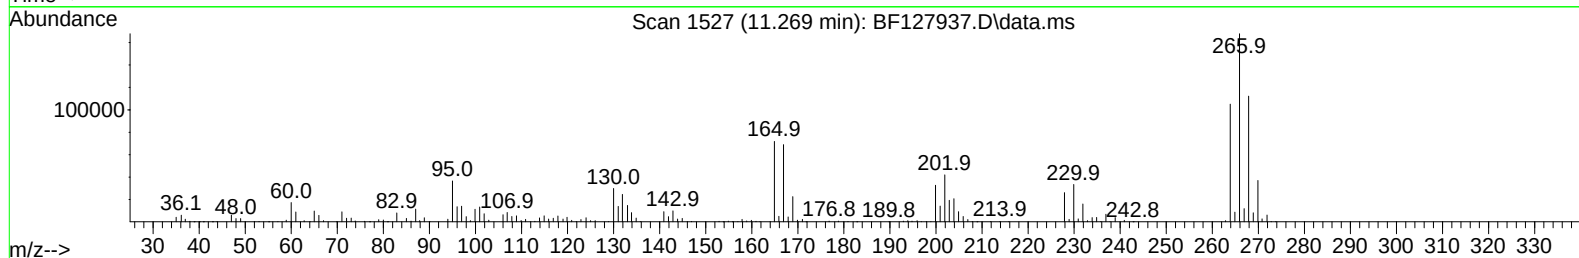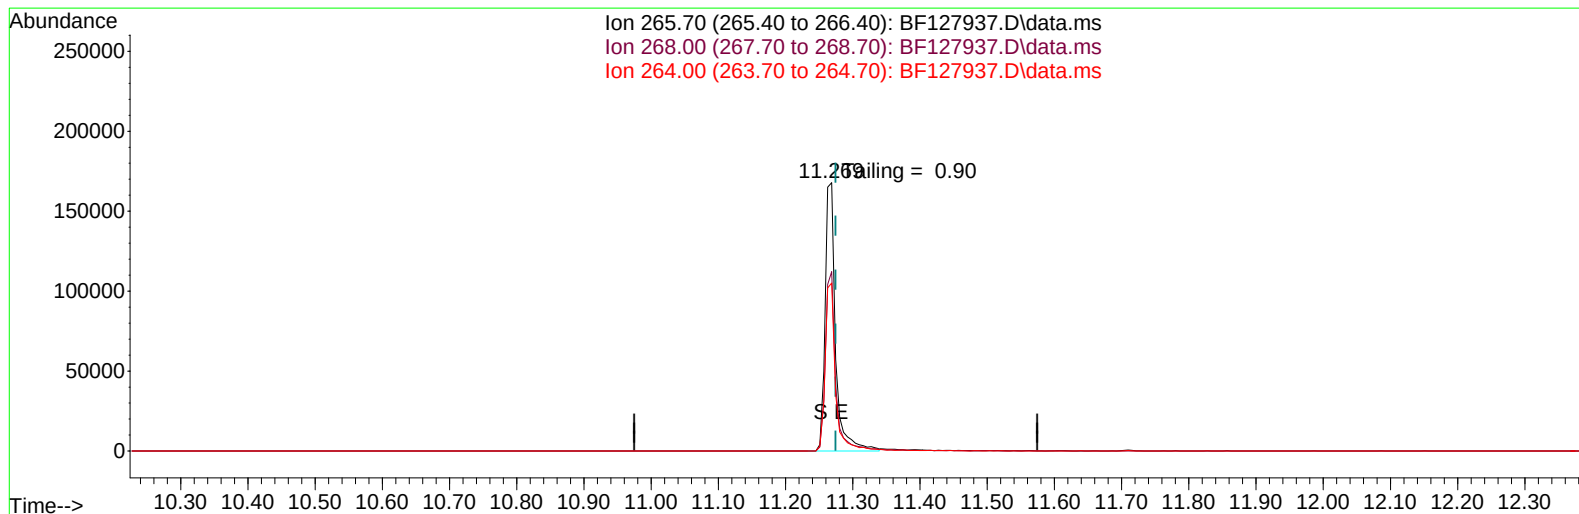

TIC: BF127937.D\data.ms

(70) Pentachlorophenol (C)

11.269min (-0.006) 399318.13 ng




response 183833

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	66.83
264.00	66.40	62.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042722\
Data File : BF127937.D
Acq On : 27 Apr 2022 11:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 27 17:52:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 00:43:03 2022
Response via : Initial Calibration

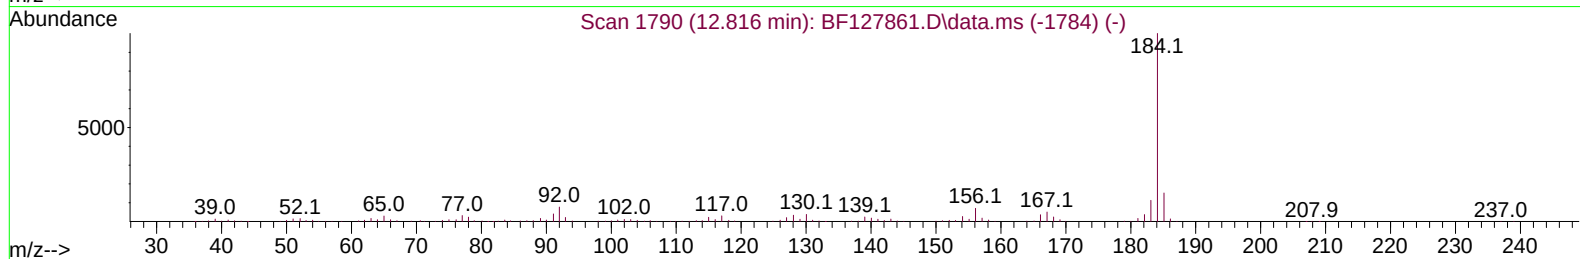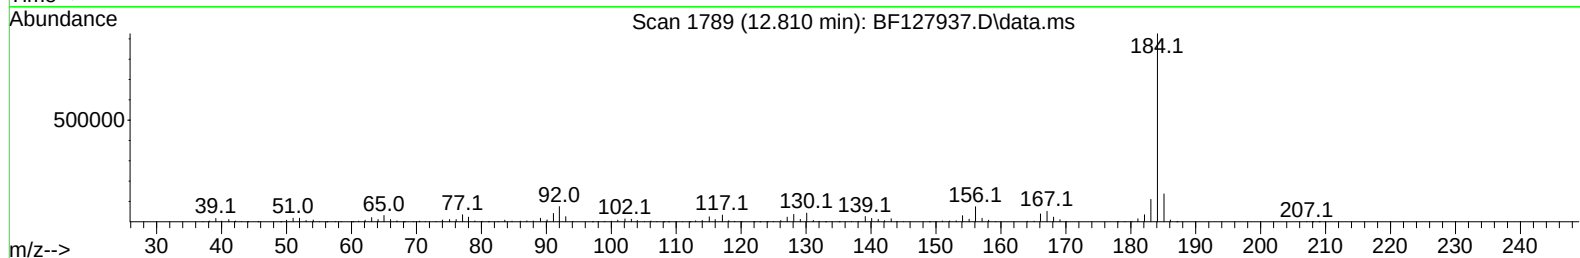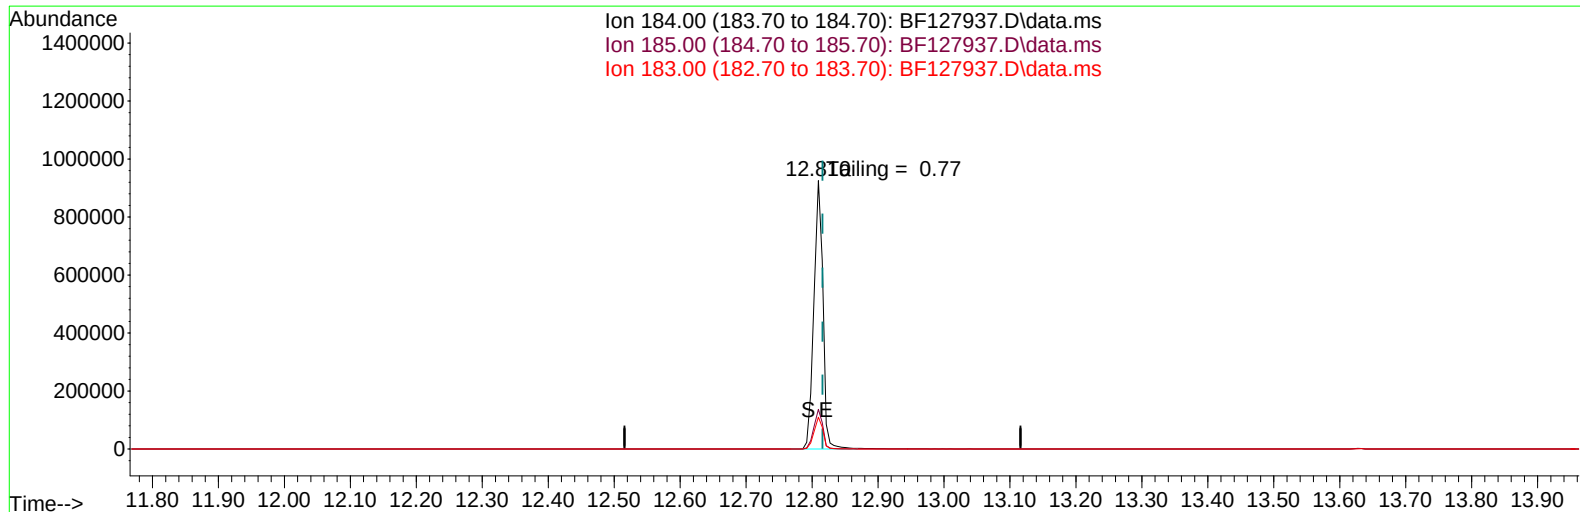

TIC: BF127937.D\data.ms

(77) Benzidine

12.810min (-0.006) 856985.51 ng

response 891847

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.79
183.00	11.20	11.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/27/2022	BNA_F	<u>BF127937.D</u>
Compound Name	Response	Retention Time
DDT	457207	13.62
DDD	5347	13.32
DDE	1434	12.99
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6781	463988	1.46