
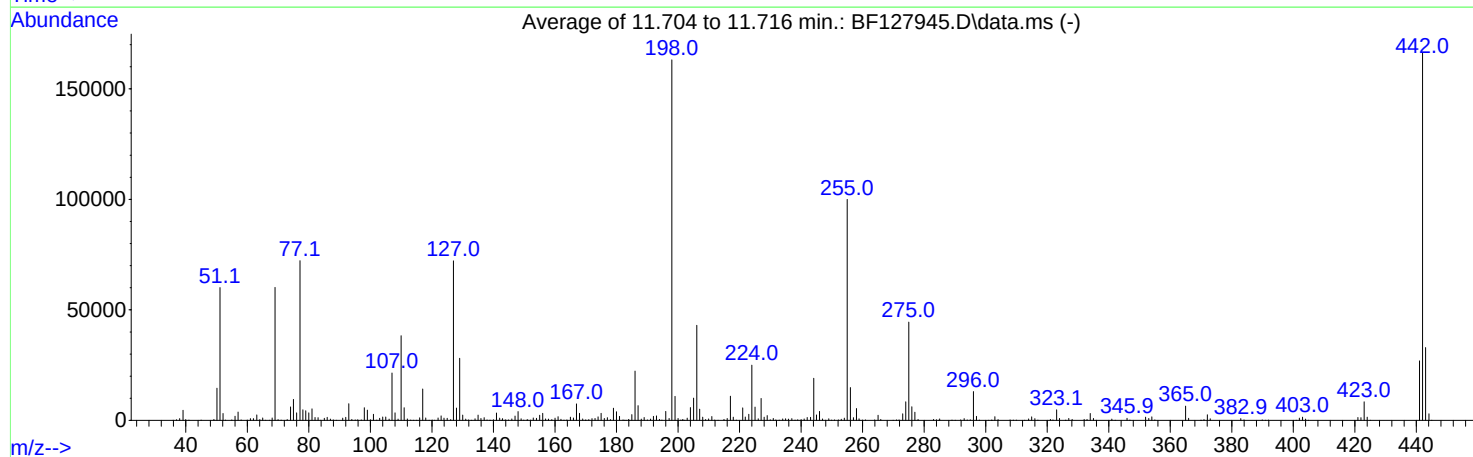


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042722\
 Data File : BF127945.D
 Acq On : 27 Apr 2022 15:08
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 28 05:13:03 2022

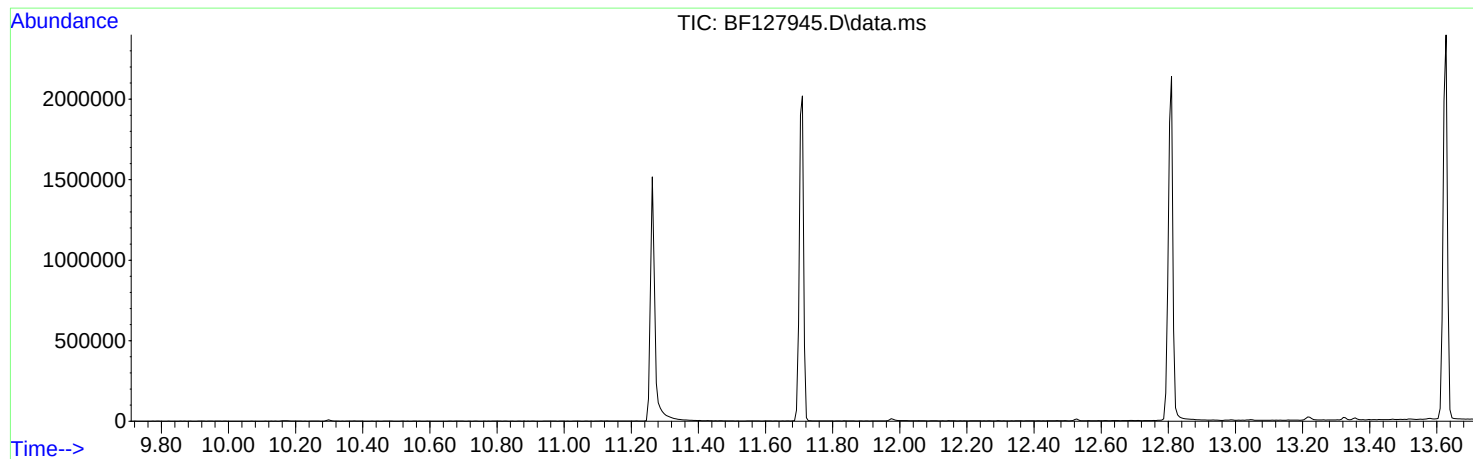




AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	60107	PASS
68	69	0.00	2	1.8	1080	PASS
69	198	0.00	100	36.9	60182	PASS
70	69	0.00	2	0.6	354	PASS
127	198	10	80	44.2	72165	PASS
197	198	0.00	2	0.5	867	PASS
198	198	100	100	100.0	163104	PASS
199	198	5	9	6.7	10853	PASS
275	198	10	60	27.3	44480	PASS
365	198	1	100	4.0	6462	PASS
441	198	0.01	100	16.5	26907	PASS
442	442	50	100	100.0	166459	PASS
443	442	15	24	19.8	32952	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042722\
 Data File : BF127945.D
 Acq On : 27 Apr 2022 15:08
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 27 17:45:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Apr 24 00:43:03 2022
 Response via : Initial Calibration

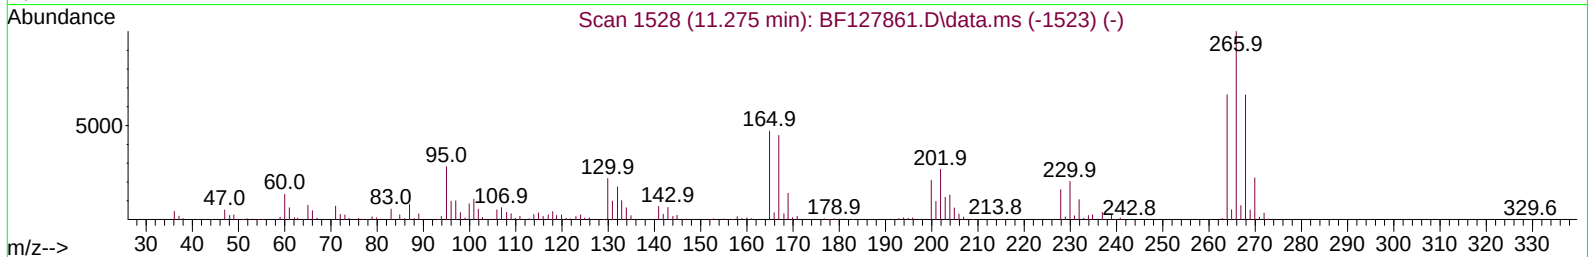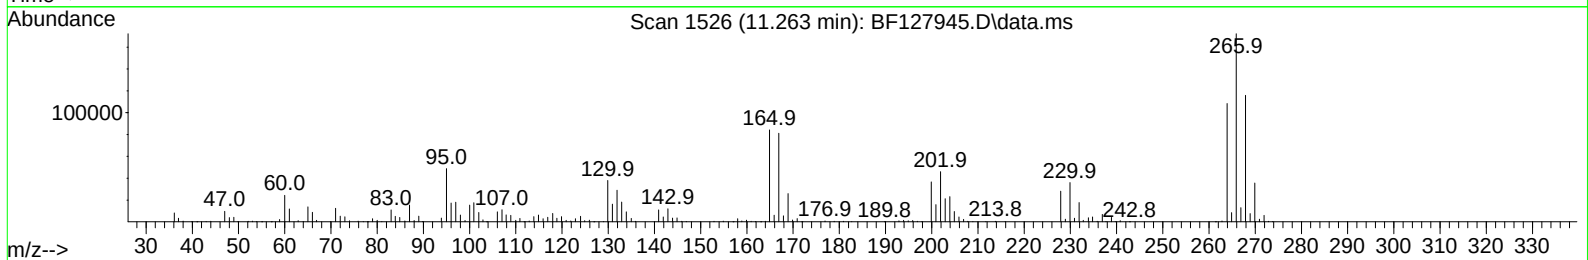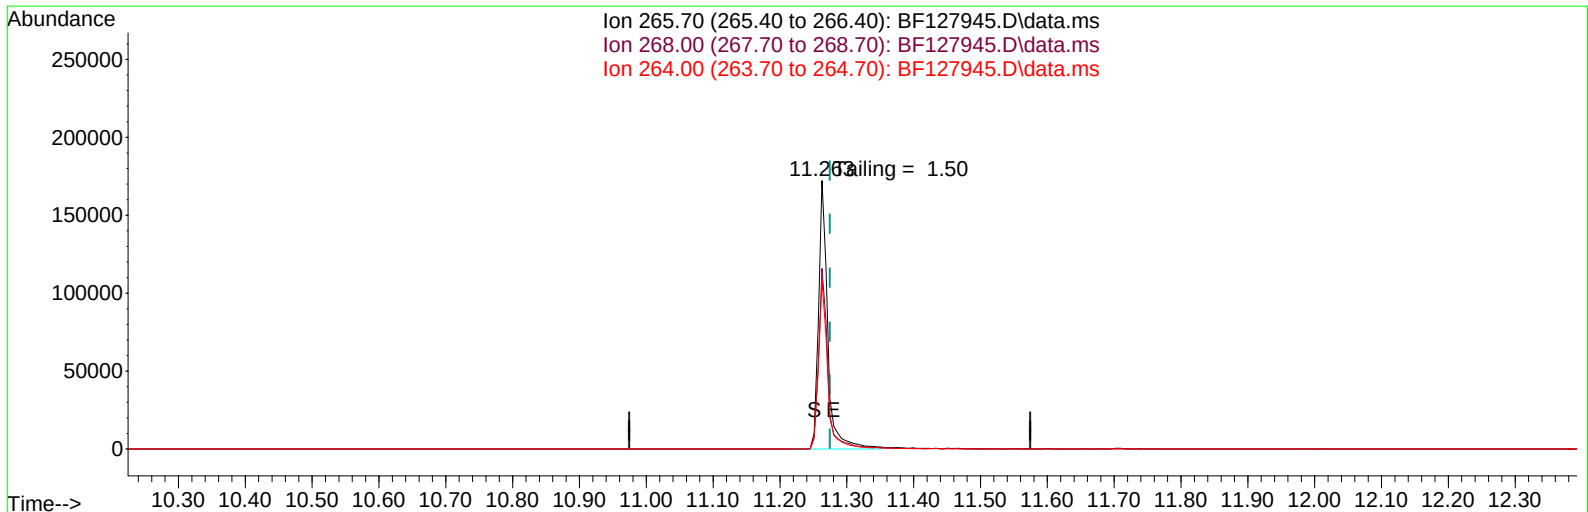

TIC: BF127945.D\data.ms

(70) Pentachlorophenol (C)

11.263min (-0.012) 158127.67 ng




response 167324

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	67.27
264.00	66.40	62.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042722\
 Data File : BF127945.D
 Acq On : 27 Apr 2022 15:08
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 27 17:45:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Apr 24 00:43:03 2022
 Response via : Initial Calibration

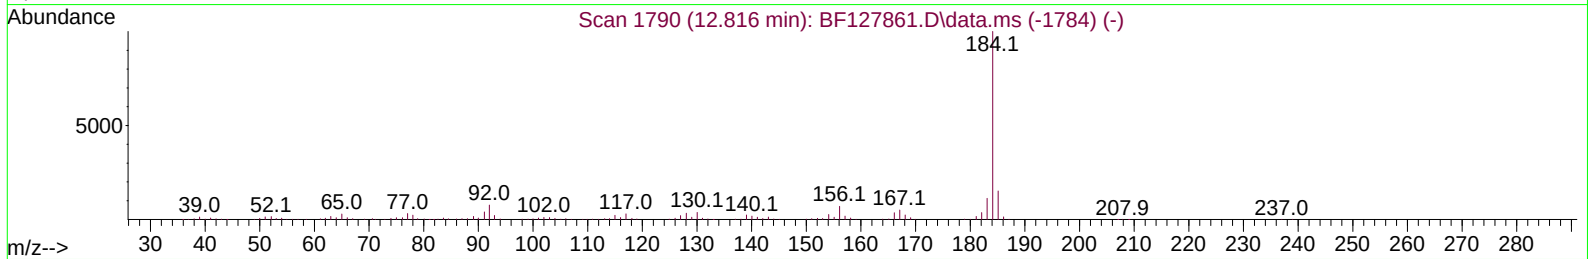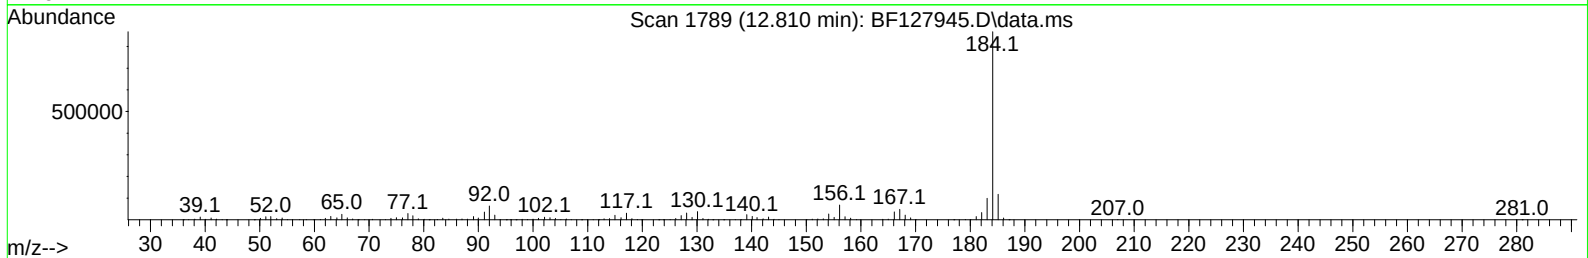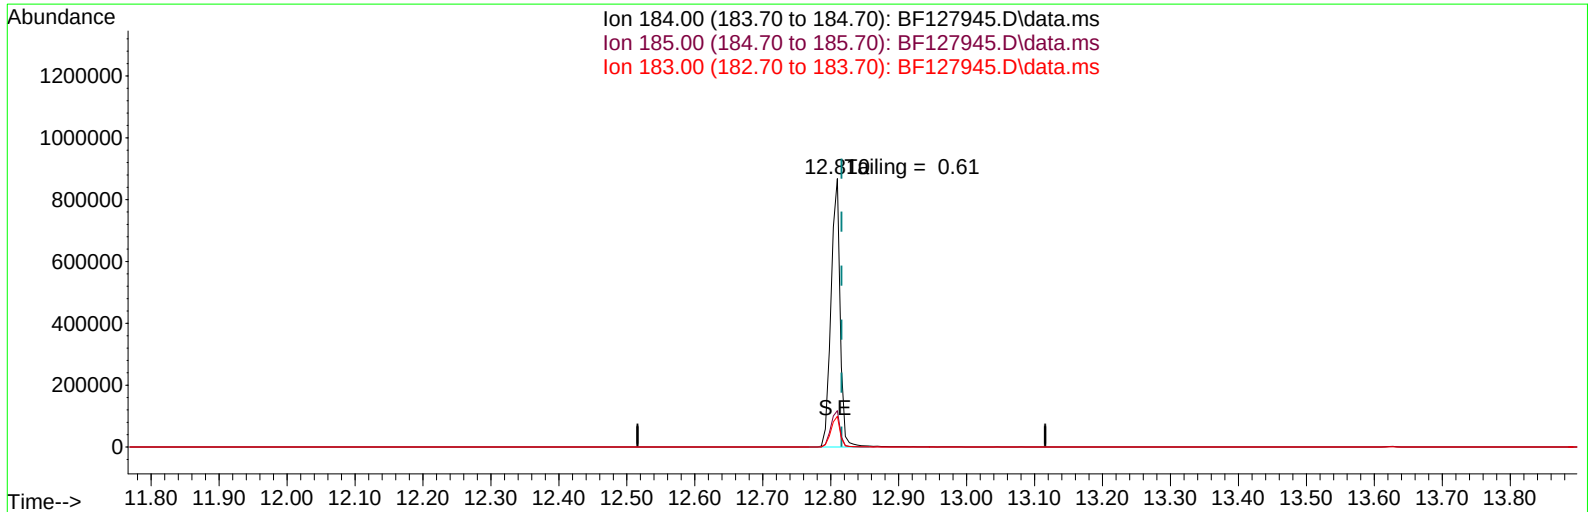

TIC: BF127945.D\data.ms

(77) Benzidine

12.810min (-0.006) 97720.20 ng

response 811714

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.54
183.00	11.20	11.46
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/27/2022	BNA_F	<u>BF127945.D</u>
Compound Name	Response	Retention Time
DDT	407638	13.62
DDD	3241	13.32
DDE	373	12.99
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3614	411252	0.88