
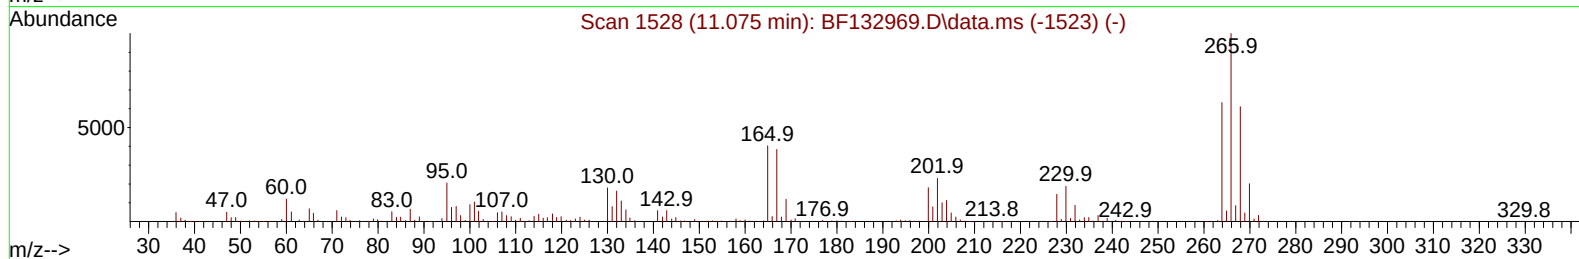
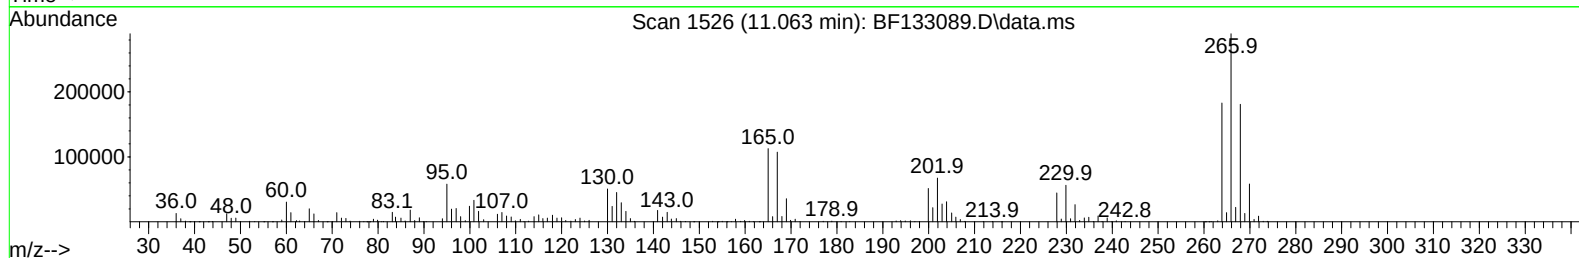


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042723\
Data File : BF133089.D
Acq On : 27 Apr 2023 09:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 05:13:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 28 02:00:53 2023
Response via : Initial Calibration

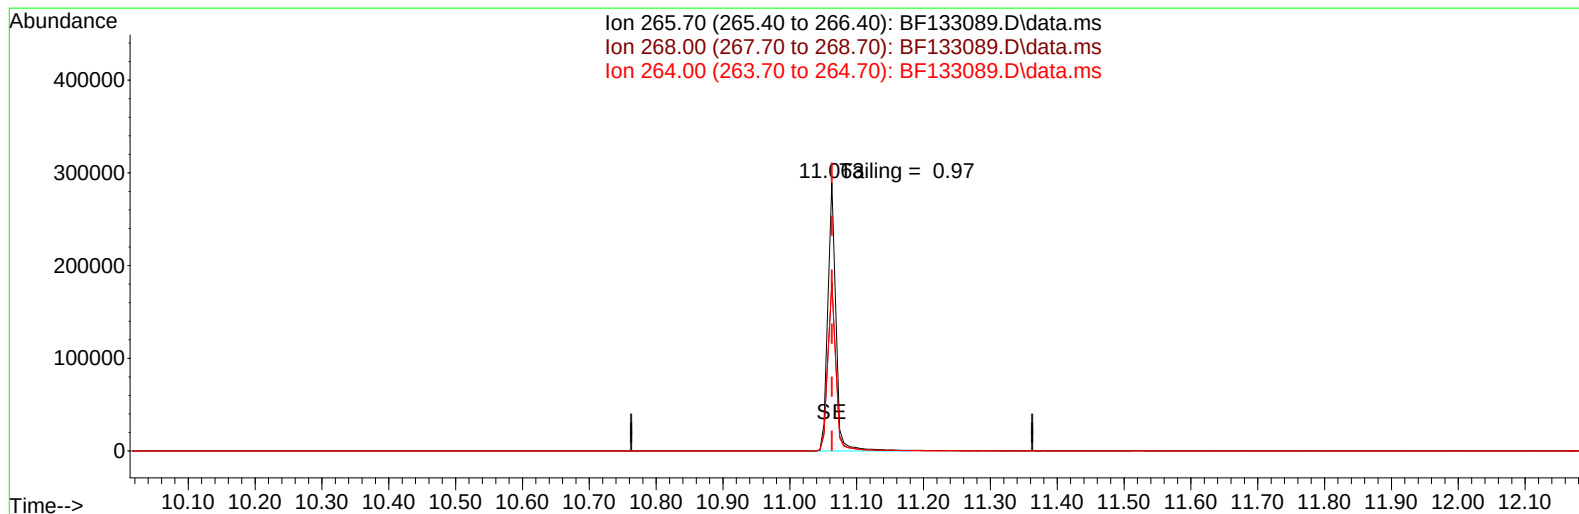

TIC: BF133089.D\data.ms

(70) Pentachlorophenol (C)




11.063min (-0.000) 37163.58 ng

response 245022

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	62.48
264.00	63.30	63.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042723\
Data File : BF133089.D
Acq On : 27 Apr 2023 09:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 05:13:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 28 02:00:53 2023
Response via : Initial Calibration

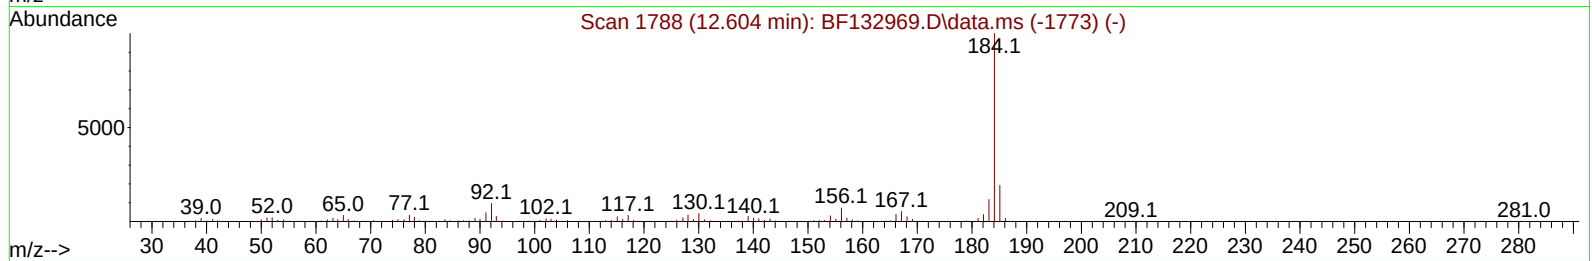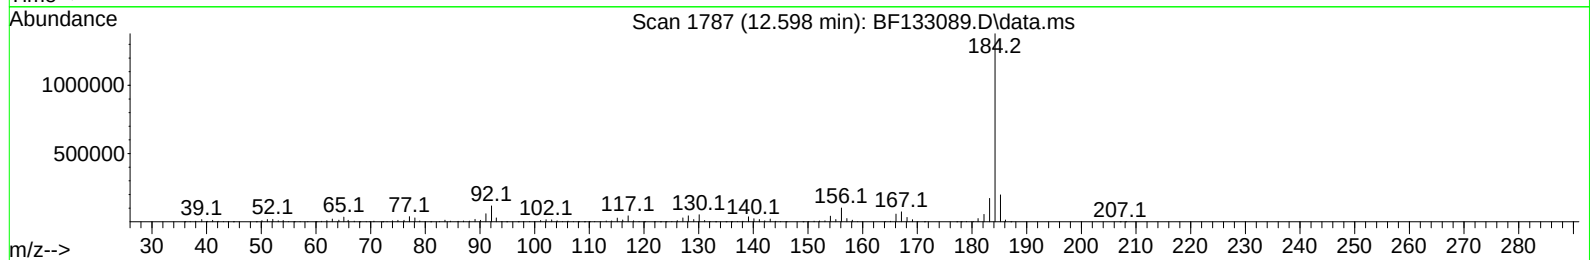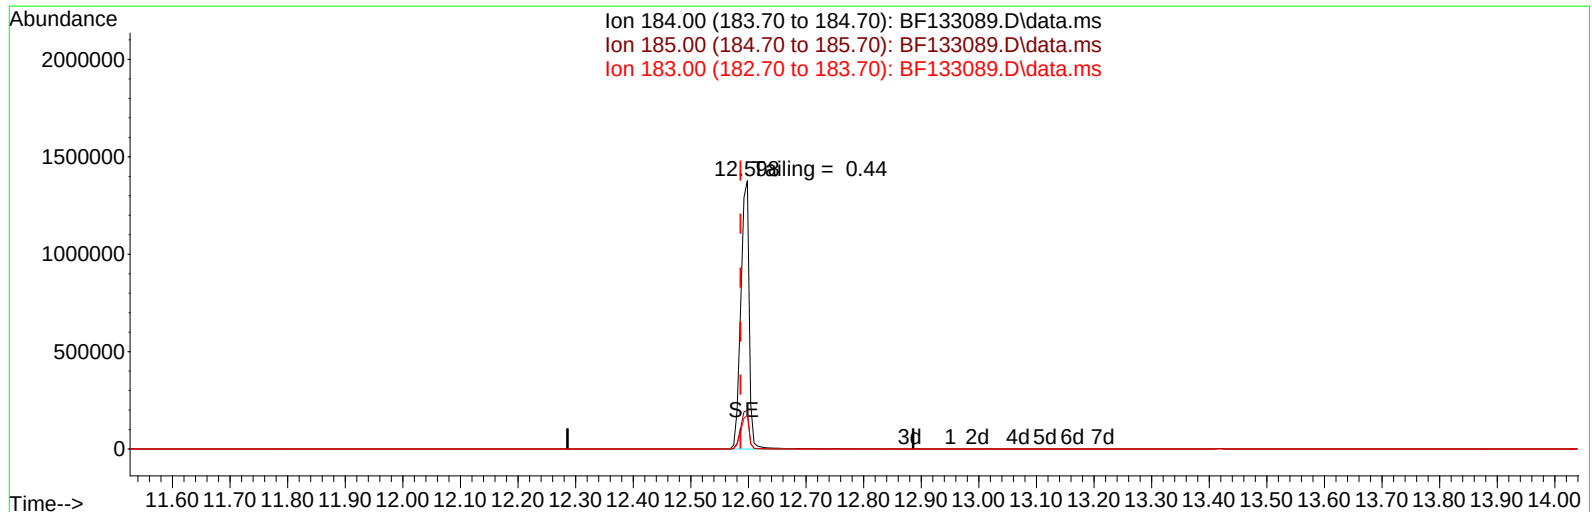

TIC: BF133089.D\data.ms

(77) Benzidine**12.598min (+ 0.012) 1381697.62 ng****response 1401914**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.31#
183.00	11.70	12.44
0.00	0.00	0.00