

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042723\
 Data File : BF133097.D
 Acq On : 27 Apr 2023 13:49
 Operator : CG\JU
 Sample : 02448-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 20230345-COMP-23

Quant Time: Apr 28 02:07:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 28 02:00:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.734	152	212234	20.000	ng	0.00
21) Naphthalene-d8	8.016	136	882994	20.000	ng	0.00
39) Acenaphthene-d10	9.769	164	465254	20.000	ng	0.00
64) Phenanthrene-d10	11.251	188	830163	20.000	ng	0.00
76) Chrysene-d12	13.886	240	555745	20.000	ng	-0.01
86) Perylene-d12	15.309	264	484798	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.357	112	1486080	105.774	ng	0.01
7) Phenol-d6	6.375	99	1843706	105.727	ng	0.00
23) Nitrobenzene-d5	7.298	82	1097815	67.109	ng	0.00
42) 2,4,6-Tribromophenol	10.563	330	519763	111.084	ng	0.00
45) 2-Fluorobiphenyl	9.098	172	1895050	68.144	ng	0.00
79) Terphenyl-d14	12.839	244	2026954	62.903	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042723\
Data File : BF133097.D
Acq On : 27 Apr 2023 13:49
Operator : CG\JU
Sample : 02448-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20230345-COMP-23

Quant Time: Apr 28 02:07:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 28 02:00:53 2023
Response via : Initial Calibration




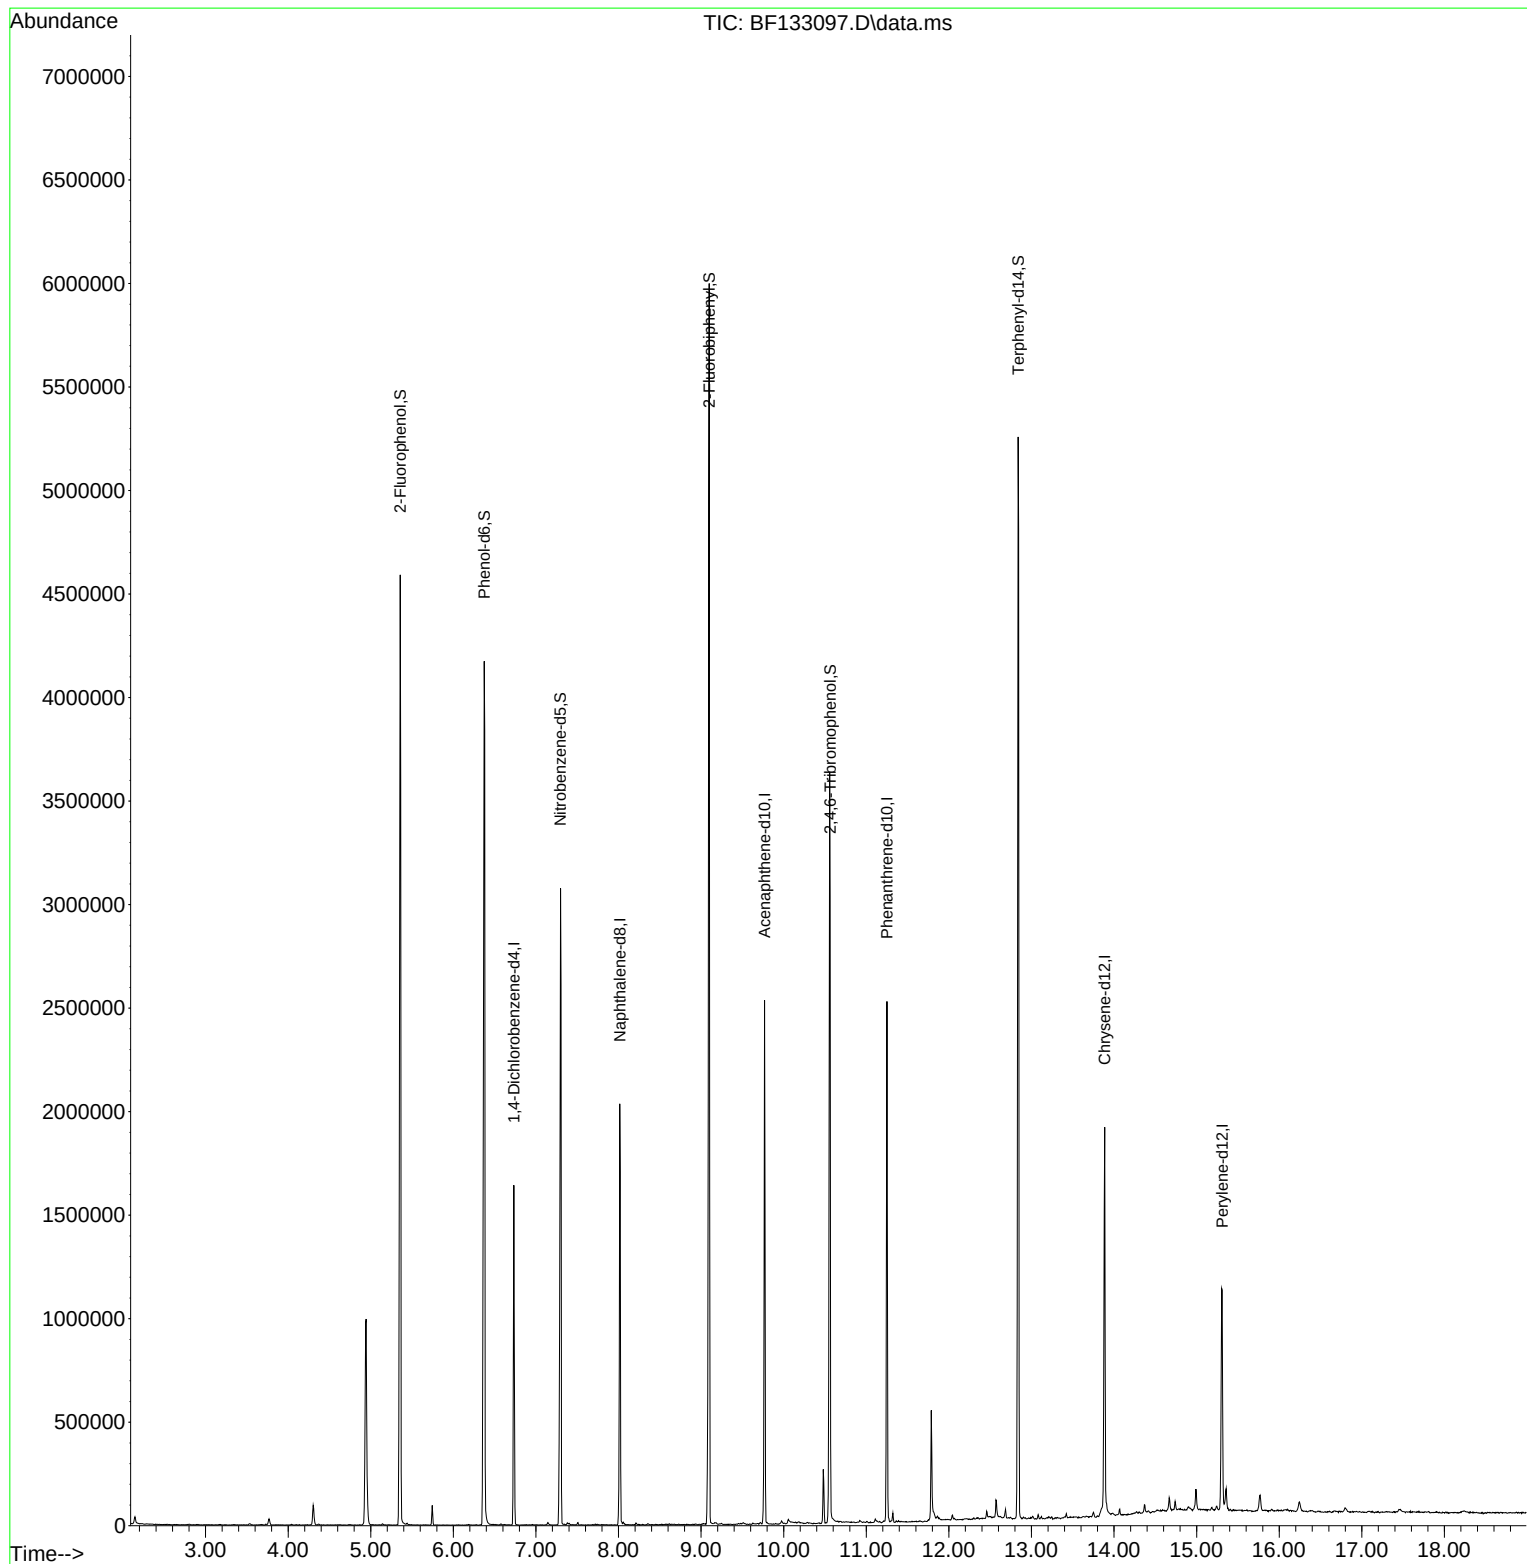


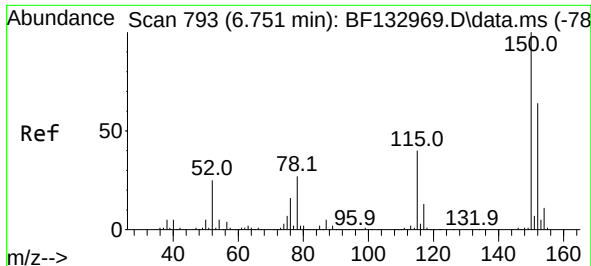

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.734 min Scan# 793
Delta R.T. -0.006 min
Lab File: BF133097.D
Acq: 27 Apr 2023 13:49




Instrument :
BNA_F
ClientSampleId :
20230345-COMP-23


Tgt Ion:152 Resp: 212234
Ion Ratio Lower Upper
152 100
150 161.5 124.8 187.2
115 61.8 49.9 74.9

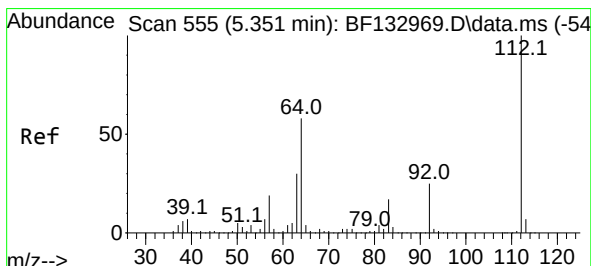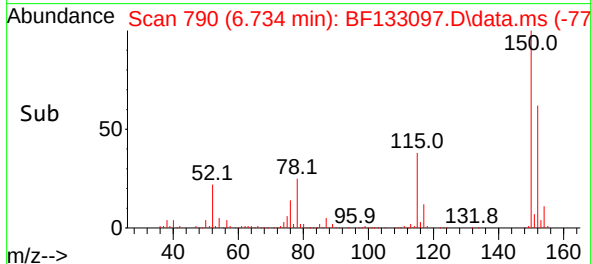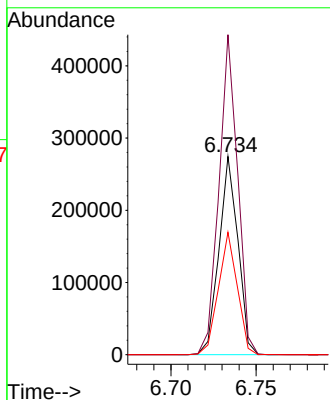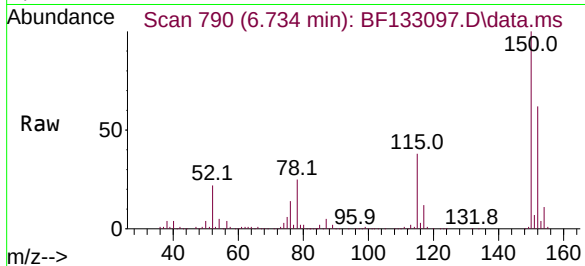

#5
2-Fluorophenol
Concen: 105.774 ng
RT: 5.357 min Scan# 556
Delta R.T. 0.011 min
Lab File: BF133097.D
Acq: 27 Apr 2023 13:49

Tgt Ion:112 Resp: 1486080
Ion Ratio Lower Upper
112 100
64 57.5 46.8 70.2
63 29.3 23.8 35.8


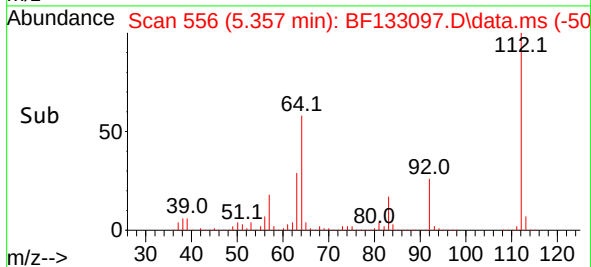
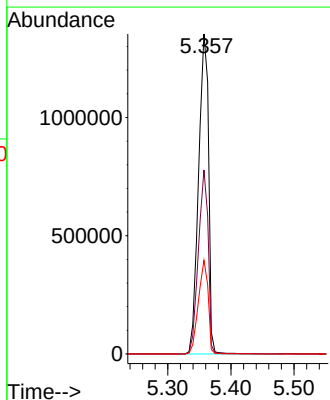
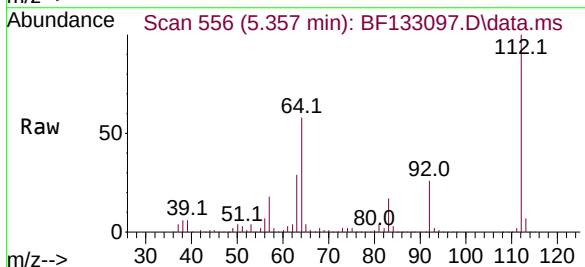


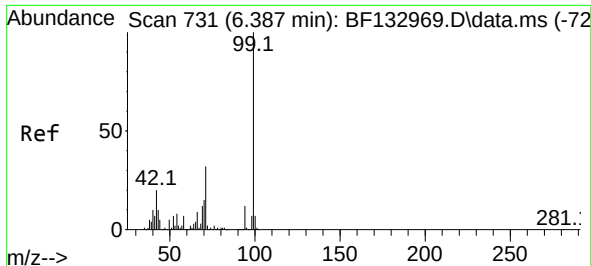

#7
Phenol-d6
Concen: 105.727 ng
RT: 6.375 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF133097.D
Acq: 27 Apr 2023 13:49




Instrument :
BNA_F
ClientSampleId :
20230345-COMP-23


Tgt Ion: 99 Resp: 1843706
Ion Ratio Lower Upper
99 100
42 19.1 16.3 24.5
71 33.0 25.6 38.4

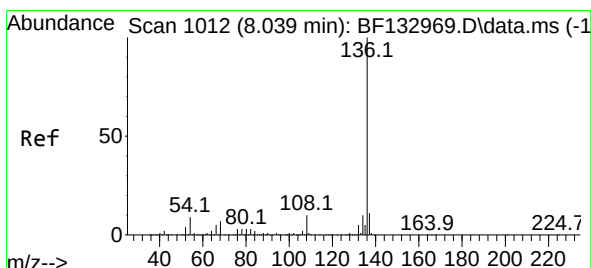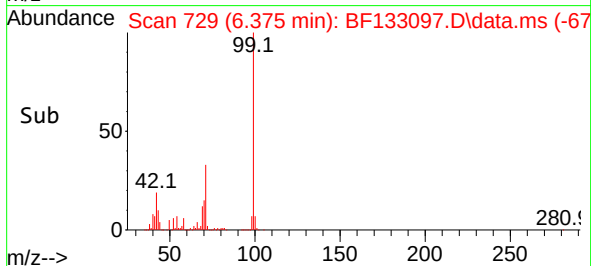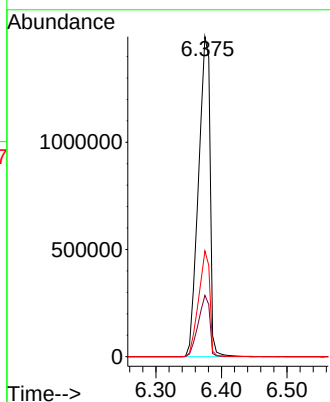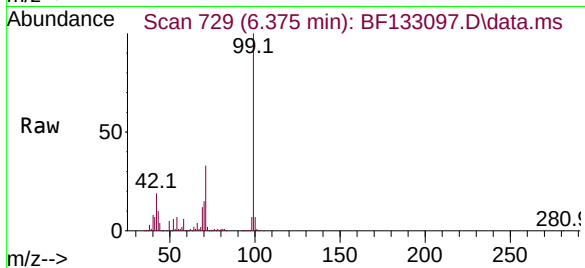

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.016 min Scan# 1008
Delta R.T. -0.006 min
Lab File: BF133097.D
Acq: 27 Apr 2023 13:49

Tgt Ion: 136 Resp: 882994
Ion Ratio Lower Upper
136 100
137 11.3 8.6 13.0
54 9.3 7.0 10.4
68 7.4 5.4 8.2

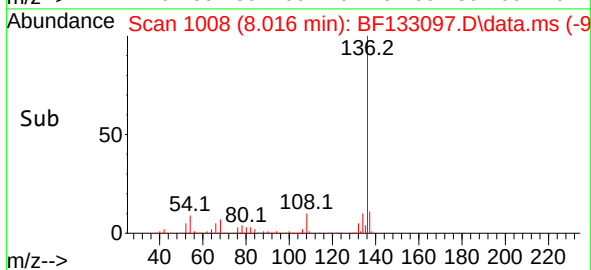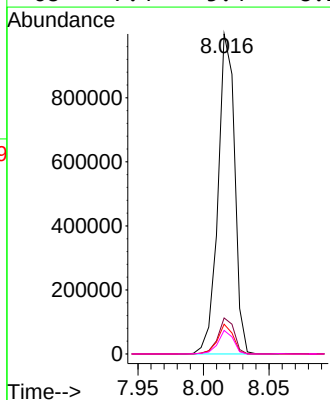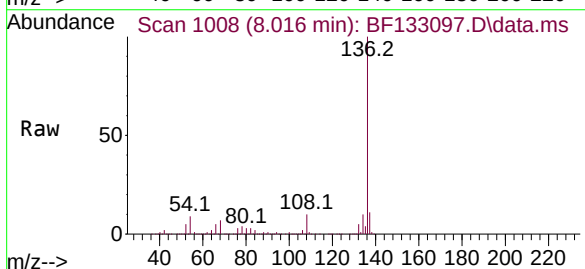

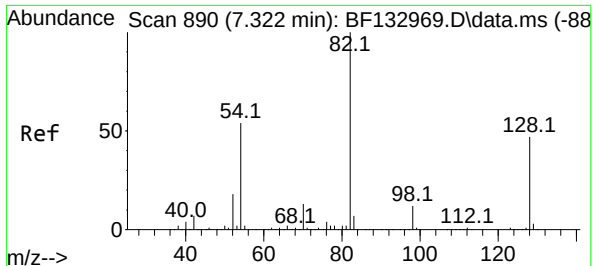

#23

Nitrobenzene-d5

Concen: 67.109 ng

RT: 7.298 min Scan# 81

Delta R.T. -0.006 min

Lab File: BF133097.D

Acq: 27 Apr 2023 13:49

Instrument :





BNA_F

ClientSampleId :

20230345-COMP-23

Tgt Ion: 82 Resp: 1097815

Ion	Ratio	Lower	Upper
82	100		
128	46.9	37.7	56.5
54	53.9	43.0	64.4

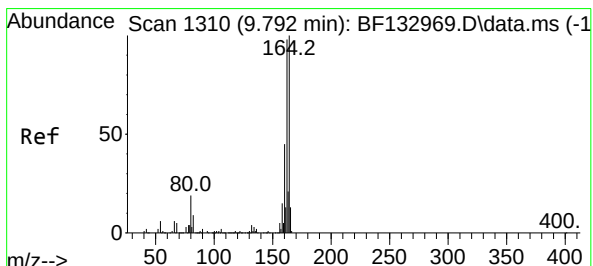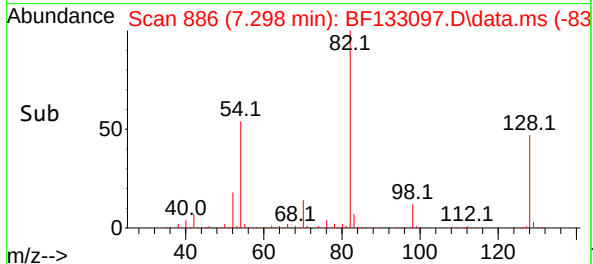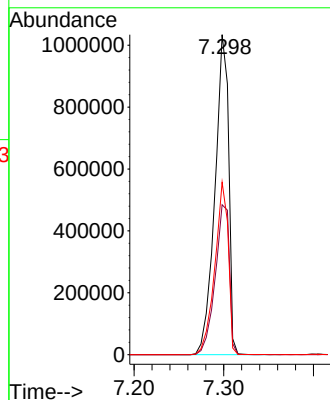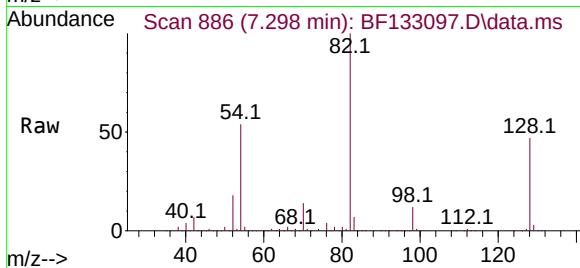

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.769 min Scan# 1306




Delta R.T. -0.006 min


Lab File: BF133097.D

Acq: 27 Apr 2023 13:49

Tgt Ion:164 Resp: 465254

Ion	Ratio	Lower	Upper
164	100		
162	101.1	78.7	118.1
160	44.2	35.8	53.6

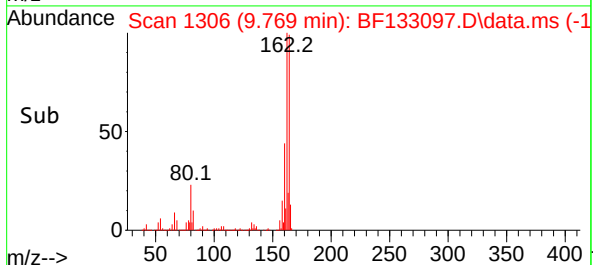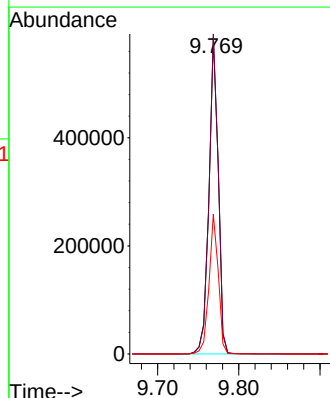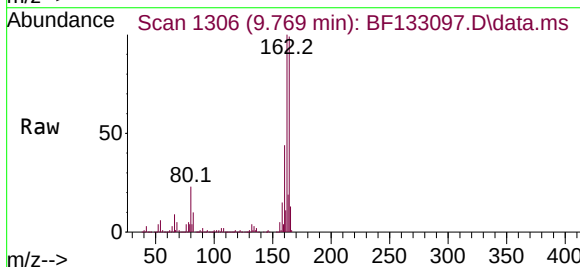

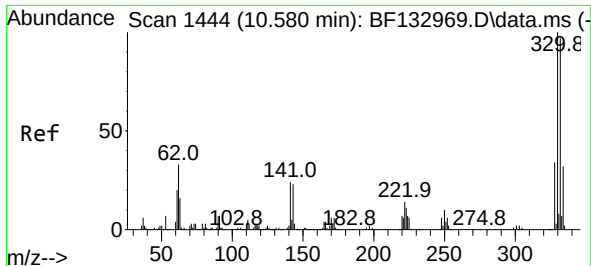

#42

2,4,6-Tribromophenol

Concen: 111.084 ng

RT: 10.563 min Scan# 1441

Delta R.T. -0.000 min

Lab File: BF133097.D


Acq: 27 Apr 2023 13:49

Instrument :

BNA_F

ClientSampleId :

20230345-COMP-23

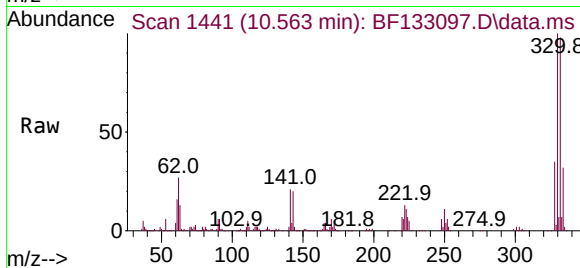




Tgt Ion:330 Resp: 519763

Ion Ratio Lower Upper

330 100

332 96.5 77.1 115.7

141 28.7 25.8 38.8

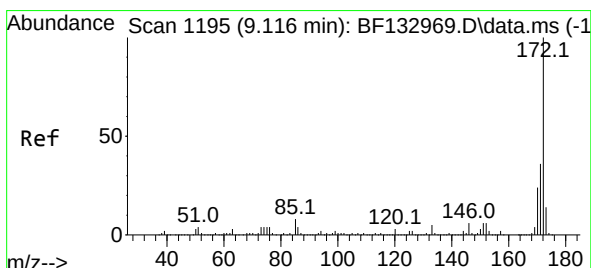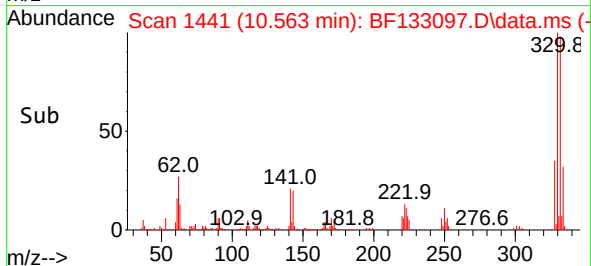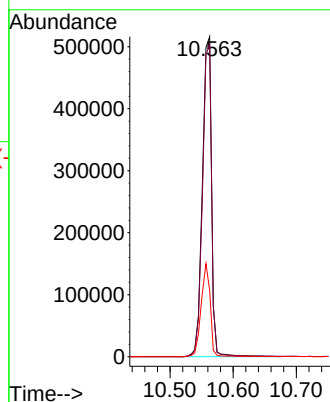

#45

2-Fluorobiphenyl

Concen: 68.144 ng

RT: 9.098 min Scan# 1192

Delta R.T. -0.000 min

Lab File: BF133097.D

Acq: 27 Apr 2023 13:49




Tgt Ion:172 Resp: 1895050


Ion Ratio Lower Upper

172 100

171 36.8 28.8 43.2

170 24.6 19.4 29.2


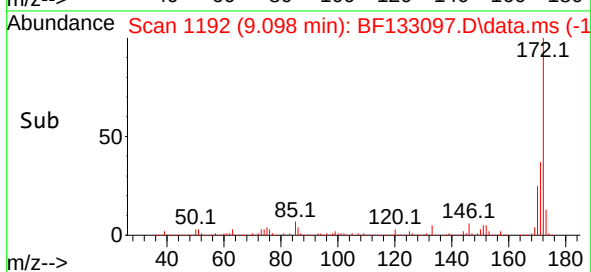
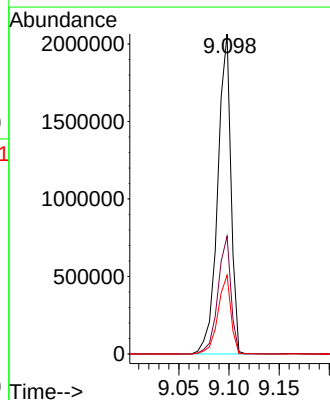
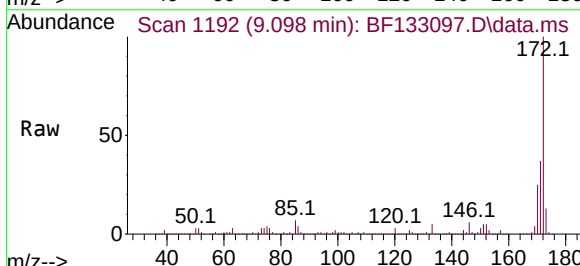


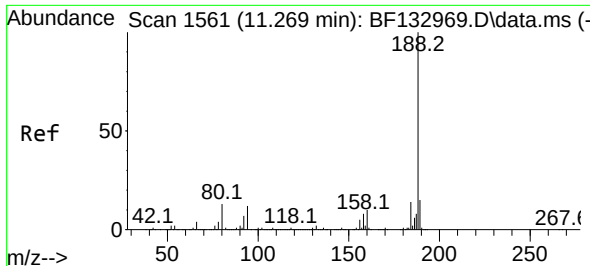

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.251 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF133097.D
Acq: 27 Apr 2023 13:49




Instrument :
BNA_F
ClientSampleId :
20230345-COMP-23


Tgt Ion:188 Resp: 830163
Ion Ratio Lower Upper
188 100
94 11.2 9.7 14.5
80 11.5 10.4 15.6

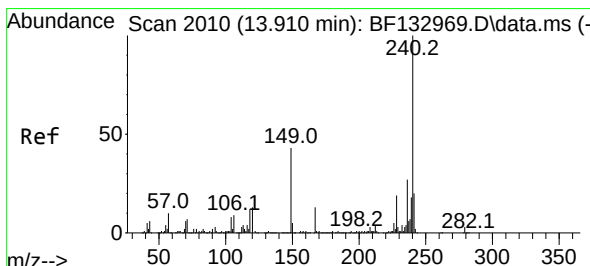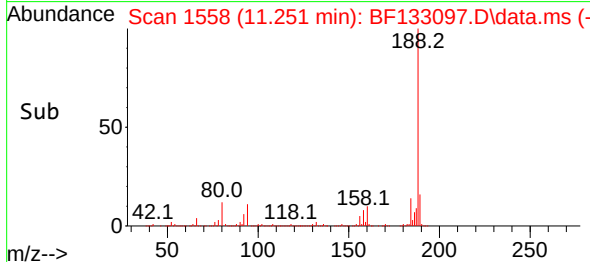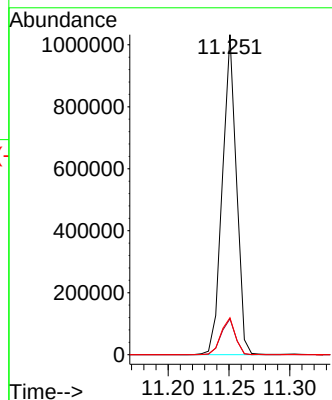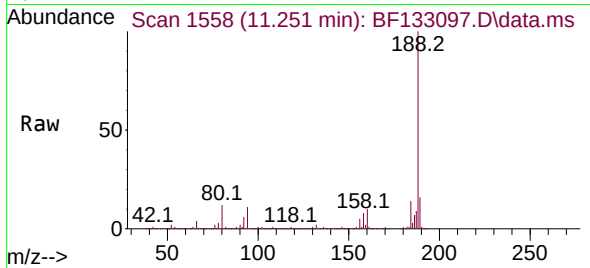

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.886 min Scan# 2006
Delta R.T. -0.012 min
Lab File: BF133097.D
Acq: 27 Apr 2023 13:49

Tgt Ion:240 Resp: 555745
Ion Ratio Lower Upper
240 100
120 13.2 10.5 15.7
236 26.3 21.5 32.3


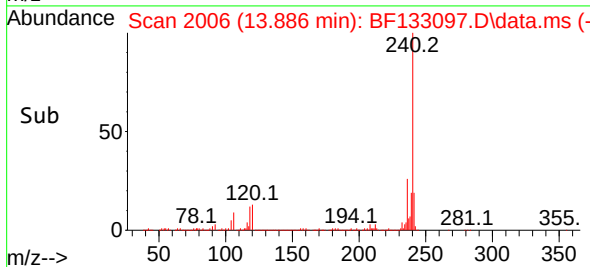
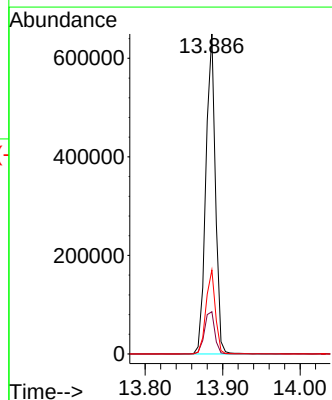
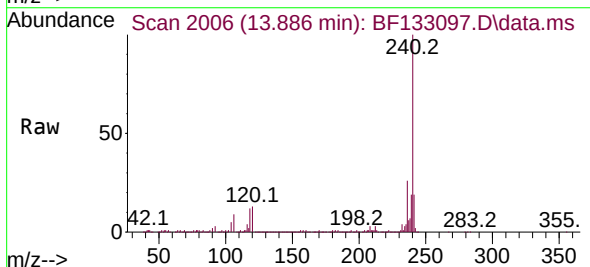


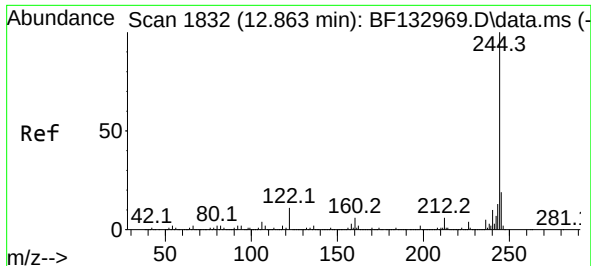

#79
 Terphenyl-d14
 Concen: 62.903 ng
 RT: 12.839 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BF133097.D
 Acq: 27 Apr 2023 13:49

Instrument :
 BNA_F
 ClientSampleId :
 20230345-COMP-23

Tgt Ion:244 Resp: 2026954
 Ion Ratio Lower Upper
 244 100
 212 6.5 5.1 7.7
 122 12.8 8.6 13.0

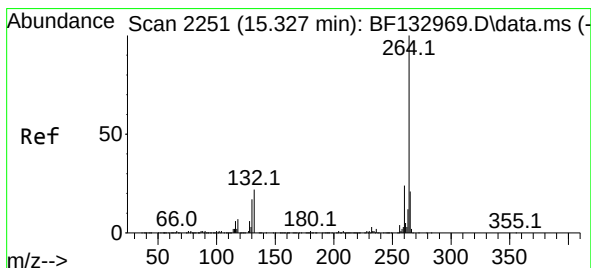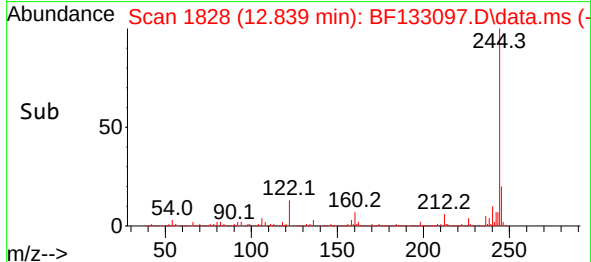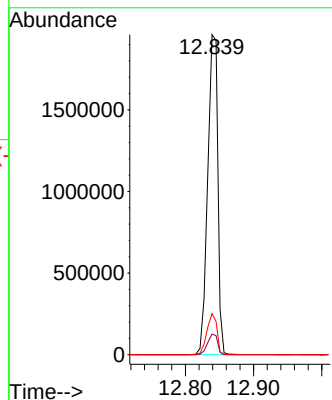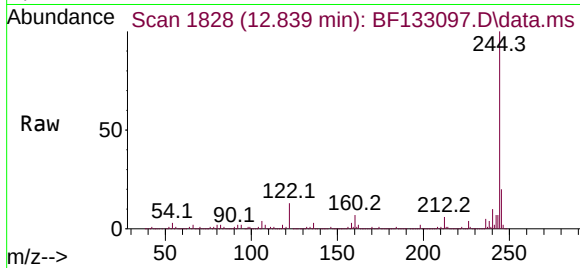

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.309 min Scan# 2248
 Delta R.T. -0.006 min
 Lab File: BF133097.D
 Acq: 27 Apr 2023 13:49

Tgt Ion:264 Resp: 484798
 Ion Ratio Lower Upper
 264 100
 260 23.9 18.8 28.2
 265 21.4 17.0 25.4

