


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042723\
 Data File : BF133089.D
 Acq On : 27 Apr 2023 09:29
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 28 02:00:53 2023

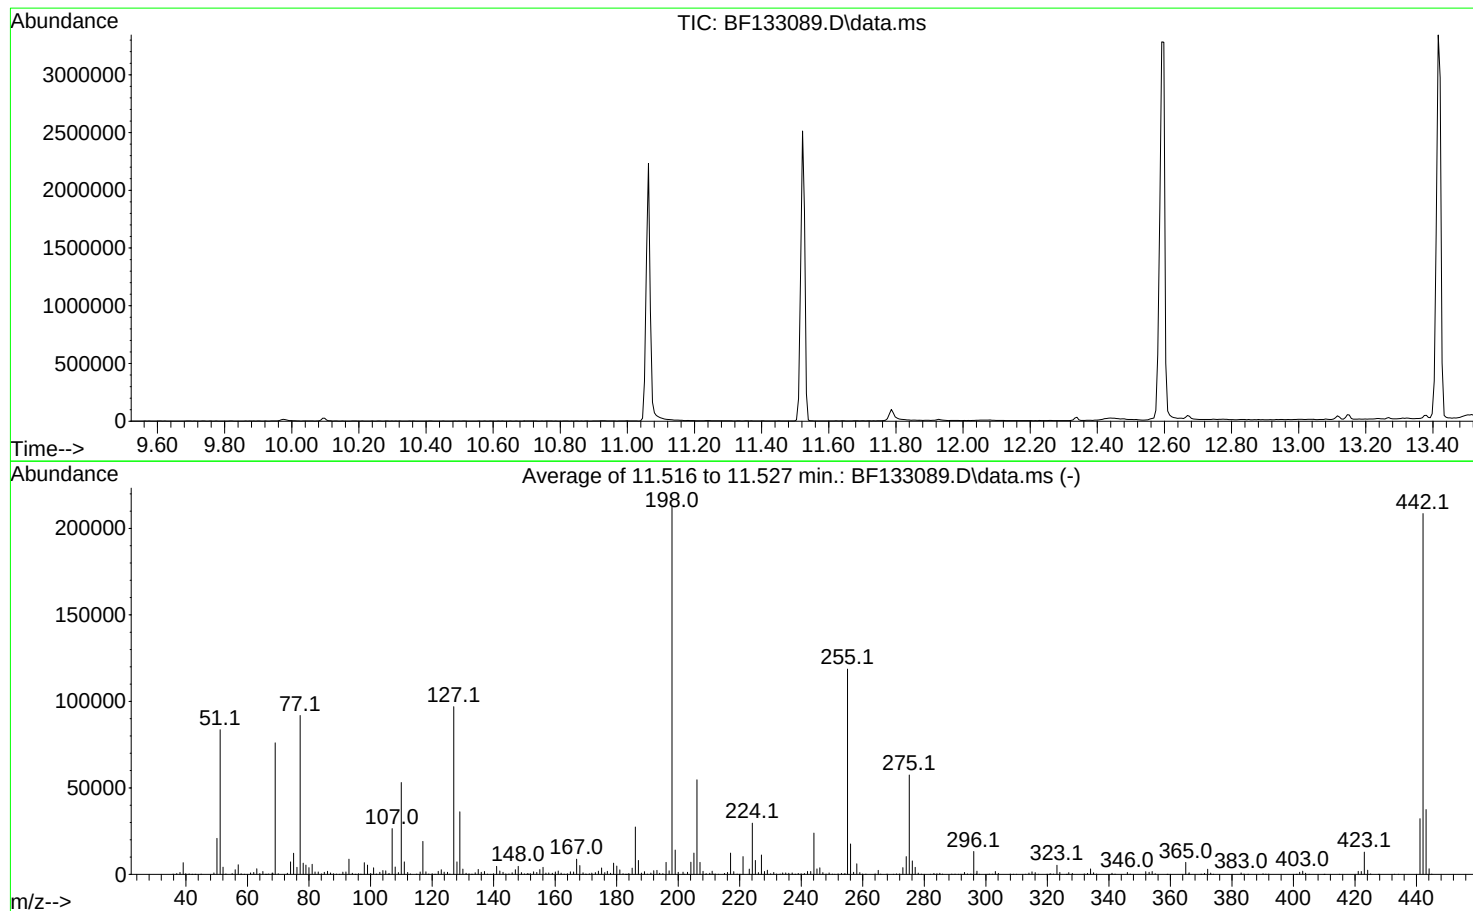

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	83619	PASS
68	69	0.00	2	0.9	718	PASS
69	198	0.00	100	35.8	76046	PASS
70	69	0.00	2	0.5	398	PASS
127	198	10	80	45.6	96984	PASS
197	198	0.00	2	1.0	2059	PASS
198	198	100	100	100.0	212672	PASS
199	198	5	9	6.6	14026	PASS
275	198	10	60	27.0	57469	PASS
365	198	1	100	3.3	6928	PASS
441	198	0.01	100	15.1	32197	PASS
442	442	50	100	100.0	208568	PASS
443	442	15	24	18.0	37455	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/27/2023	BNA_F	<u>BF133089.D</u>
Compound Name	Response	Retention Time
DDT	618871	13.416
DDD	10355	13.145
DDE	658	12.786
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11013	629884	1.75

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042723\
Data File : BF133089.D
Acq On : 27 Apr 2023 09:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 28 05:13:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 28 02:00:53 2023
Response via : Initial Calibration

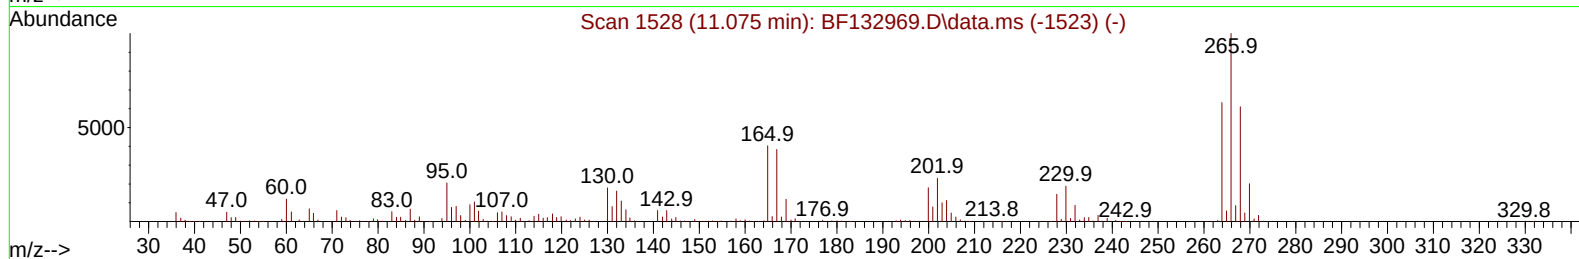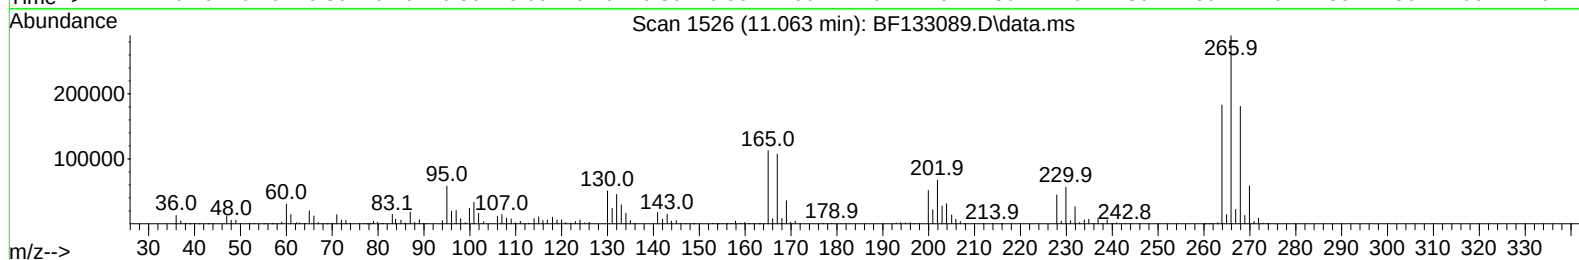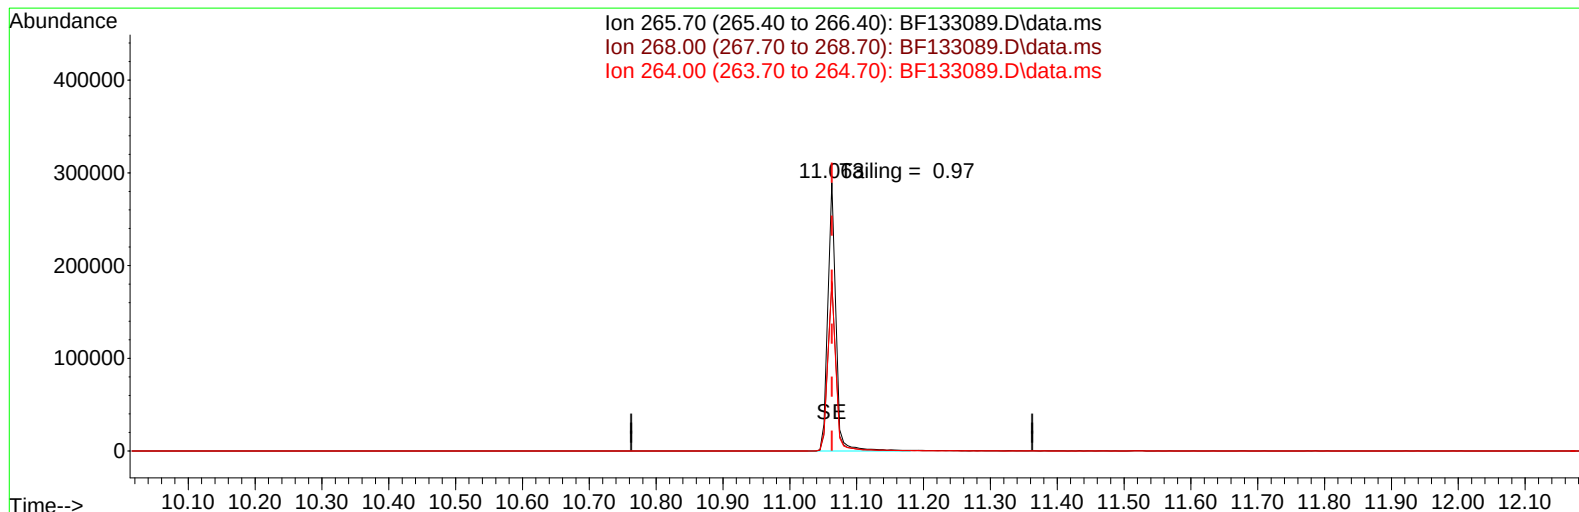

TIC: BF133089.D\data.ms

(70) Pentachlorophenol (C)

11.063min (-0.000) 37163.58 ng




response 245022

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	62.48
264.00	63.30	63.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042723\
 Data File : BF133089.D
 Acq On : 27 Apr 2023 09:29
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 28 05:13:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 28 02:00:53 2023
 Response via : Initial Calibration

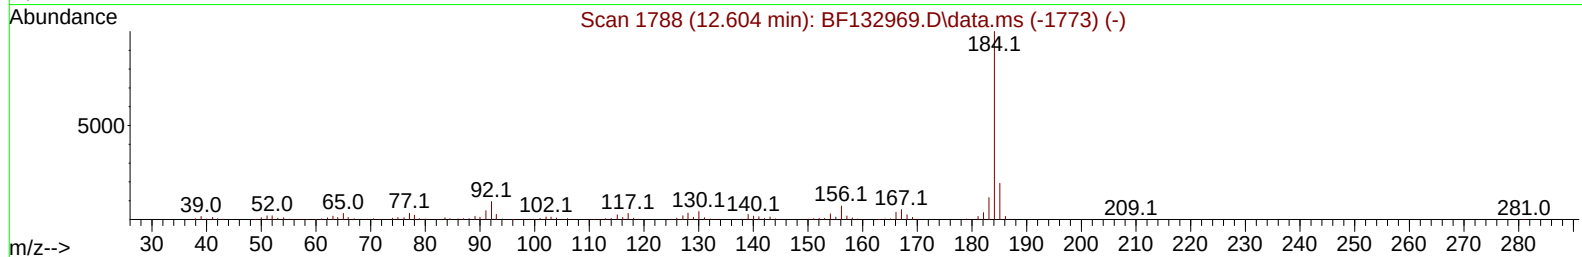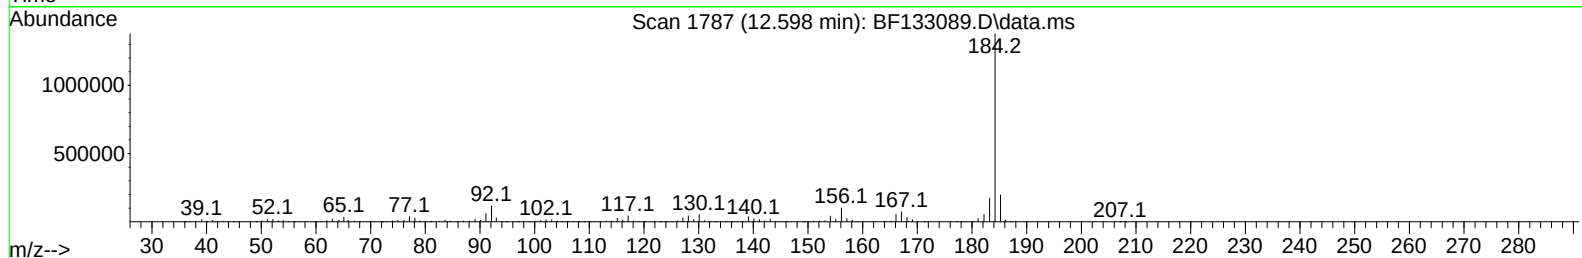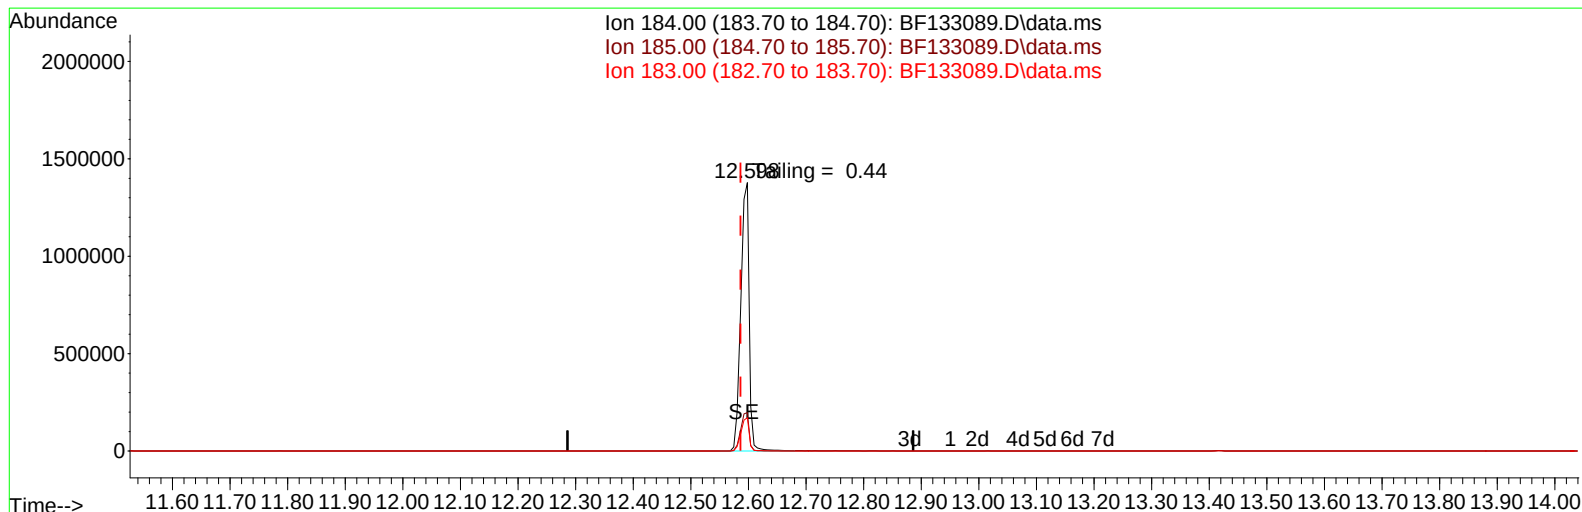

TIC: BF133089.D\data.ms

(77) Benzidine

12.598min (+ 0.012) 1381697.62 ng

response 1401914

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.31#
183.00	11.70	12.44
0.00	0.00	0.00