


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042815\
 Data File : BF078782.D
 Acq On : 28 Apr 2015 19:00
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 29 03:47:53 2015

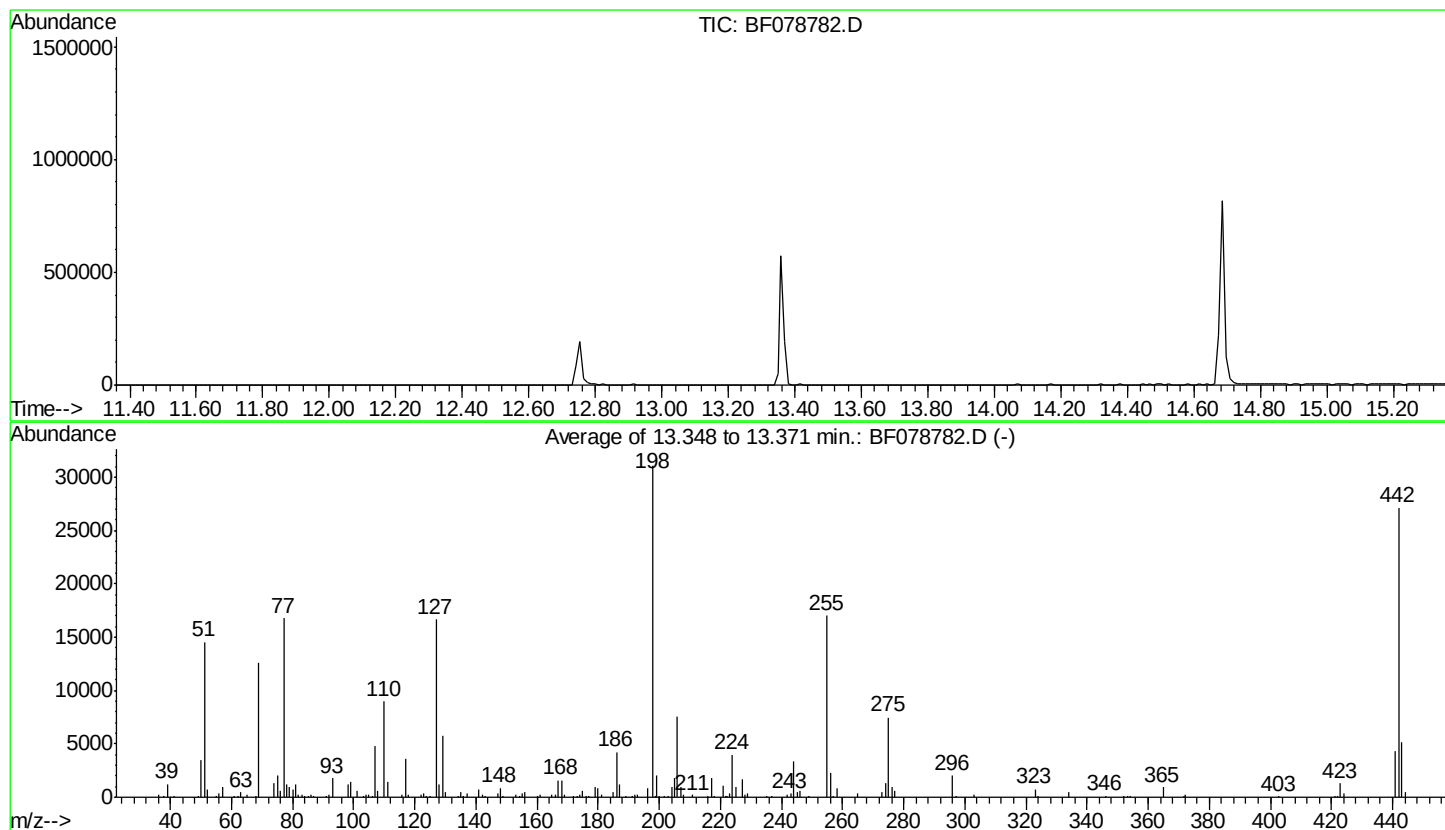

AutoFind: Scans 1064, 1065, 1066; Background Corrected with Scan 1061

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.8	14537	PASS
68	69	0.00	2	1.2	147	PASS
69	198	0.00	100	40.5	12565	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.6	16661	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	31063	PASS
199	198	5	9	6.4	2003	PASS
275	198	10	60	24.1	7480	PASS
365	198	1	100	3.1	959	PASS
441	442	0.01	24	16.0	4353	PASS
442	198	50	100	87.3	27125	PASS
443	442	15	24	18.8	5105	PASS