




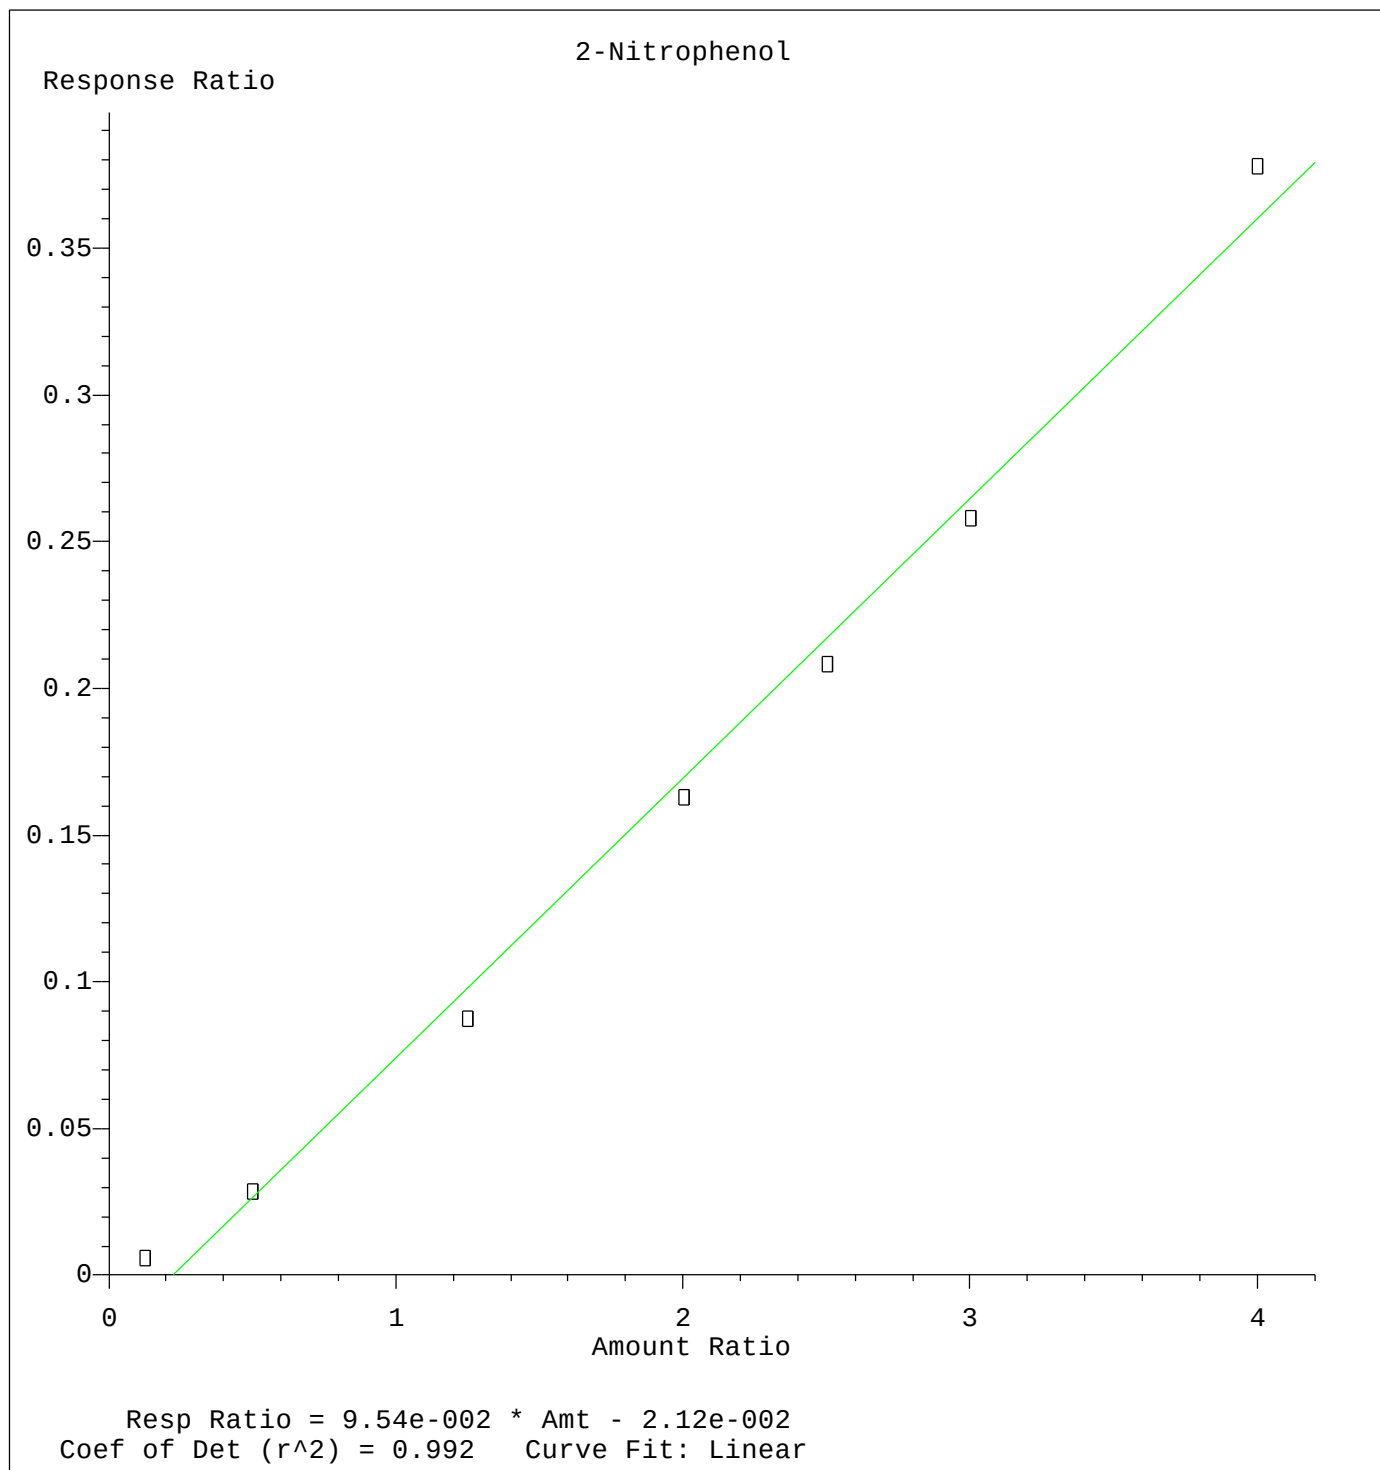


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF042815.M
Calibration Table Last Updated: Wed Apr 29 03:40:48 2015

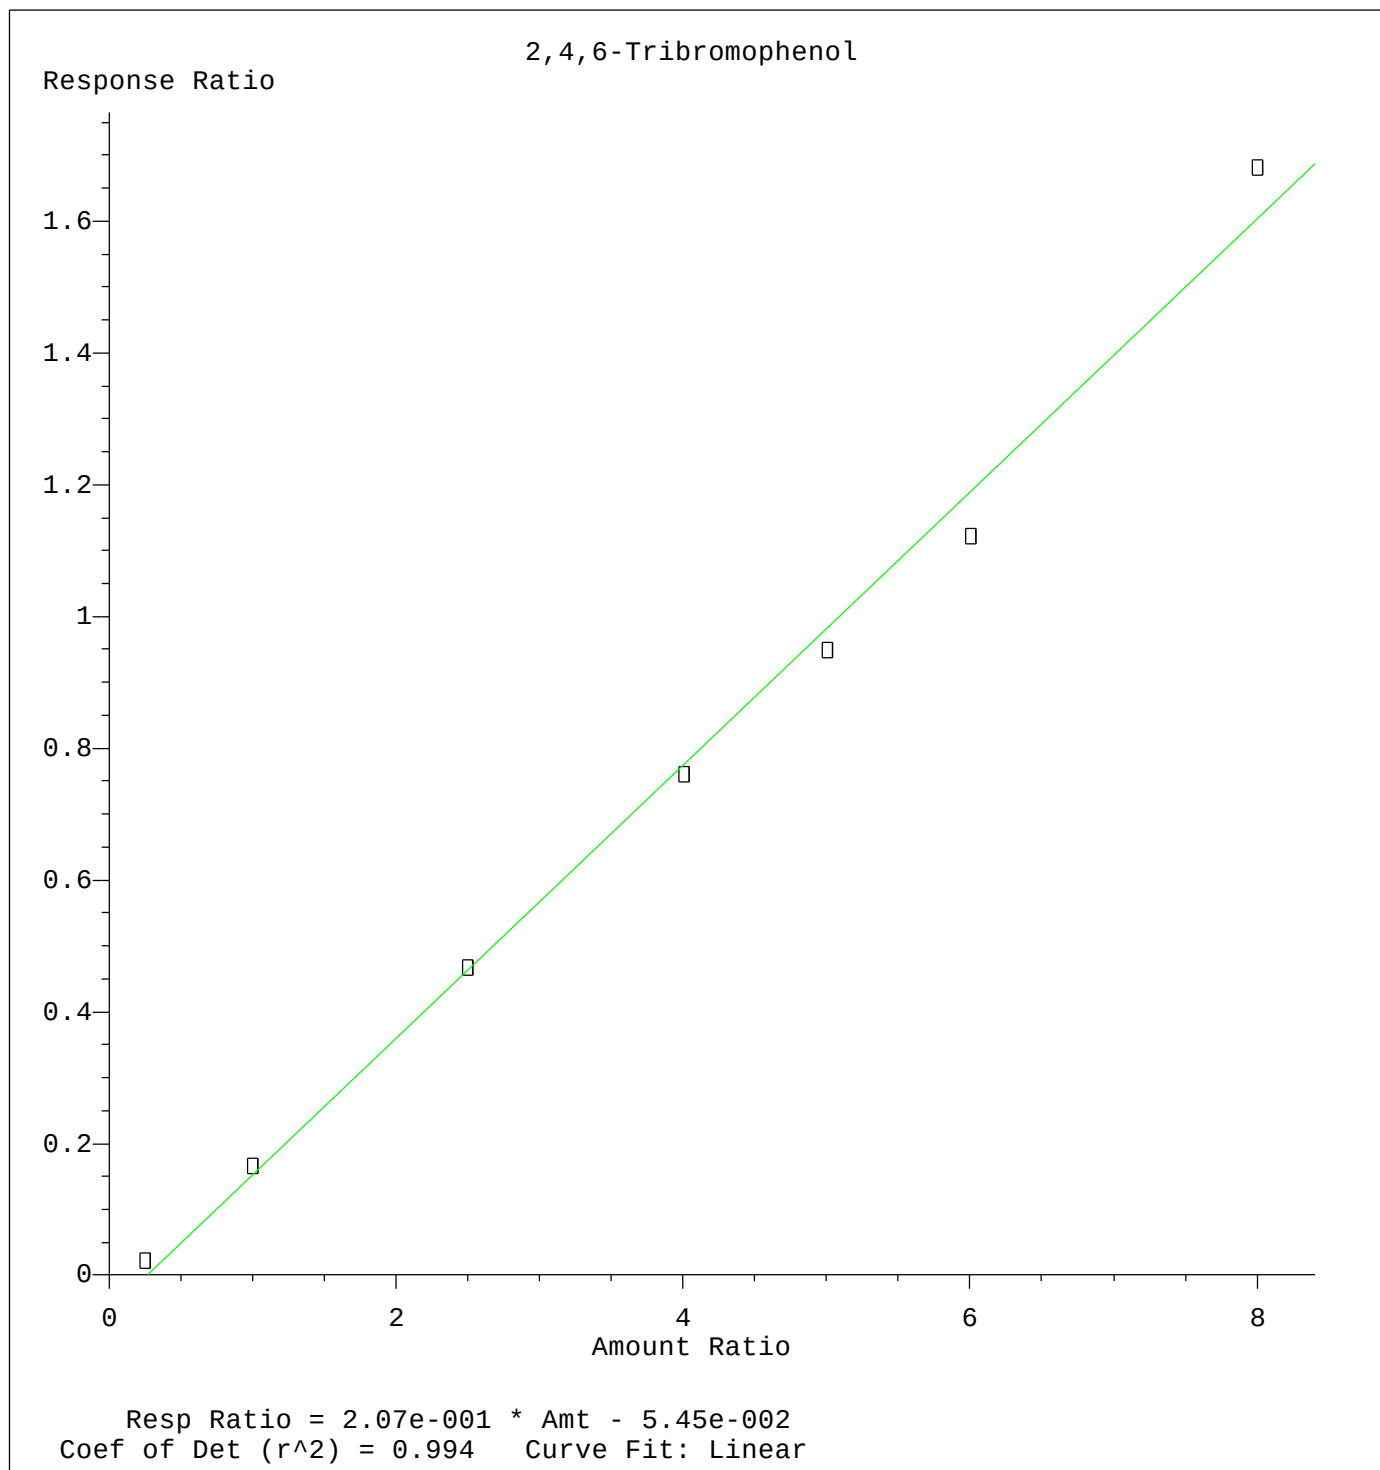

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF042815.M
Calibration Table Last Updated: Wed Apr 29 03:42:05 2015

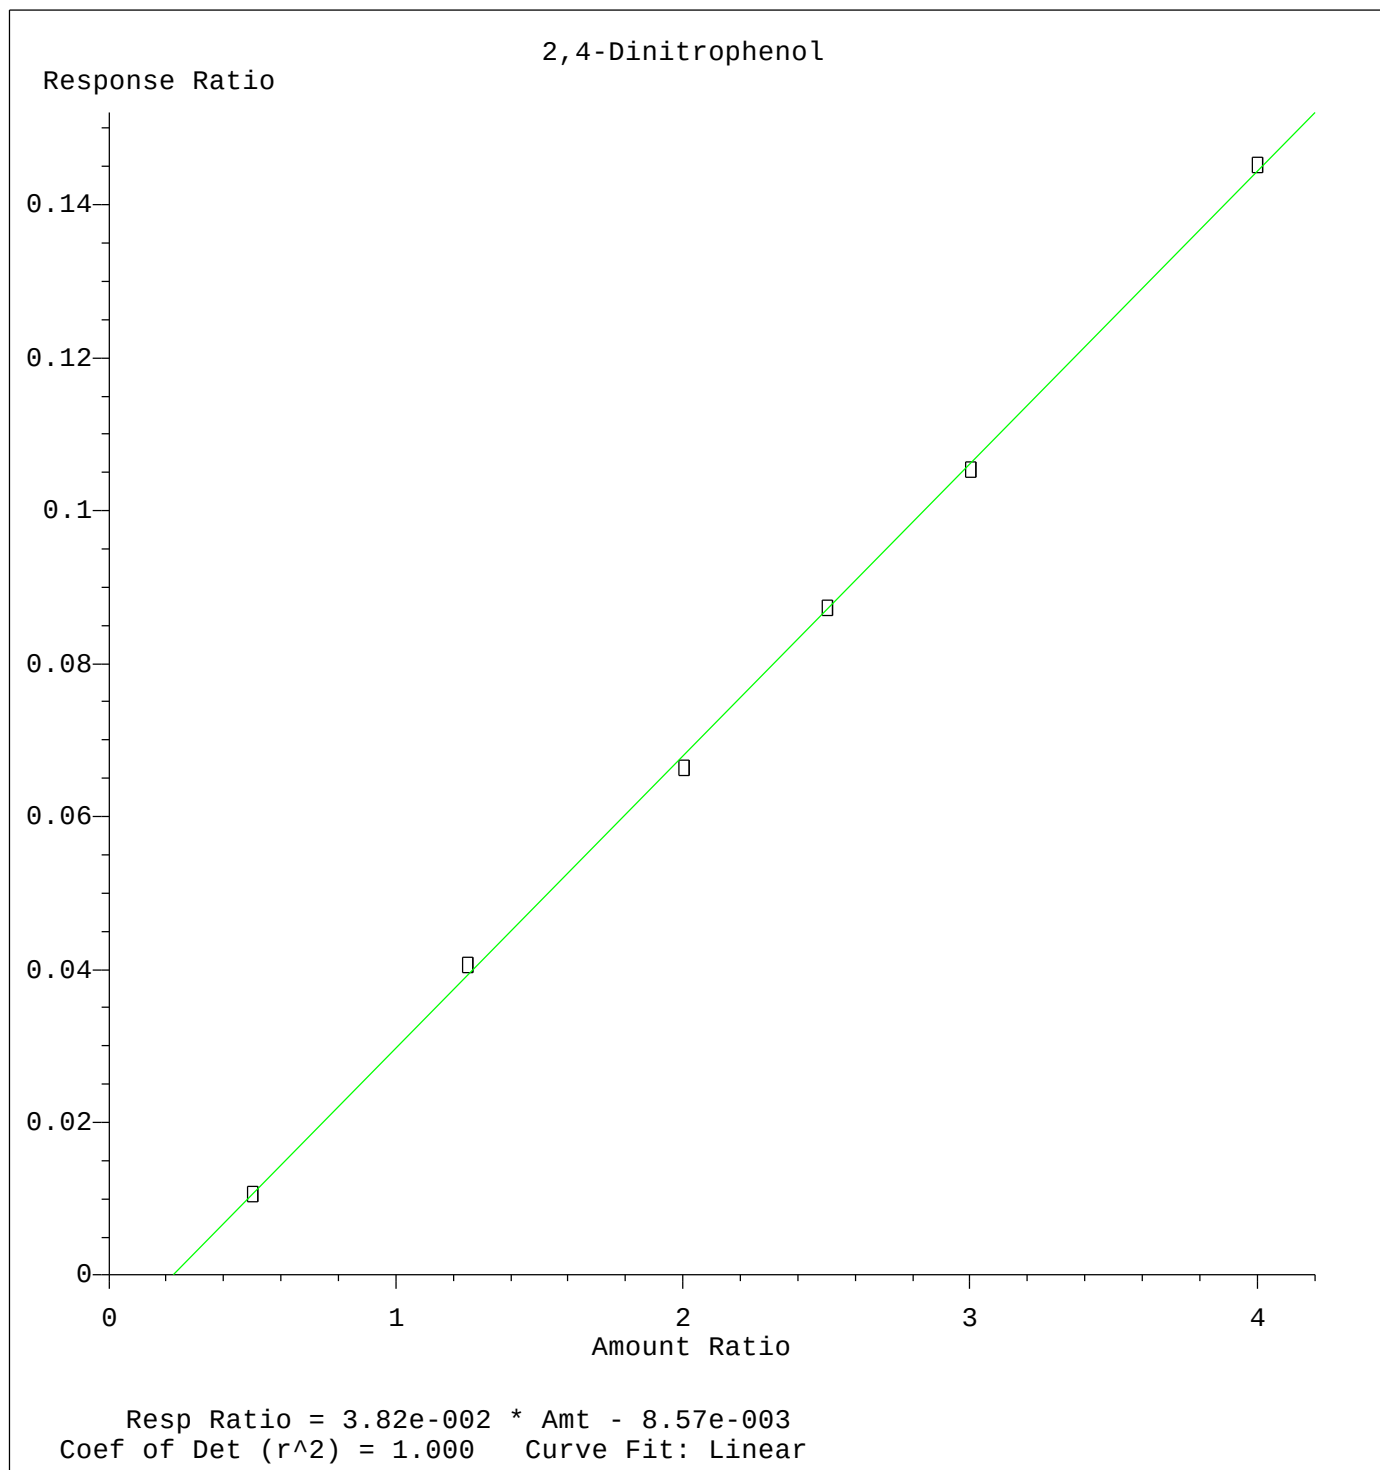


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF042815.M
Calibration Table Last Updated: Wed Apr 29 03:43:59 2015

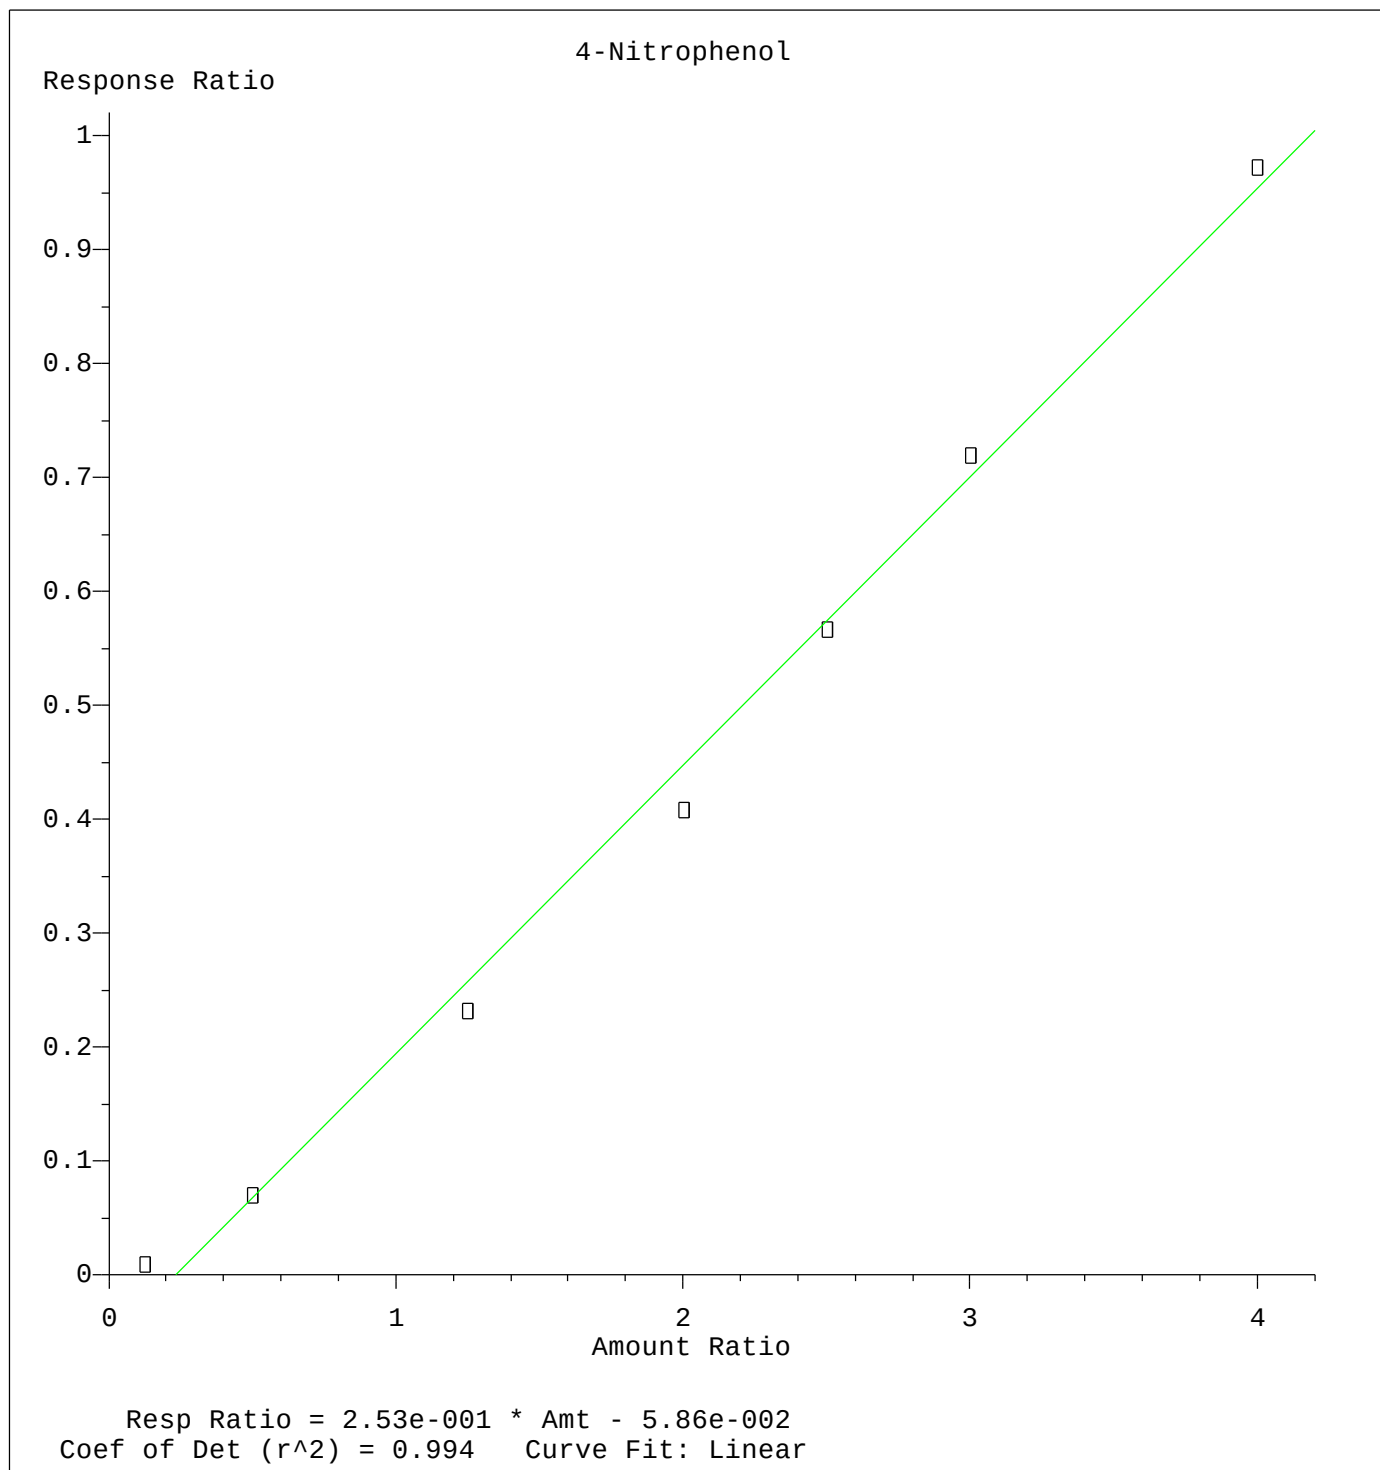

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF042815.M
Calibration Table Last Updated: Wed Apr 29 03:44:14 2015

2,4-Dinitrotoluene

Response Ratio

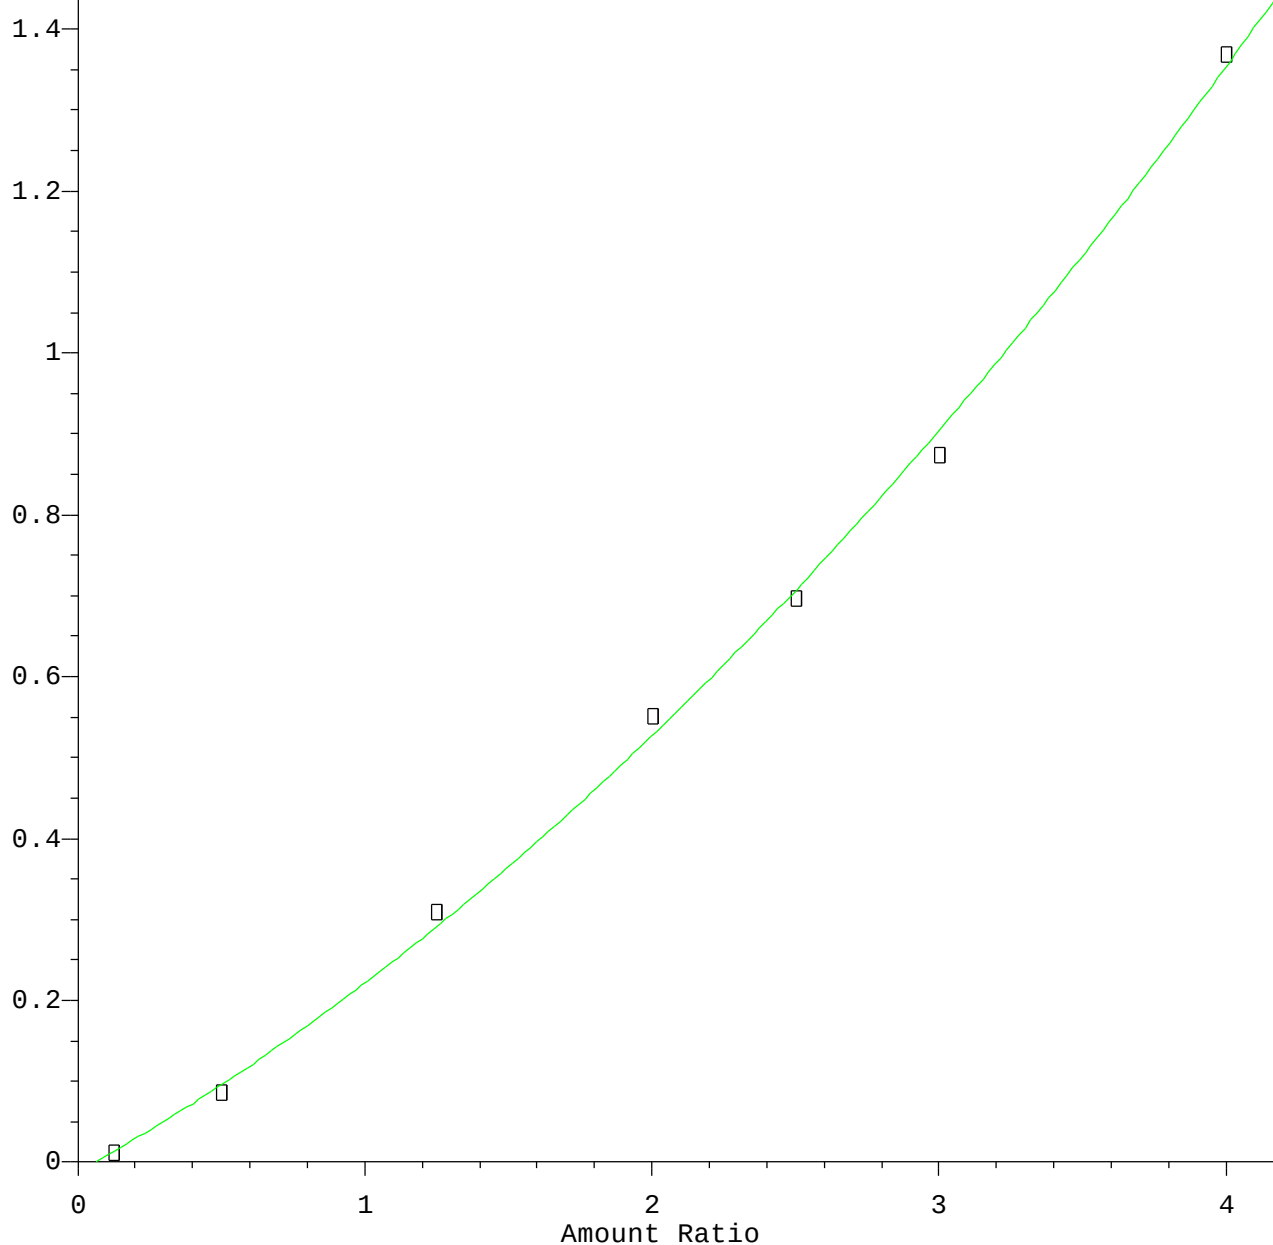


$R = 3.60e-002 A^2 + 1.97e-001 A - 1.21e-002$
Coef of Det (r^2) = 0.998 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF042815.M
Calibration Table Last Updated: Wed Apr 29 03:44:30 2015

4-Nitroaniline

Response Ratio

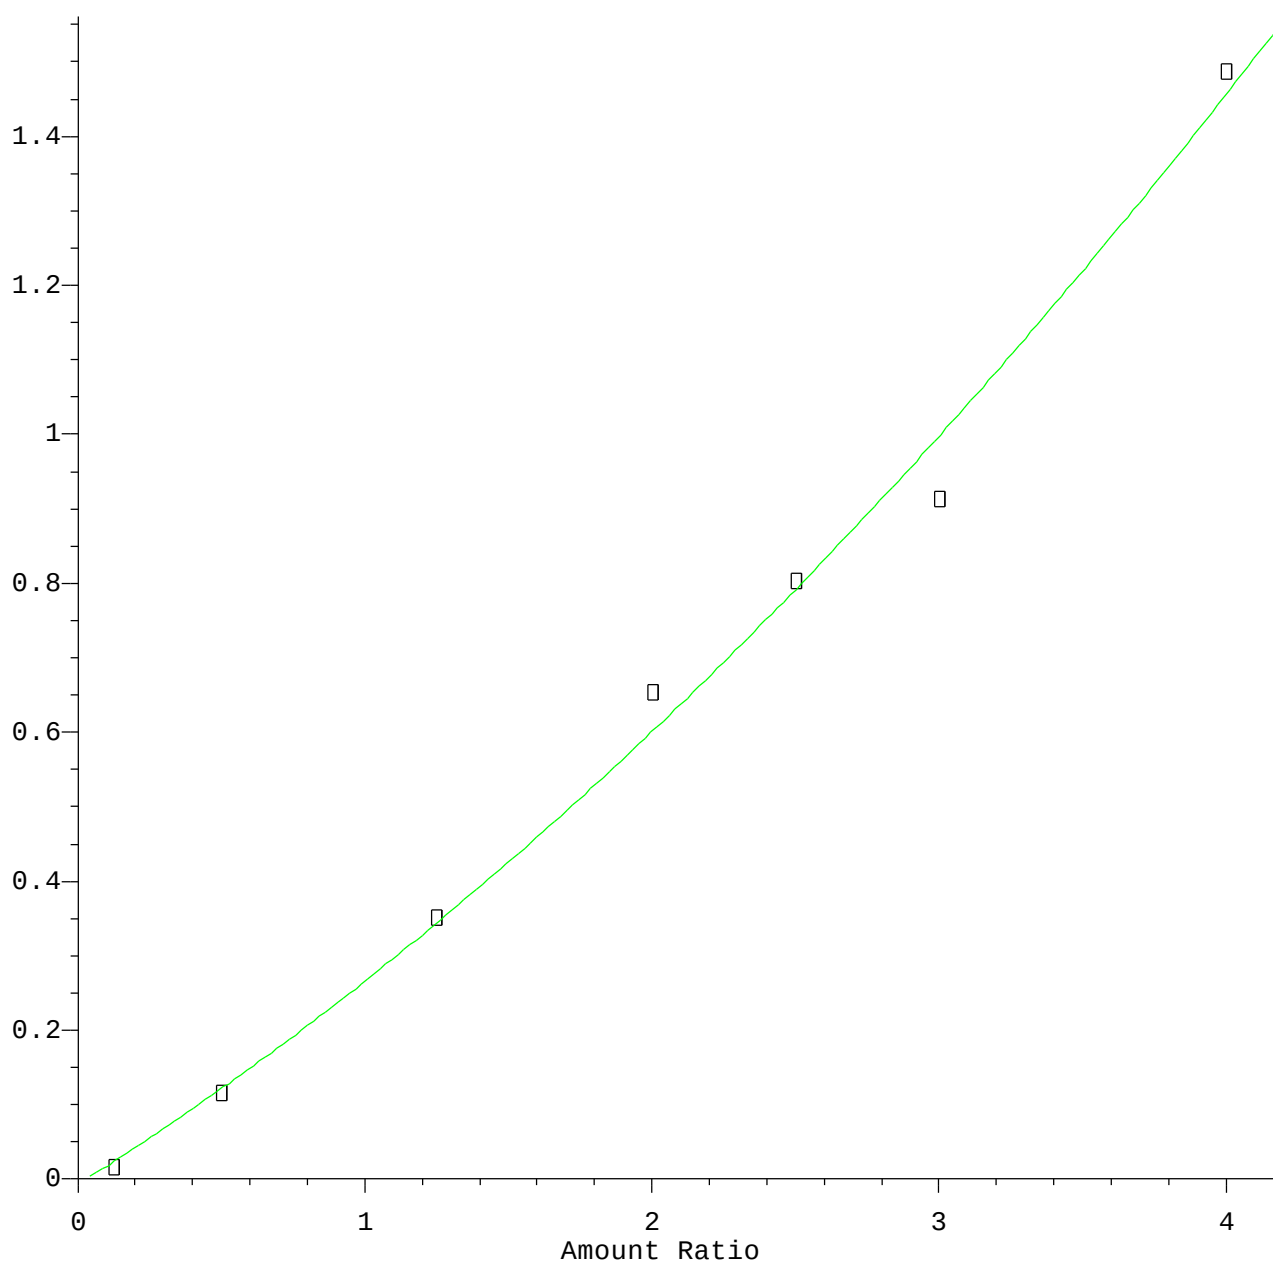


$R = 3.09e-002 A^2 + 2.42e-001 A - 7.29e-003$
Coef of Det (r^2) = 0.993 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF042815.M
Calibration Table Last Updated: Wed Apr 29 03:45:10 2015


4,6-Dinitro-2-methylphenol

Response Ratio

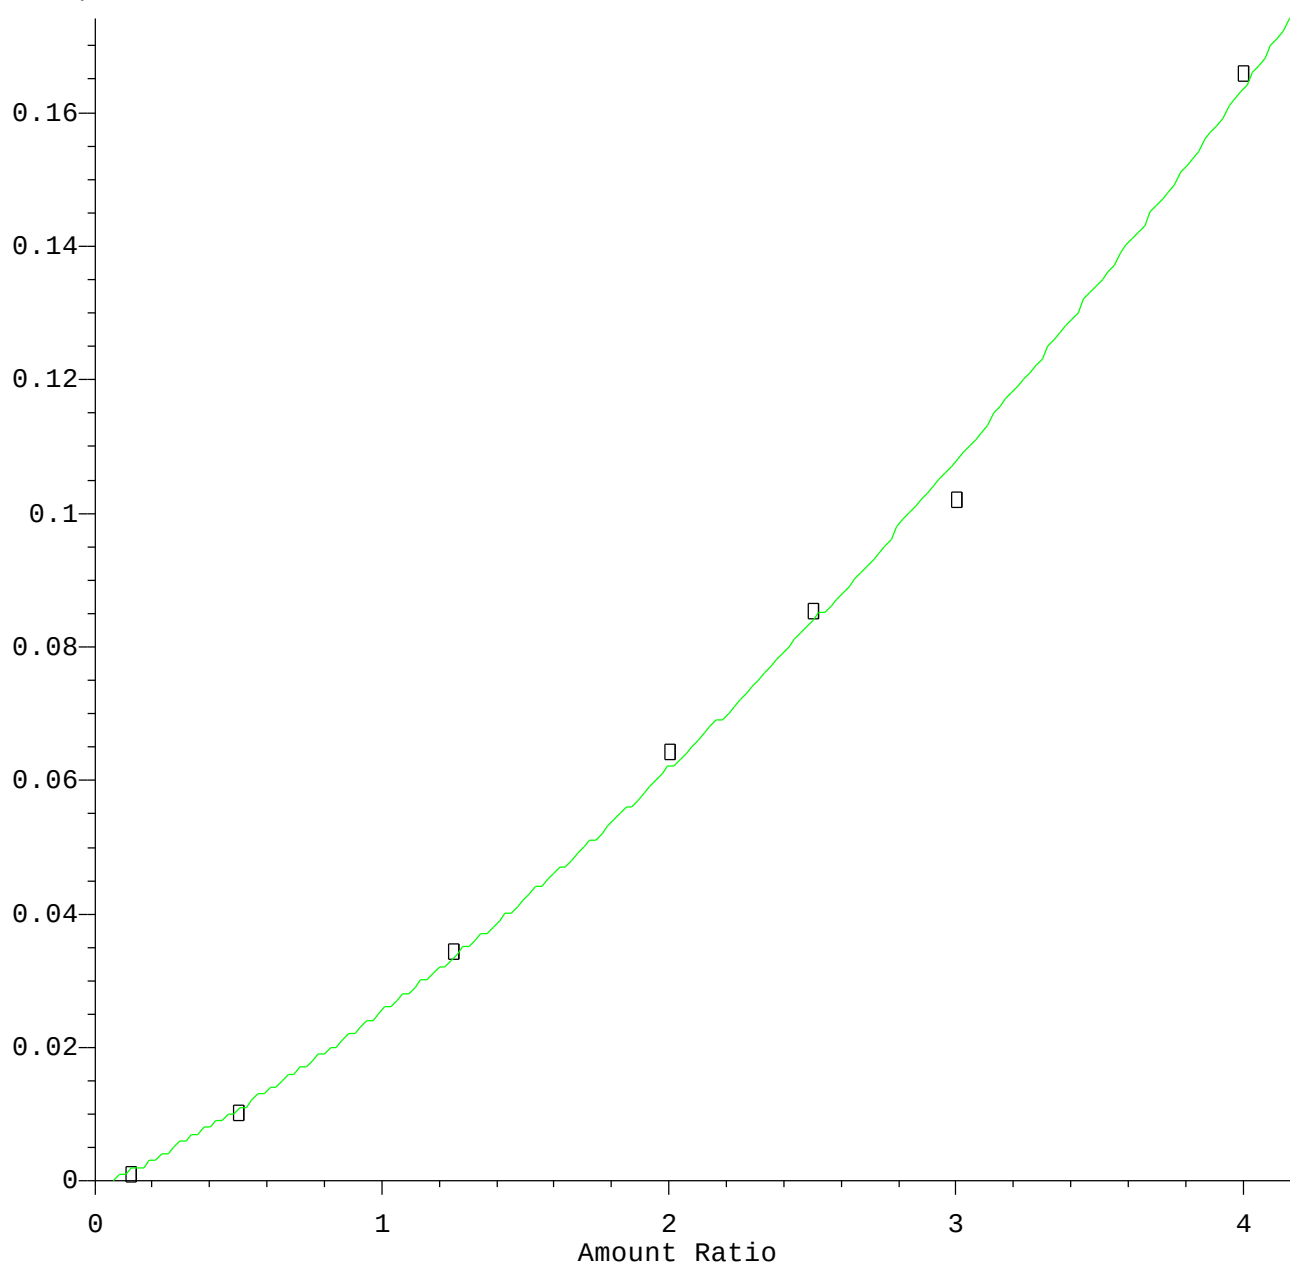


$R = 4.88e-003 A^2 + 2.17e-002 A - 1.31e-003$
Coef of Det (r^2) = 0.998 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF042815.M
Calibration Table Last Updated: Wed Apr 29 03:45:29 2015

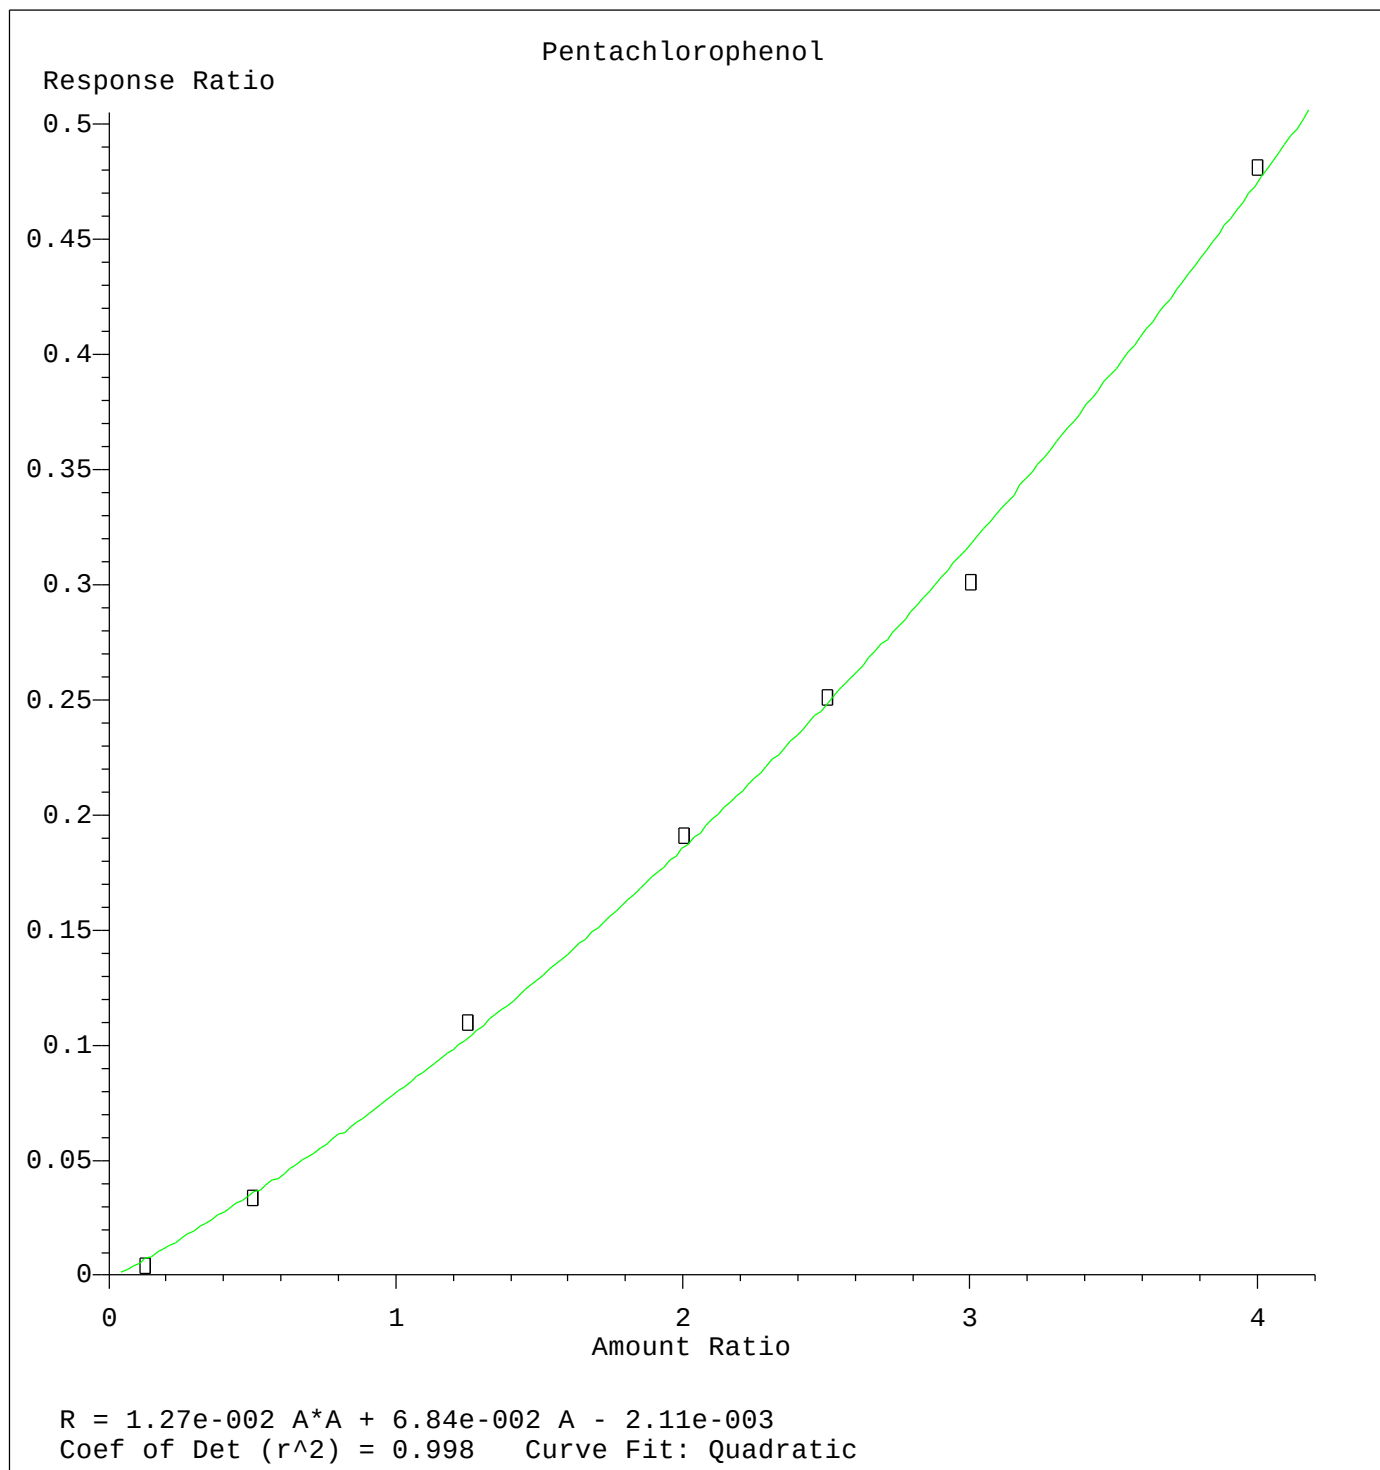

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF042815.M
Calibration Table Last Updated: Wed Apr 29 03:45:48 2015

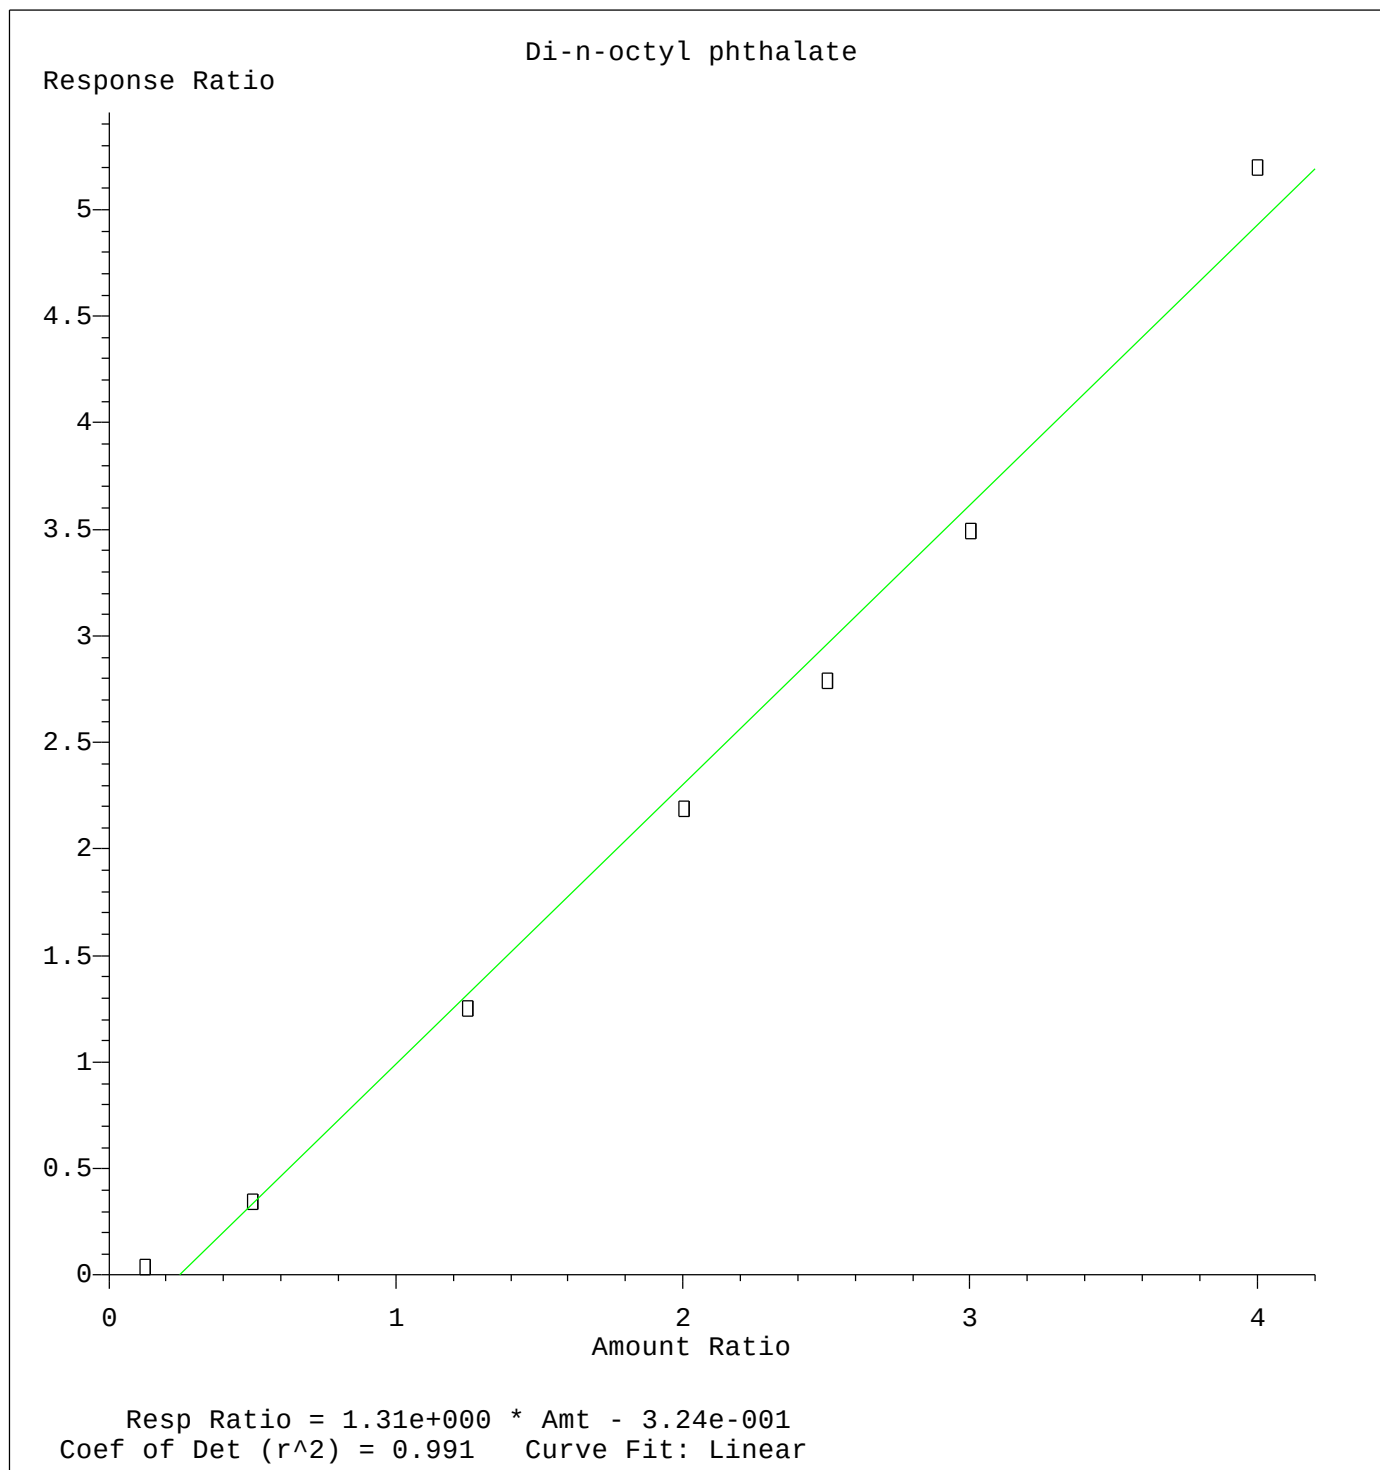

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF042815.M
Calibration Table Last Updated: Wed Apr 29 03:47:37 2015