
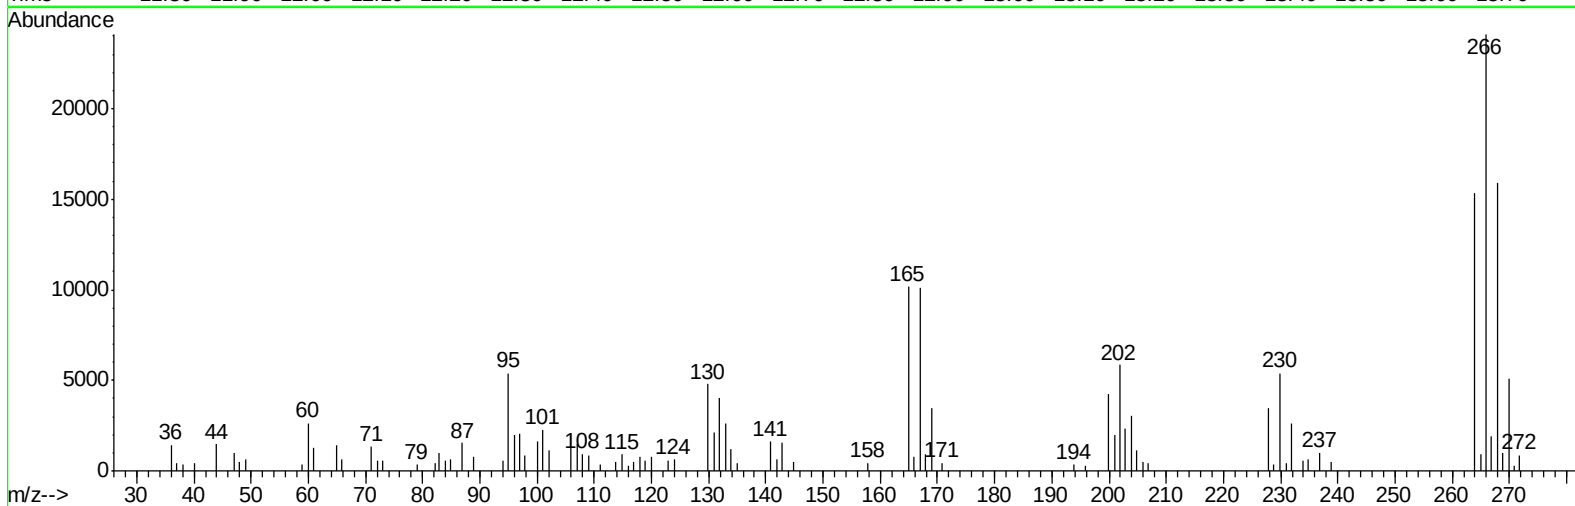


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042815\
Data File : BF078782.D
Acq On : 28 Apr 2015 19:00
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 07:46:51 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 29 03:47:53 2015
Response via : Initial Calibration

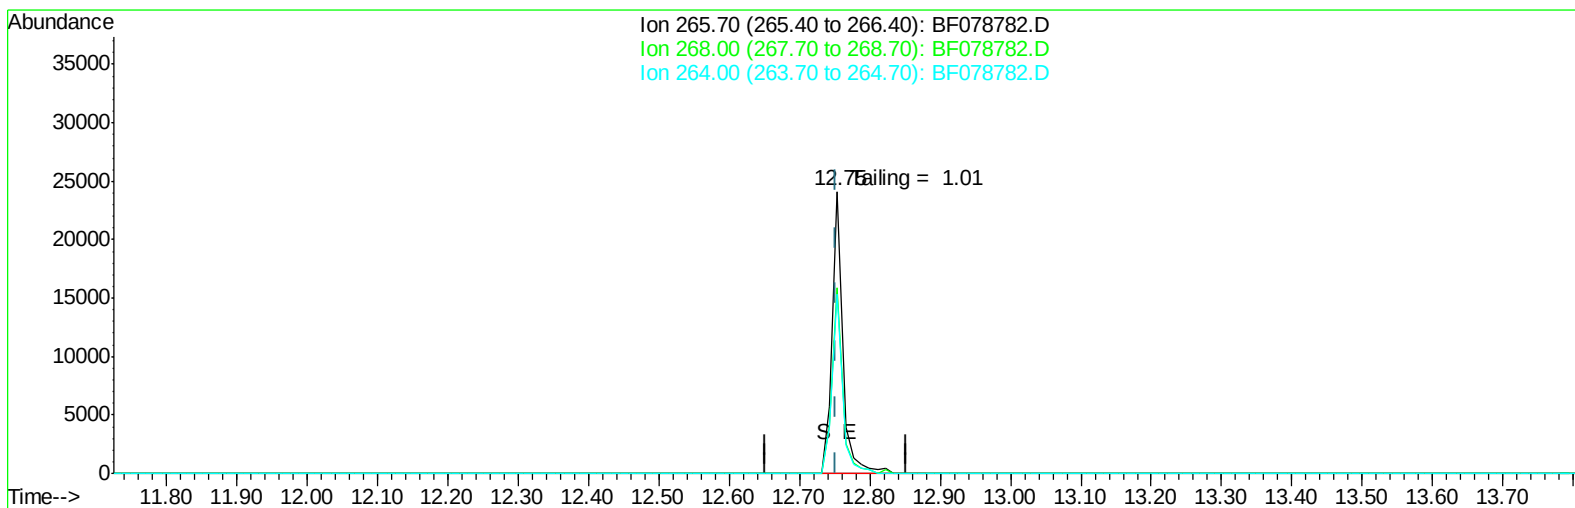

TIC: BF078782.D

(69) Pentachlorophenol (C)



12.754min (+0.001) 0.00ng

response 25202

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	65.92
264.00	60.20	63.54
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042815\
Data File : BF078782.D
Acq On : 28 Apr 2015 19:00
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 07:46:51 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 29 03:47:53 2015
Response via : Initial Calibration

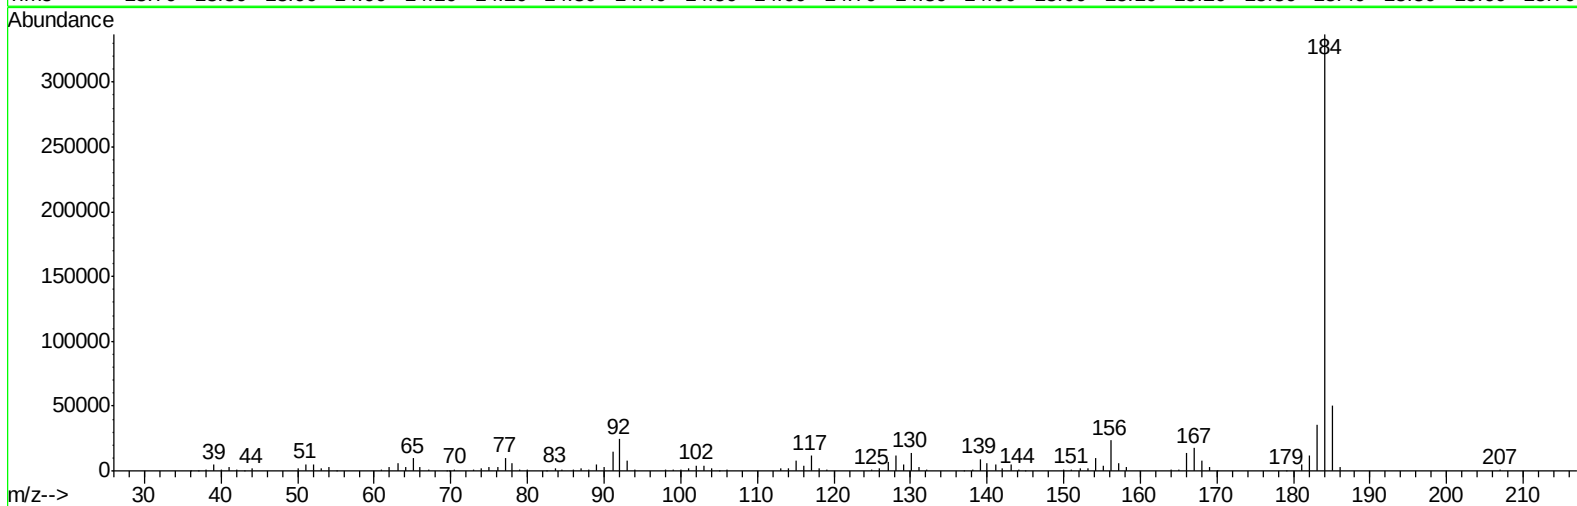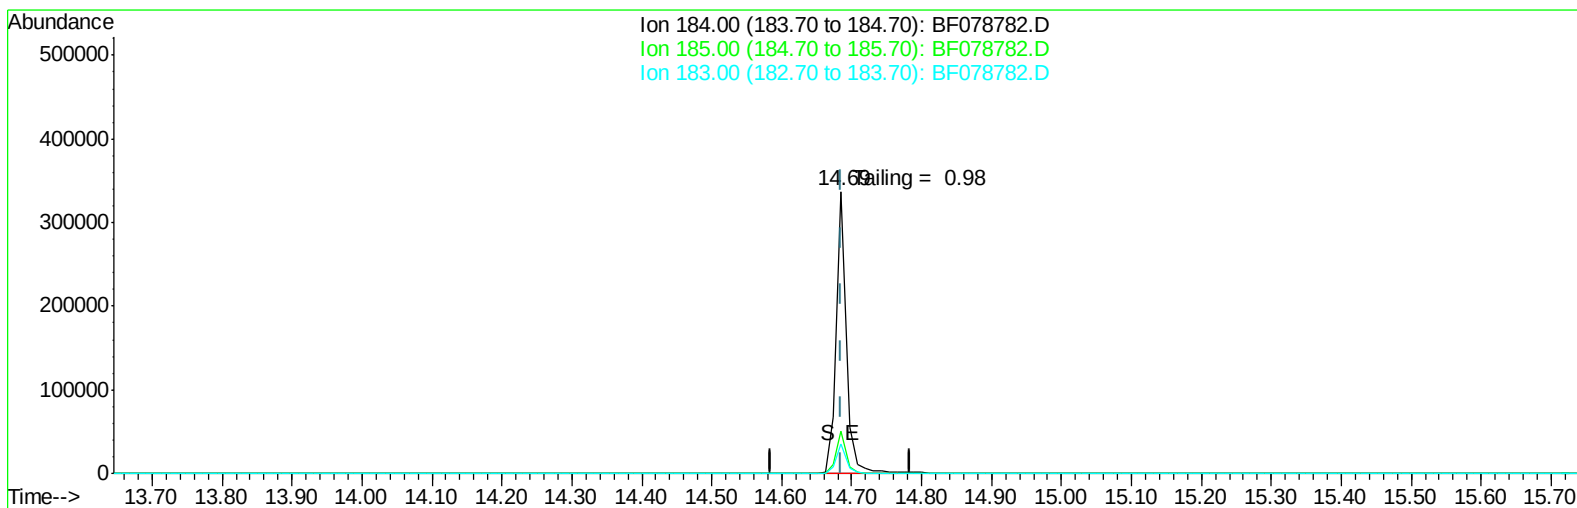

TIC: BF078782.D

(76) Benzidine

14.685min (+0.000) 0.00ng

response 331473

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	15.02
183.00	10.50	10.53
0.00	0.00	0.00