
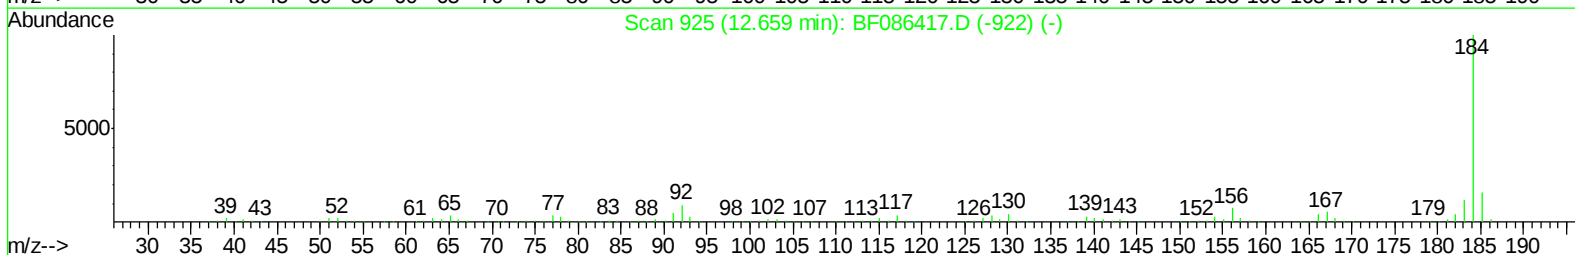
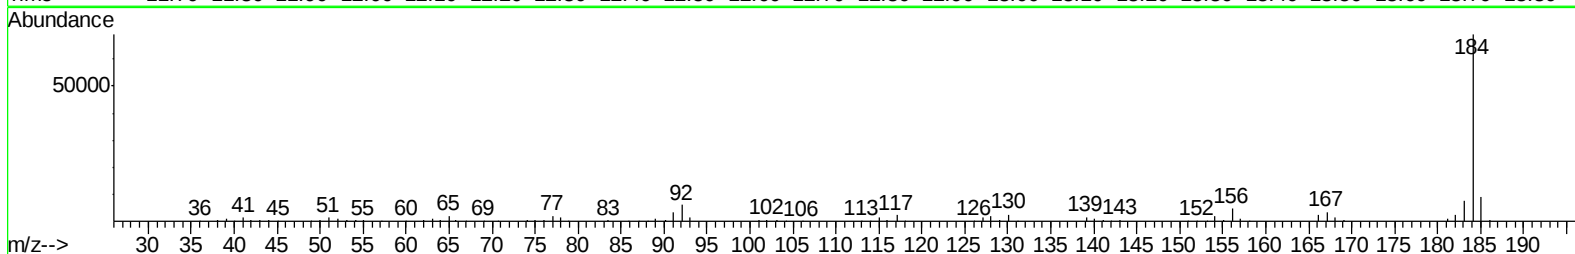


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF042816\  
Data File : BF086469.D  
Acq On : 28 Apr 2016 15:10  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 07:18:39 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF042716.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Apr 27 14:20:52 2016  
Response via : Initial Calibration

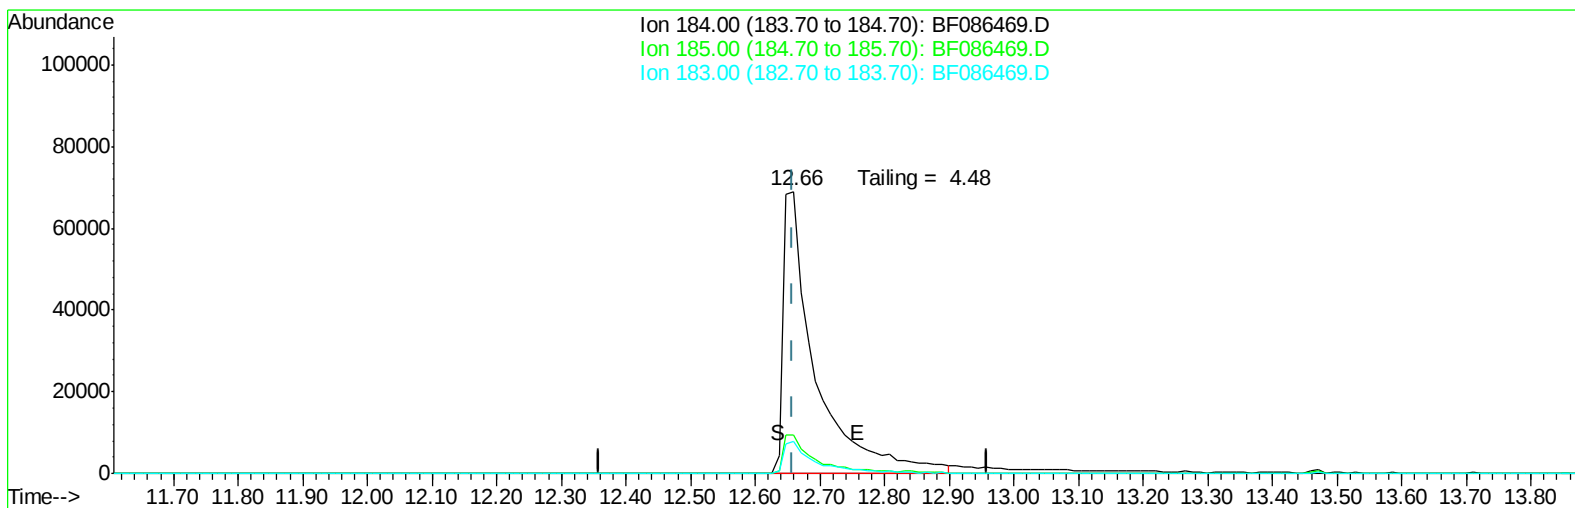

TIC: BF086469.D

(76) Benzidine




12.659min (+0.000) 9881.54ng

response 236352

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 17.00 | 13.50# |
| 183.00 | 12.20 | 11.56  |
| 0.00   | 0.00  | 0.00   |

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF042816\  
Data File : BF086469.D  
Acq On : 28 Apr 2016 15:10  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 07:18:39 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF042716.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Apr 27 14:20:52 2016  
Response via : Initial Calibration

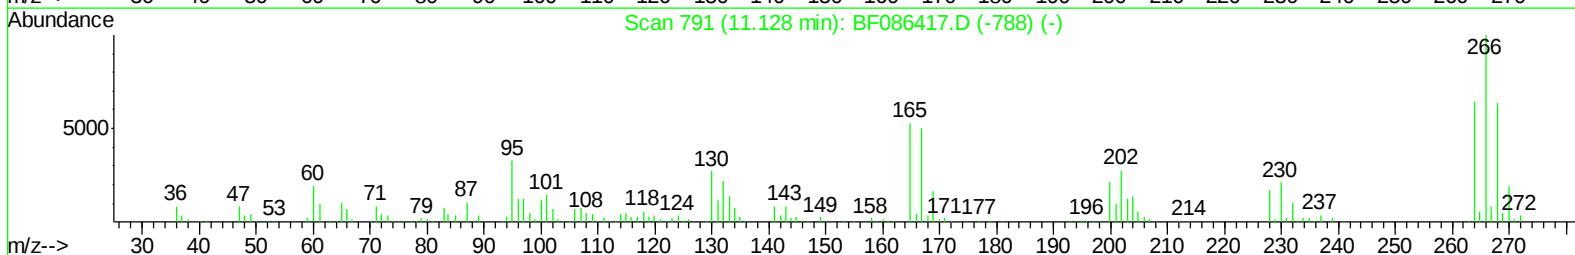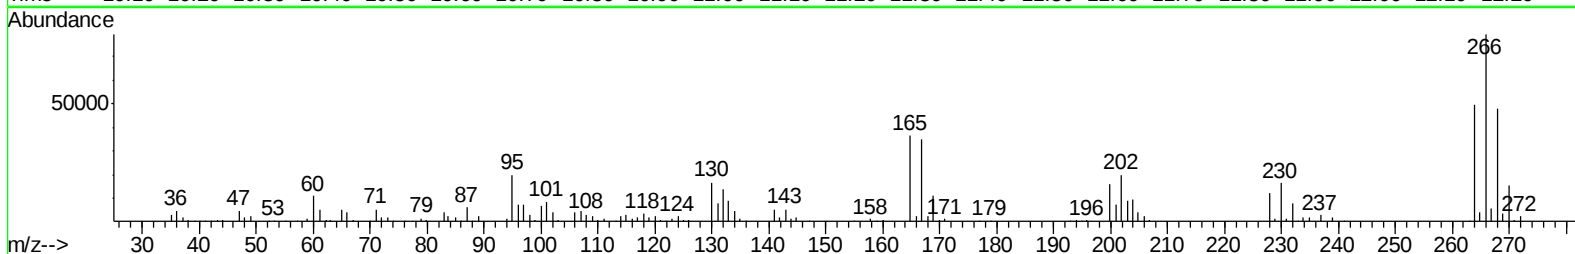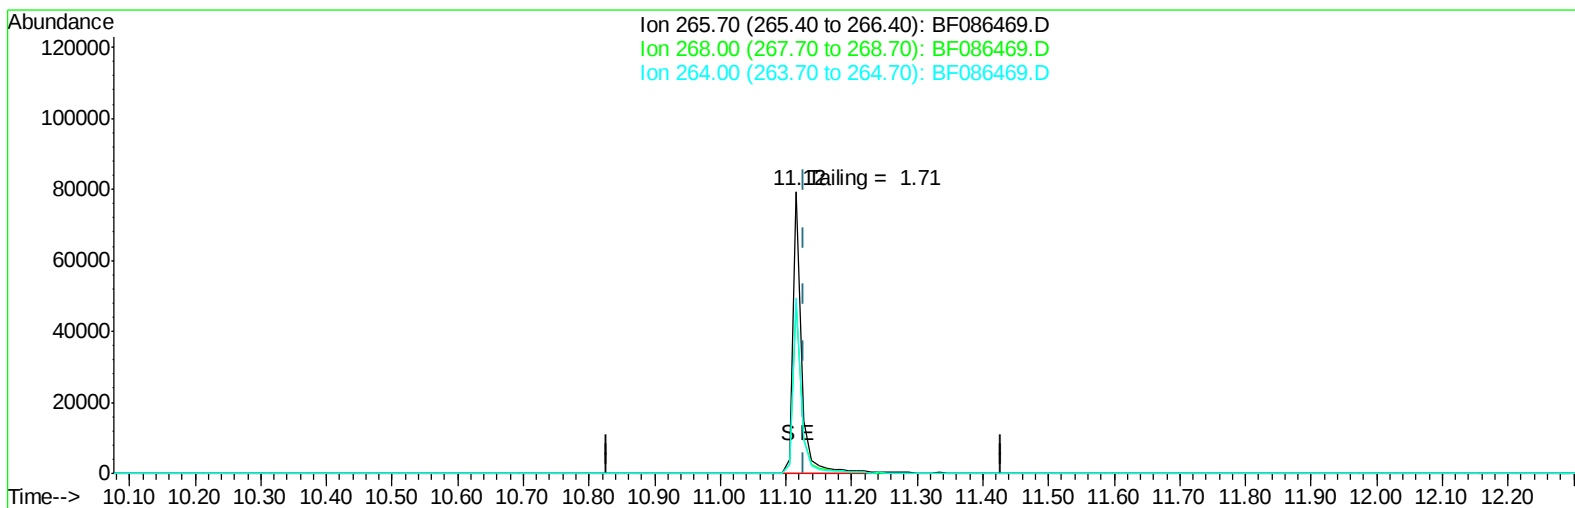

TIC: BF086469.D

(69) Pentachlorophenol (C)

11.116min (-0.011) 10064.87ng

response 76710

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 64.40 | 60.26 |
| 264.00 | 66.10 | 62.36 |
| 0.00   | 0.00  | 0.00  |