


Data Path : Z:\HPCHEM1\BNA F\Data\BF042816\
 Data File : BF086469.D
 Acq On : 28 Apr 2016 15:10
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 27 14:20:52 2016

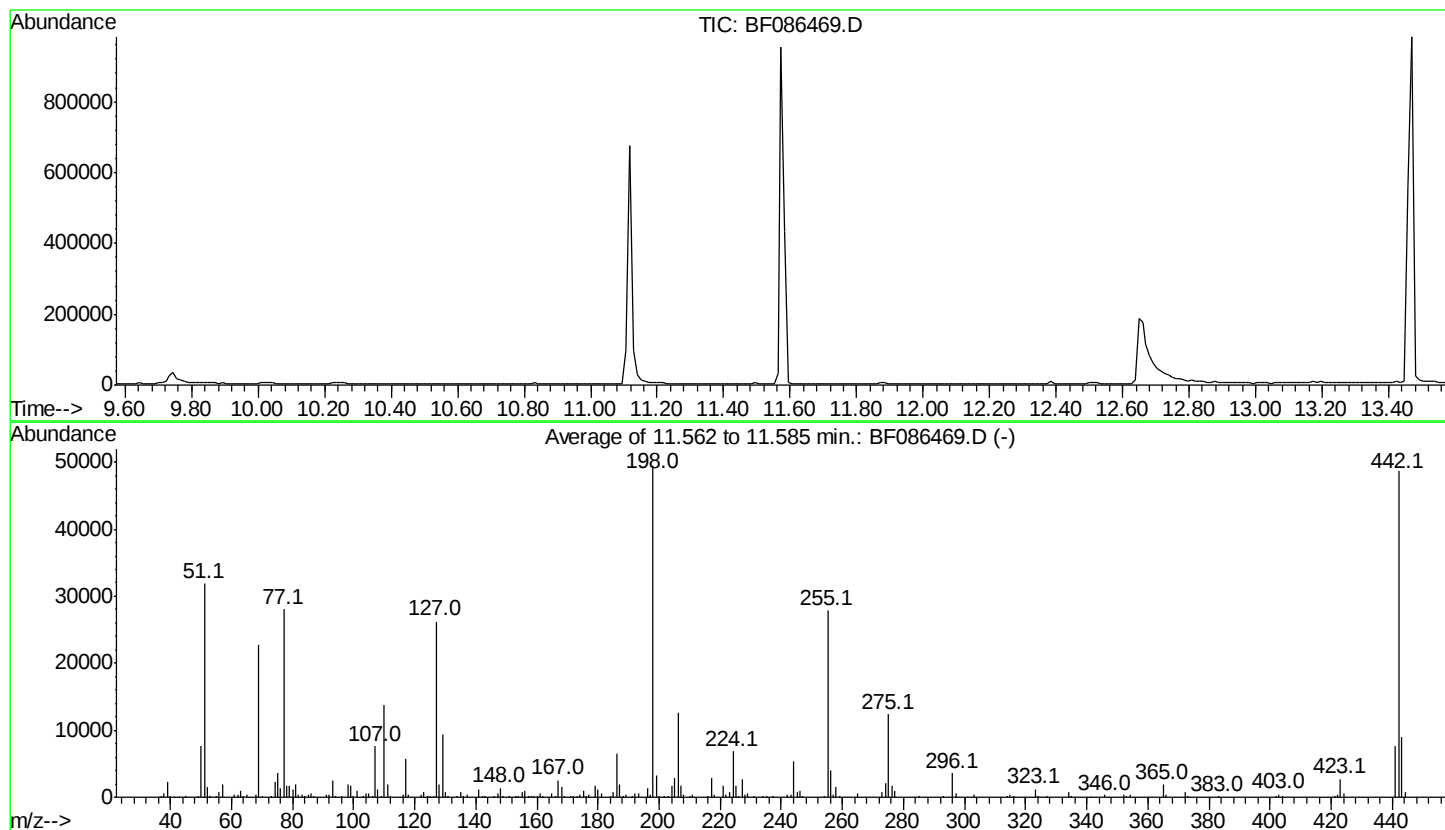

AutoFind: Scans 829, 830, 831; Background Corrected with Scan 826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.5	31889	PASS
68	69	0.00	2	1.7	381	PASS
69	198	0.00	100	45.8	22683	PASS
70	69	0.00	2	0.6	144	PASS
127	198	10	80	53.1	26253	PASS
197	198	0.00	2	0.9	422	PASS
198	198	100	100	100.0	49474	PASS
199	198	5	9	6.7	3307	PASS
275	198	10	60	24.9	12330	PASS
365	198	1	100	3.7	1833	PASS
441	442	0.01	24	15.8	7717	PASS
442	198	50	100	98.6	48757	PASS
443	442	15	24	18.5	9032	PASS